

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037638.D
 Acq On : 28 Sep 2024 03:06
 Operator : SY/MD
 Sample : P4185-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	53	rBV	18098	32068	0.13%	0.054%
2	1.282	68	75	99	rVB2	1571774	1756637	7.15%	2.983%
3	1.548	146	158	178	rVB2	808384	1188141	4.84%	2.018%
4	2.060	307	317	338	rBV3	580889	931857	3.79%	1.583%
5	2.690	503	513	538	rVB	458170	767203	3.12%	1.303%
6	3.105	627	642	672	rVB	5759838	11635925	47.38%	19.762%
7	3.481	757	759	760	rBV	517	263	0.00%	0.000%
8	3.609	797	799	802	rVB3	709	372	0.00%	0.001%
9	3.642	807	809	812	rBV	600	345	0.00%	0.001%
10	3.806	843	860	918	rBV	10630888	24557400	100.00%	41.708%
11	4.243	983	996	1026	rVB	359652	903225	3.68%	1.534%
12	4.506	1063	1078	1098	rVB2	352740	887347	3.61%	1.507%
13	4.950	1200	1216	1239	rBV2	871561	2329242	9.48%	3.956%
14	5.449	1367	1371	1374	rVB4	721	502	0.00%	0.001%
15	5.468	1374	1377	1379	rBV4	1089	541	0.00%	0.001%
16	5.529	1385	1396	1424	rBV	659901	1373146	5.59%	2.332%
17	5.828	1477	1489	1525	rBV	826555	1669646	6.80%	2.836%
18	5.986	1527	1538	1563	rVB	491295	1006081	4.10%	1.709%
19	6.506	1697	1700	1701	rBV3	527	262	0.00%	0.000%
20	6.522	1701	1705	1707	rVB4	1163	756	0.00%	0.001%
21	6.571	1716	1720	1721	rBV2	820	486	0.00%	0.001%
22	6.616	1731	1734	1735	rBV2	533	210	0.00%	0.000%
23	6.667	1745	1750	1752	rBV2	644	644	0.00%	0.001%
24	6.696	1757	1759	1762	rVV2	640	319	0.00%	0.001%
25	6.731	1769	1770	1772	rBV2	359	176	0.00%	0.000%
26	6.764	1777	1780	1782	rBV2	636	340	0.00%	0.001%
27	6.838	1801	1803	1805	rVB2	555	222	0.00%	0.000%
28	6.854	1805	1808	1810	rBV	278	197	0.00%	0.000%
29	6.870	1810	1813	1815	rBV3	475	382	0.00%	0.001%
30	6.908	1815	1825	1859	rBV	234746	466419	1.90%	0.792%
31	7.239	1917	1928	1968	rBV	989673	1769814	7.21%	3.006%
32	7.551	2016	2025	2051	rBV	160458	295446	1.20%	0.502%
33	7.776	2087	2095	2117	rVB3	19894	42078	0.17%	0.071%
34	7.899	2121	2133	2155	rBV	491587	842696	3.43%	1.431%
35	8.027	2164	2173	2216	rBV2	250286	563392	2.29%	0.957%
36	8.519	2325	2326	2329	rBV	571	401	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037638.D
 Acq On : 28 Sep 2024 03:06
 Operator : SY/MD
 Sample : P4185-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.657	2367	2369	2371	rBV3	501	295	0.00%	0.001%
38	8.674	2371	2374	2375	rBV2	548	276	0.00%	0.000%
39	8.780	2396	2407	2431	rBV	1060060	1731679	7.05%	2.941%
40	9.136	2516	2518	2520	rBV2	572	316	0.00%	0.001%
41	9.201	2536	2538	2542	rVB4	796	335	0.00%	0.001%
42	9.259	2554	2556	2557	rBV2	359	157	0.00%	0.000%
43	9.419	2601	2606	2609	rBV4	812	899	0.00%	0.002%
44	9.490	2624	2628	2631	rBV4	949	947	0.00%	0.002%
45	9.545	2640	2645	2647	rBV3	403	316	0.00%	0.001%
46	9.593	2655	2660	2662	rBV3	806	620	0.00%	0.001%
47	9.645	2673	2676	2677	rBV2	348	192	0.00%	0.000%
48	9.677	2684	2686	2689	rVB3	741	337	0.00%	0.001%
49	9.722	2698	2700	2703	rVB3	1011	532	0.00%	0.001%
50	9.809	2725	2727	2728	rBV2	609	278	0.00%	0.000%
51	9.879	2740	2749	2755	rBV9	1869	3033	0.01%	0.005%
52	9.976	2774	2779	2782	rBV5	1129	1108	0.00%	0.002%
53	10.024	2791	2794	2796	rBV3	972	488	0.00%	0.001%
54	10.069	2806	2808	2810	rBV3	506	345	0.00%	0.001%
55	10.091	2814	2815	2816	rBV3	719	259	0.00%	0.000%
56	10.146	2821	2832	2853	rBV	576624	908061	3.70%	1.542%
57	10.394	2905	2909	2913	rBV4	613	565	0.00%	0.001%
58	10.410	2913	2914	2917	rVB2	557	221	0.00%	0.000%
59	10.423	2917	2918	2920	rBV	636	267	0.00%	0.000%
60	10.455	2924	2928	2930	rBV4	634	445	0.00%	0.001%
61	10.477	2930	2935	2937	rBV5	1047	632	0.00%	0.001%
62	10.519	2945	2948	2951	rBV4	465	360	0.00%	0.001%
63	10.564	2960	2962	2964	rVV3	451	230	0.00%	0.000%
64	10.590	2968	2970	2973	rBV	537	294	0.00%	0.000%
65	10.612	2974	2977	2979	rVB3	672	329	0.00%	0.001%
66	10.625	2979	2981	2983	rBV	611	240	0.00%	0.000%
67	10.641	2983	2986	2990	rVB	468	393	0.00%	0.001%
68	10.673	2990	2996	2999	rBV4	647	498	0.00%	0.001%
69	10.690	2999	3001	3004	rVB3	647	301	0.00%	0.001%
70	10.706	3004	3006	3009	rBV2	531	339	0.00%	0.001%
71	10.783	3026	3030	3032	rBV3	1155	774	0.00%	0.001%
72	10.815	3036	3040	3043	rBV3	700	669	0.00%	0.001%
73	10.944	3076	3080	3084	rBV3	874	622	0.00%	0.001%
74	10.976	3087	3090	3094	rBV5	744	549	0.00%	0.001%
75	11.001	3094	3098	3100	rBV4	566	412	0.00%	0.001%
76	11.034	3105	3108	3112	rBV2	578	357	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
 Data File : VV037638.D
 Acq On : 28 Sep 2024 03:06
 Operator : SY/MD
 Sample : P4185-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.062	3112	3117	3121	rBV5	614	680	0.00%	0.001%
78	11.178	3142	3153	3187	rBV	986871	1580407	6.44%	2.684%
79	11.426	3228	3230	3232	rBV2	570	251	0.00%	0.000%
80	11.554	3258	3270	3302	rBV	1010546	1606154	6.54%	2.728%
81	12.233	3479	3481	3482	rBV2	600	250	0.00%	0.000%
82	12.265	3488	3491	3492	rBV3	618	354	0.00%	0.001%
83	12.304	3498	3503	3505	rBV2	474	384	0.00%	0.001%
84	12.333	3510	3512	3516	rVB4	759	550	0.00%	0.001%
85	12.352	3516	3518	3521	rBV3	460	262	0.00%	0.000%
86	12.628	3601	3604	3605	rBV2	644	429	0.00%	0.001%
87	12.670	3613	3617	3620	rVB4	590	428	0.00%	0.001%
88	12.709	3628	3629	3631	rBV	437	204	0.00%	0.000%
89	12.728	3631	3635	3643	rVV6	786	1051	0.00%	0.002%
90	12.821	3662	3664	3666	rBV2	606	246	0.00%	0.000%
91	12.914	3690	3693	3694	rBV	532	370	0.00%	0.001%
92	12.969	3707	3710	3713	rVB3	416	357	0.00%	0.001%
93	12.995	3713	3718	3720	rBV3	736	685	0.00%	0.001%
94	13.040	3728	3732	3734	rBV4	753	646	0.00%	0.001%
95	13.053	3734	3736	3738	rBV	550	245	0.00%	0.000%
96	13.590	3901	3903	3905	rBV	617	357	0.00%	0.001%
97	13.628	3913	3915	3918	rBV2	540	317	0.00%	0.001%
98	13.702	3936	3938	3940	rVB	852	409	0.00%	0.001%
99	13.789	3962	3965	3968	rBV3	779	583	0.00%	0.001%
100	14.120	4062	4068	4070	rBV4	774	873	0.00%	0.001%

Sum of corrected areas: 58879643




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037638.D
Acq On : 28 Sep 2024 03:06
Operator : SY/MD
Sample : P4185-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

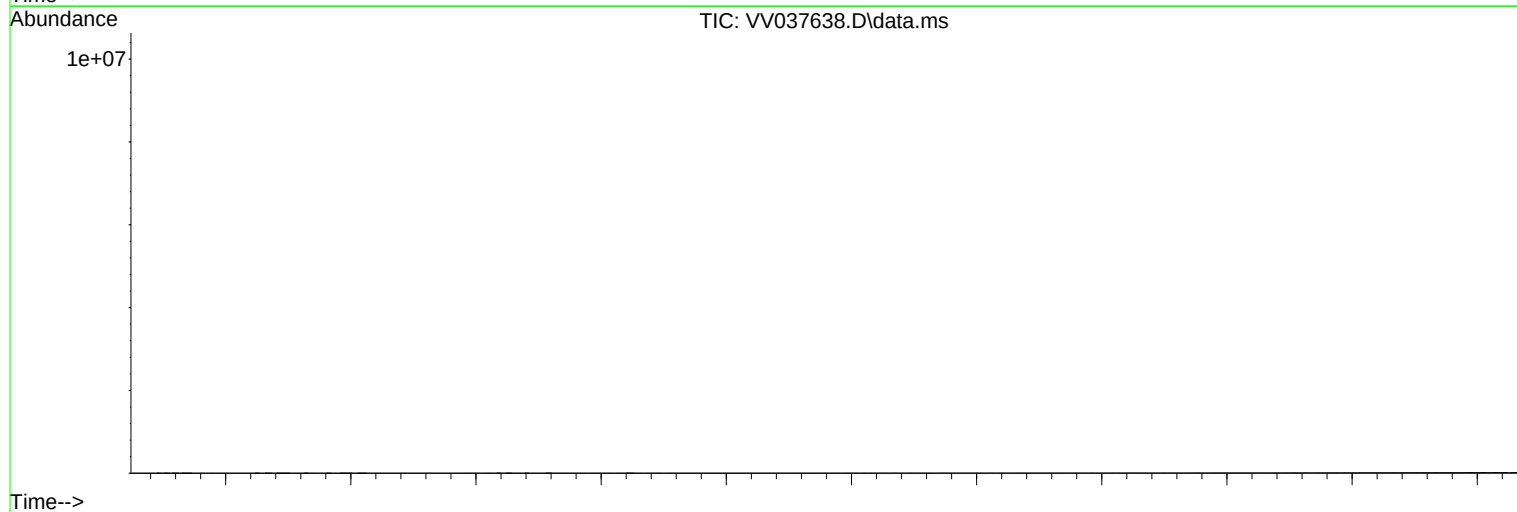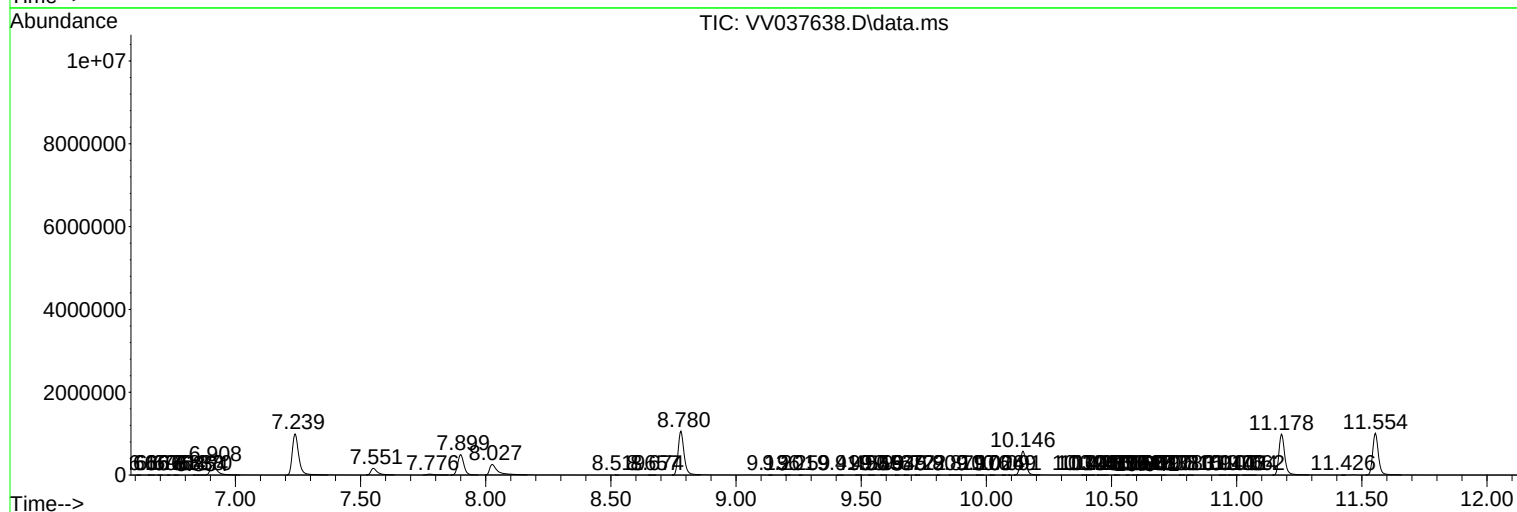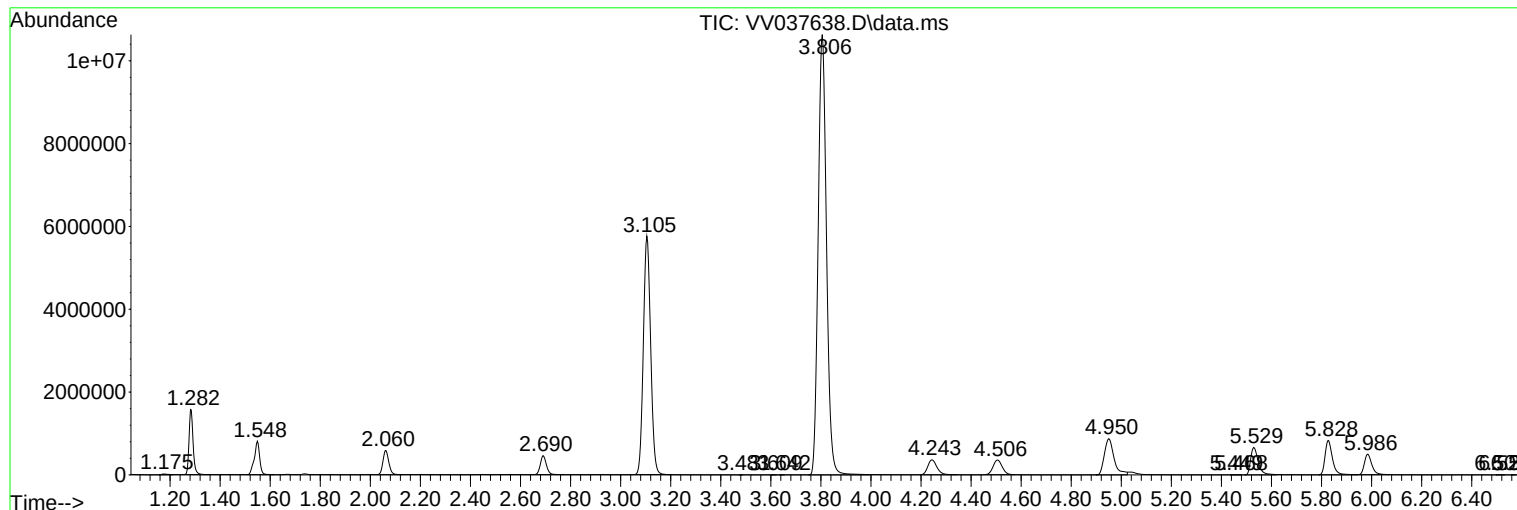

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037638.D
Acq On : 28 Sep 2024 03:06
Operator : SY/MD
Sample : P4185-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037638.D
Acq On : 28 Sep 2024 03:06
Operator : SY/MD
Sample : P4185-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------