
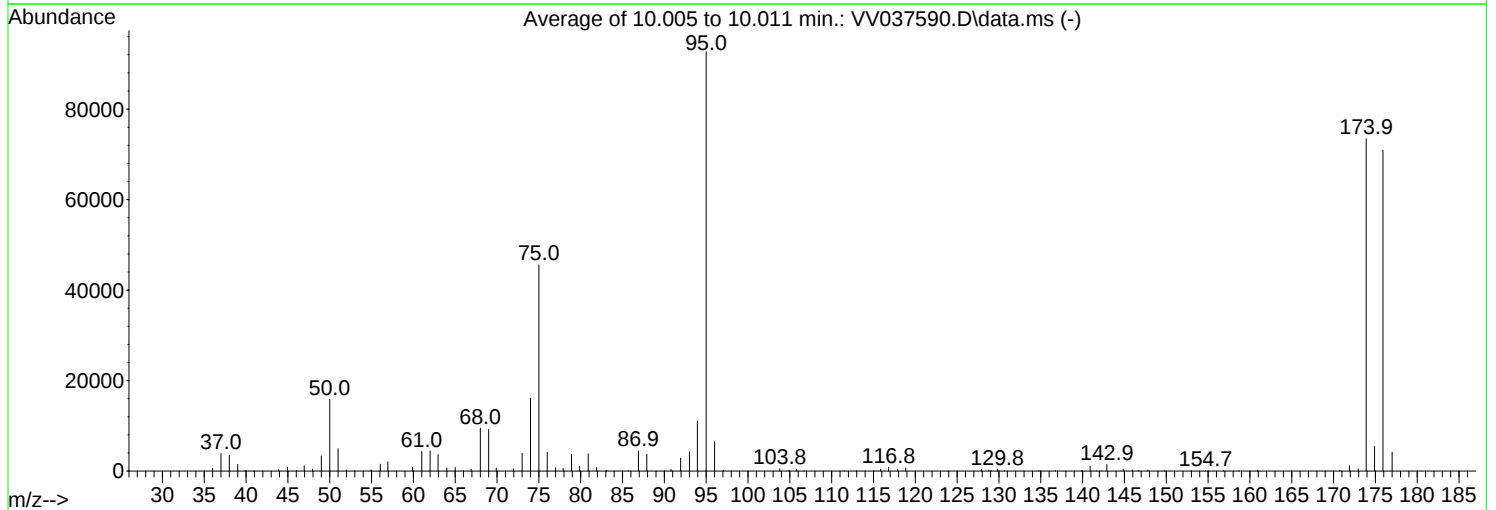


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092724\
Data File : VV037590.D
Acq On : 27 Sep 2024 08:24
Operator : SY/MD
Sample : BFB382
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB382

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Sat Sep 28 00:49:19 2024

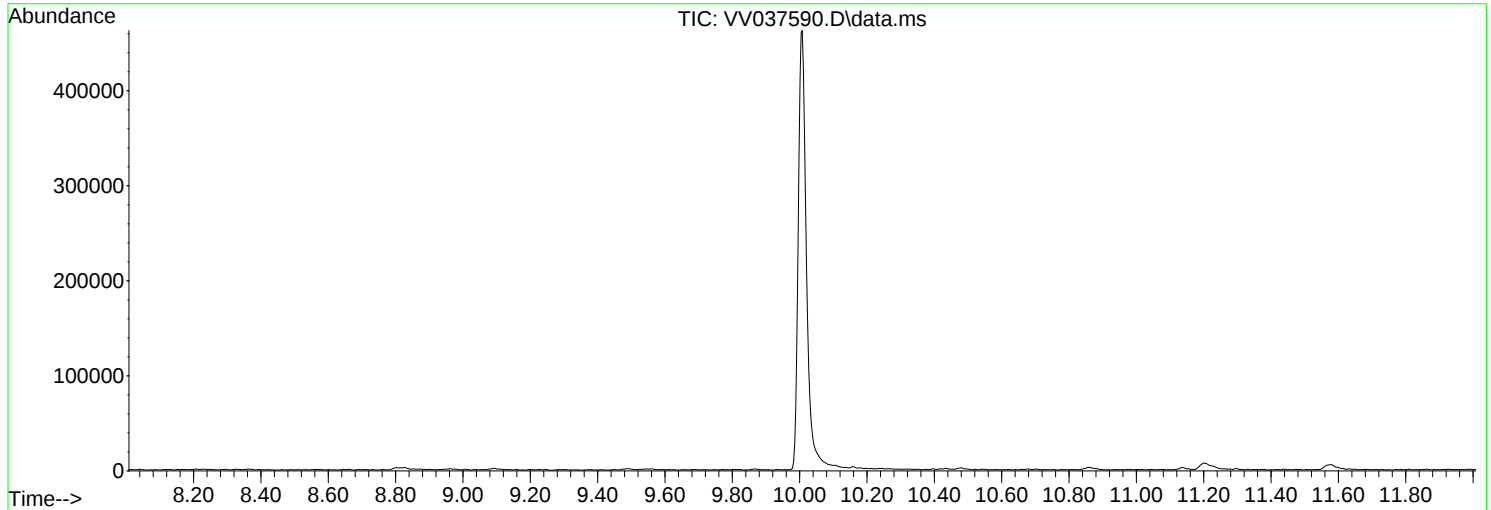

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	15853	PASS
75	95	30	80	49.2	45605	PASS
95	95	100	100	100.0	92688	PASS
96	95	5	9	7.0	6474	PASS
173	174	0.00	2	0.6	472	PASS
174	95	50	120	79.2	73451	PASS
175	174	5	9	7.4	5457	PASS
176	174	95	105	96.6	70944	PASS
177	176	5	10	5.9	4193	PASS

m/z	Abundance
36.10	136.0
39.90	268.0
43.90	680.0
60.70	108.0
76.60	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382

m/z	Abundance
36.00	801.0
37.00	3960.0
38.00	3665.0
39.00	1504.0
40.00	413.0
43.90	1039.0
44.90	806.0
46.00	142.0
47.00	1072.0
48.00	493.0
49.00	3594.0
50.00	16728.0
51.00	5517.0
51.90	231.0
55.00	335.0
56.00	1567.0
57.00	2093.0
57.80	109.0
59.90	906.0
61.00	4625.0
62.00	4551.0
63.00	3692.0
64.00	659.0
65.00	738.0
66.90	414.0
68.00	9747.0
69.00	9418.0
69.90	722.0
71.90	566.0
73.00	4338.0
74.00	16544.0
75.00	47944.0
76.00	4356.0
77.00	748.0
77.90	543.0
78.90	3804.0
79.80	1153.0
80.90	3802.0
81.90	812.0
83.10	178.0
85.70	154.0
86.90	4432.0
87.90	3802.0
90.70	460.0
91.90	3003.0
93.00	4250.0
93.90	11326.0
95.00	95104.0
96.00	6668.0
97.00	139.0
103.80	508.0
104.90	161.0
105.80	488.0
106.70	141.0
111.50	124.0
113.00	121.0
115.10	102.0
115.80	378.0
116.80	932.0
117.90	376.0
118.80	741.0
123.80	107.0
127.90	324.0
128.80	191.0
129.80	408.0
130.60	164.0
136.80	172.0
139.90	116.0
140.90	935.0
141.70	127.0
142.20	117.0
142.90	1603.0
144.80	370.0
146.00	196.0
146.70	123.0
147.80	242.0
149.80	144.0
153.00	125.0
154.70	148.0
155.00	139.0
156.90	184.0
160.90	213.0
170.80	151.0
171.90	1126.0
173.90	74536.0
174.90	5318.0
175.90	71568.0
177.00	4268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382

m/z	Abundance
36.00	720.0
37.00	4027.0
38.00	3641.0
39.00	1526.0
40.00	455.0
43.90	966.0
44.90	853.0
46.10	179.0
46.90	1227.0
48.00	466.0
49.00	3486.0
50.00	16238.0
51.00	5014.0
52.00	241.0
54.90	276.0
56.10	1585.0
57.00	2040.0
59.90	856.0
61.00	4397.0
62.00	4587.0
62.90	3766.0
64.00	698.0
65.00	766.0
66.00	138.0
66.90	405.0
68.00	9832.0
69.00	9384.0
69.90	706.0
71.90	509.0
73.00	3977.0
74.00	16544.0
75.00	46928.0
76.00	4285.0
77.00	813.0
77.90	608.0
78.90	3825.0
79.90	1116.0
80.90	3984.0
81.90	788.0
83.10	164.0
86.90	4695.0
87.90	3817.0
90.80	376.0
91.90	2954.0
93.00	4464.0
94.00	11422.0
95.00	95416.0
96.00	6748.0
97.10	204.0
103.80	501.0
104.90	204.0
105.80	422.0
106.70	115.0
112.90	123.0
115.90	352.0
116.80	878.0
117.90	370.0
118.90	717.0
127.90	390.0
128.80	180.0
129.80	415.0
130.70	149.0
134.70	103.0
135.00	109.0
136.70	133.0
139.90	153.0
140.90	1036.0
142.90	1475.0
144.90	438.0
146.00	265.0
146.70	134.0
147.80	229.0
149.80	136.0
153.00	124.0
154.70	186.0
156.80	177.0
158.70	135.0
160.90	178.0
170.70	131.0
171.90	1232.0
173.00	768.0
173.90	75864.0
174.90	5644.0
175.90	73360.0
177.00	4381.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382

m/z	Abundance
36.00	638.0
37.00	3661.0
38.00	3199.0
39.00	1427.0
39.90	434.0
40.90	109.0
44.00	882.0
45.00	858.0
46.10	162.0
46.90	1202.0
47.90	392.0
49.00	3056.0
50.00	14594.0
51.00	4335.0
52.10	254.0
53.00	109.0
54.90	220.0
56.00	1392.0
56.90	1981.0
59.90	766.0
61.00	3887.0
62.00	4283.0
62.90	3504.0
64.00	667.0
65.00	836.0
66.00	178.0
66.90	337.0
68.00	8904.0
69.00	8813.0
69.90	621.0
72.00	410.0
73.00	3429.0
74.00	15252.0
75.00	41944.0
76.00	3816.0
77.00	715.0
77.90	539.0
78.90	3469.0
79.90	1005.0
80.90	3715.0
81.90	770.0
83.10	132.0
86.90	4273.0
87.90	3529.0
90.90	290.0
92.00	2626.0
93.00	4135.0
94.00	10410.0
95.00	87544.0
96.00	6006.0
97.10	229.0
103.80	452.0
104.90	202.0
105.80	363.0
115.90	329.0
116.80	707.0
117.90	340.0
118.90	612.0
127.90	467.0
128.80	159.0
129.10	160.0
129.80	389.0
134.80	149.0
139.90	134.0
140.90	1098.0
142.90	1271.0
144.90	438.0
145.90	239.0
146.70	118.0
147.80	186.0
154.70	184.0
156.80	132.0
158.70	153.0
160.90	126.0
170.70	138.0
171.90	1195.0
172.90	647.0
173.90	69952.0
174.90	5409.0
175.90	67904.0
177.00	3930.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382