

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007950.D
 Acq On : 28 Sep 2018 13:33
 Operator : SY/MD
 Sample : J5063-16
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC37

Quant Time: Oct 01 02:32:10 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 01:51:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91897	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	87718	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43874	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18831	3.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.40%
7) Chloroethane-d5	1.59	69	18519	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.00%
11) 1,1-Dichloroethene-d2	2.14	63	32847	2.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.00%#
20) 2-Butanone-d5	3.96	46	64653	43.63	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.26%
24) Chloroform-d	4.41	84	48016	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
26) 1,2-Dichloroethane-d4	5.09	65	26232	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.00%
32) Benzene-d6	5.10	84	92189	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
36) 1,2-Dichloropropane-d6	6.12	67	29769	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.36	98	85978	4.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.60%
43) trans-1,3-Dichloropropene-	7.67	79	9829	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	8.14	63	47983	42.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.06%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22910	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	36836	4.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.80%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	255334	27.459 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007950.D
Acq On : 28 Sep 2018 13:33
Operator : SY/MD
Sample : J5063-16
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC37

Quant Time: Oct 01 02:32:10 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 01:51:53 2018
Response via : Initial Calibration

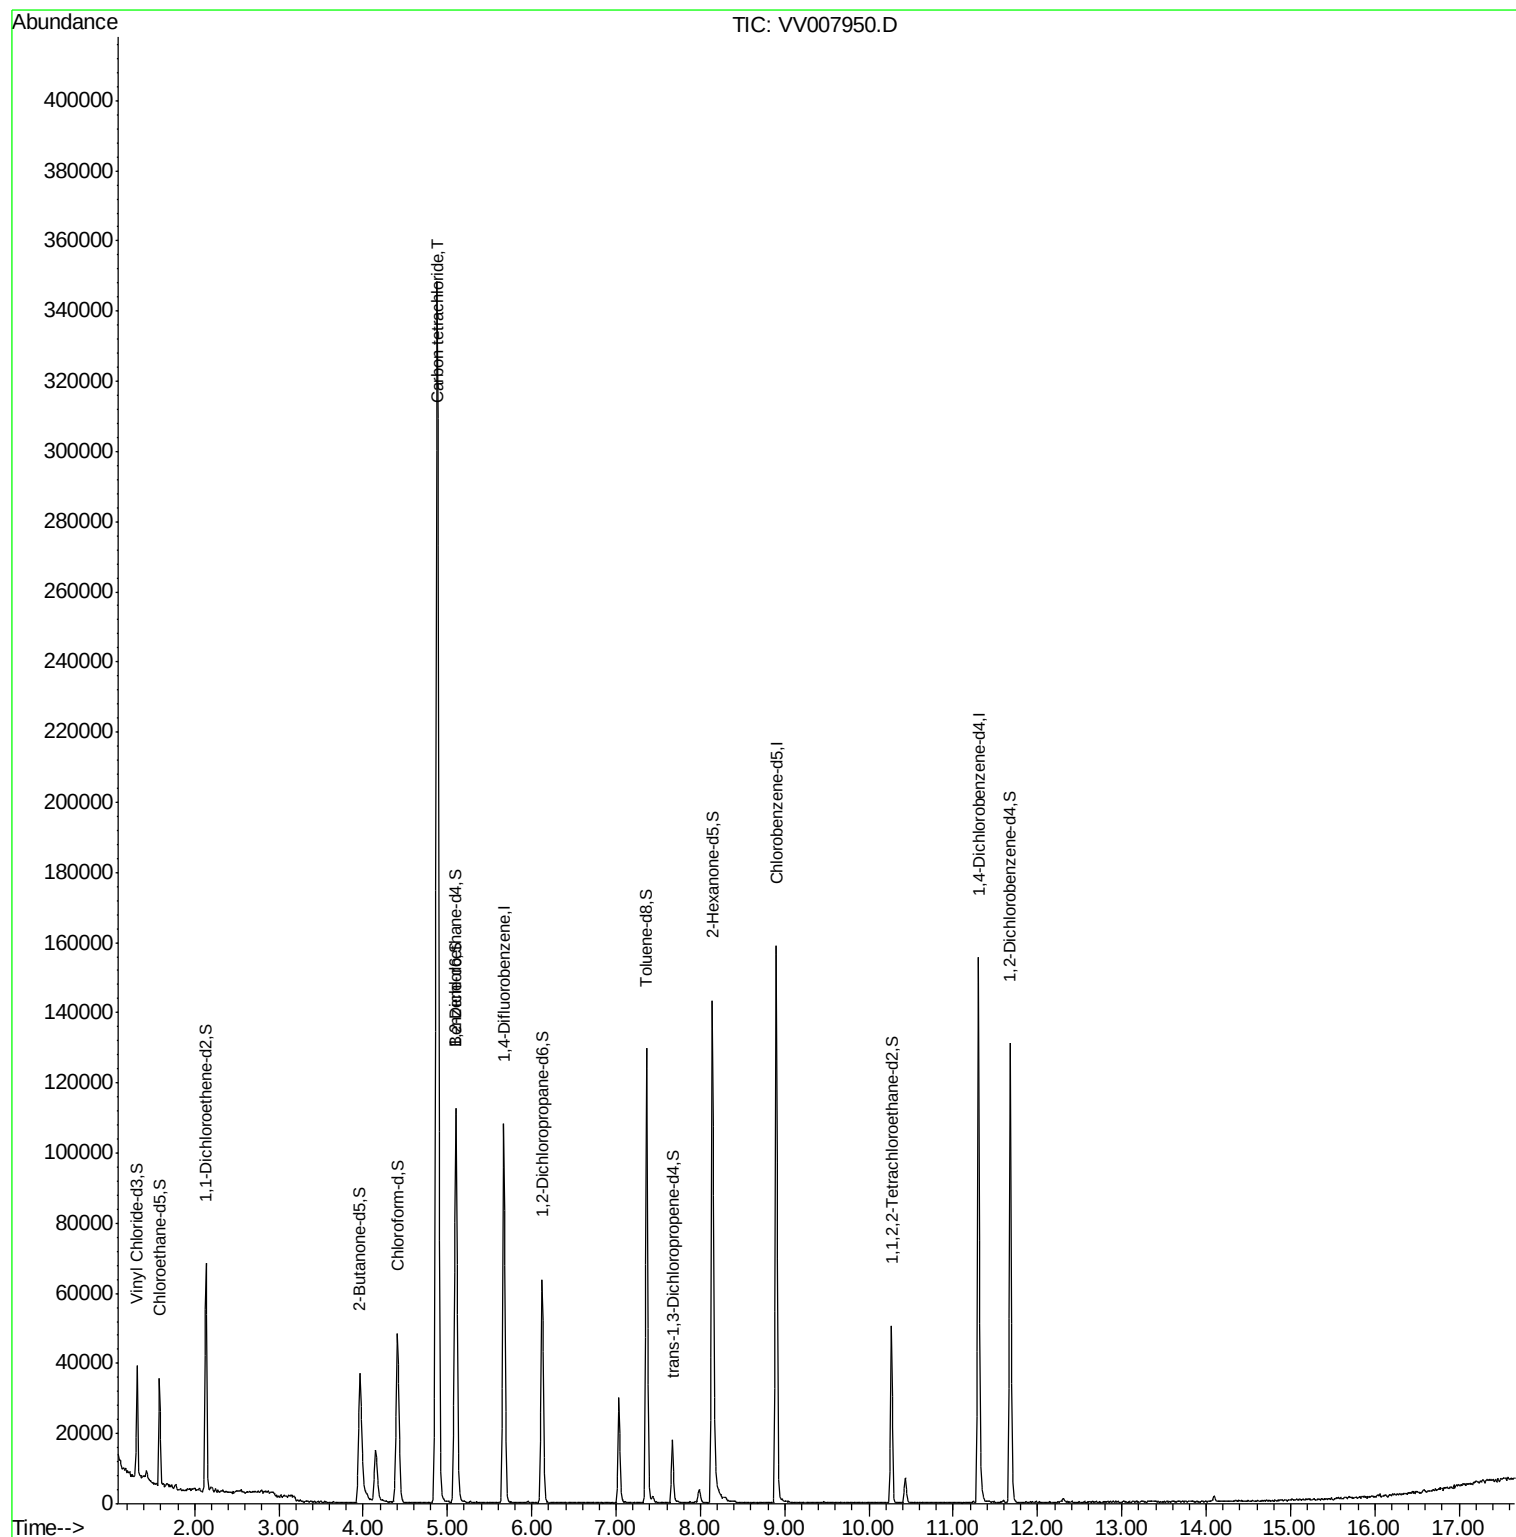

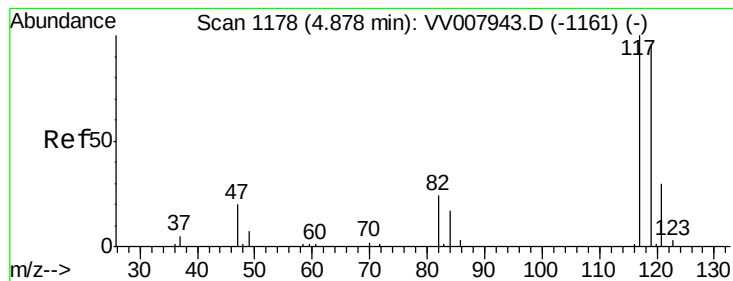

#31

Carbon tetrachloride

Concen: 27.459 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007950.D

Acq: 28 Sep 2018 13:33

Instrument :

MSVOA_V

ClientSampleId :

GAC37

Tot Ion:117 Resp: 255334

Ion Ratio Lower Upper

117 100

119 96.3 77.8 116.8

