

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007952.D
 Acq On : 28 Sep 2018 14:28
 Operator : SY/MD
 Sample : J5063-01DL 20X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC22DL

Quant Time: Oct 01 02:48:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 01:51:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	92071	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	89205	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	45288	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19571	3.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.20%
7) Chloroethane-d5	1.59	69	19443	4.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.20%
11) 1,1-Dichloroethene-d2	2.14	63	33127	2.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.40%#
20) 2-Butanone-d5	3.96	46	69820	47.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.06%
24) Chloroform-d	4.41	84	50603	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
26) 1,2-Dichloroethane-d4	5.09	65	28234	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
32) Benzene-d6	5.10	84	96354	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	30936	4.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.60%
41) Toluene-d8	7.36	98	91852	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	7.67	79	10673	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.14	63	54190	47.23	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.46%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	23450	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	39364	4.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.80%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	96422	10.197 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007952.D
Acq On : 28 Sep 2018 14:28
Operator : SY/MD
Sample : J5063-01DL 20X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC22DL

Quant Time: Oct 01 02:48:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 01:51:53 2018
Response via : Initial Calibration

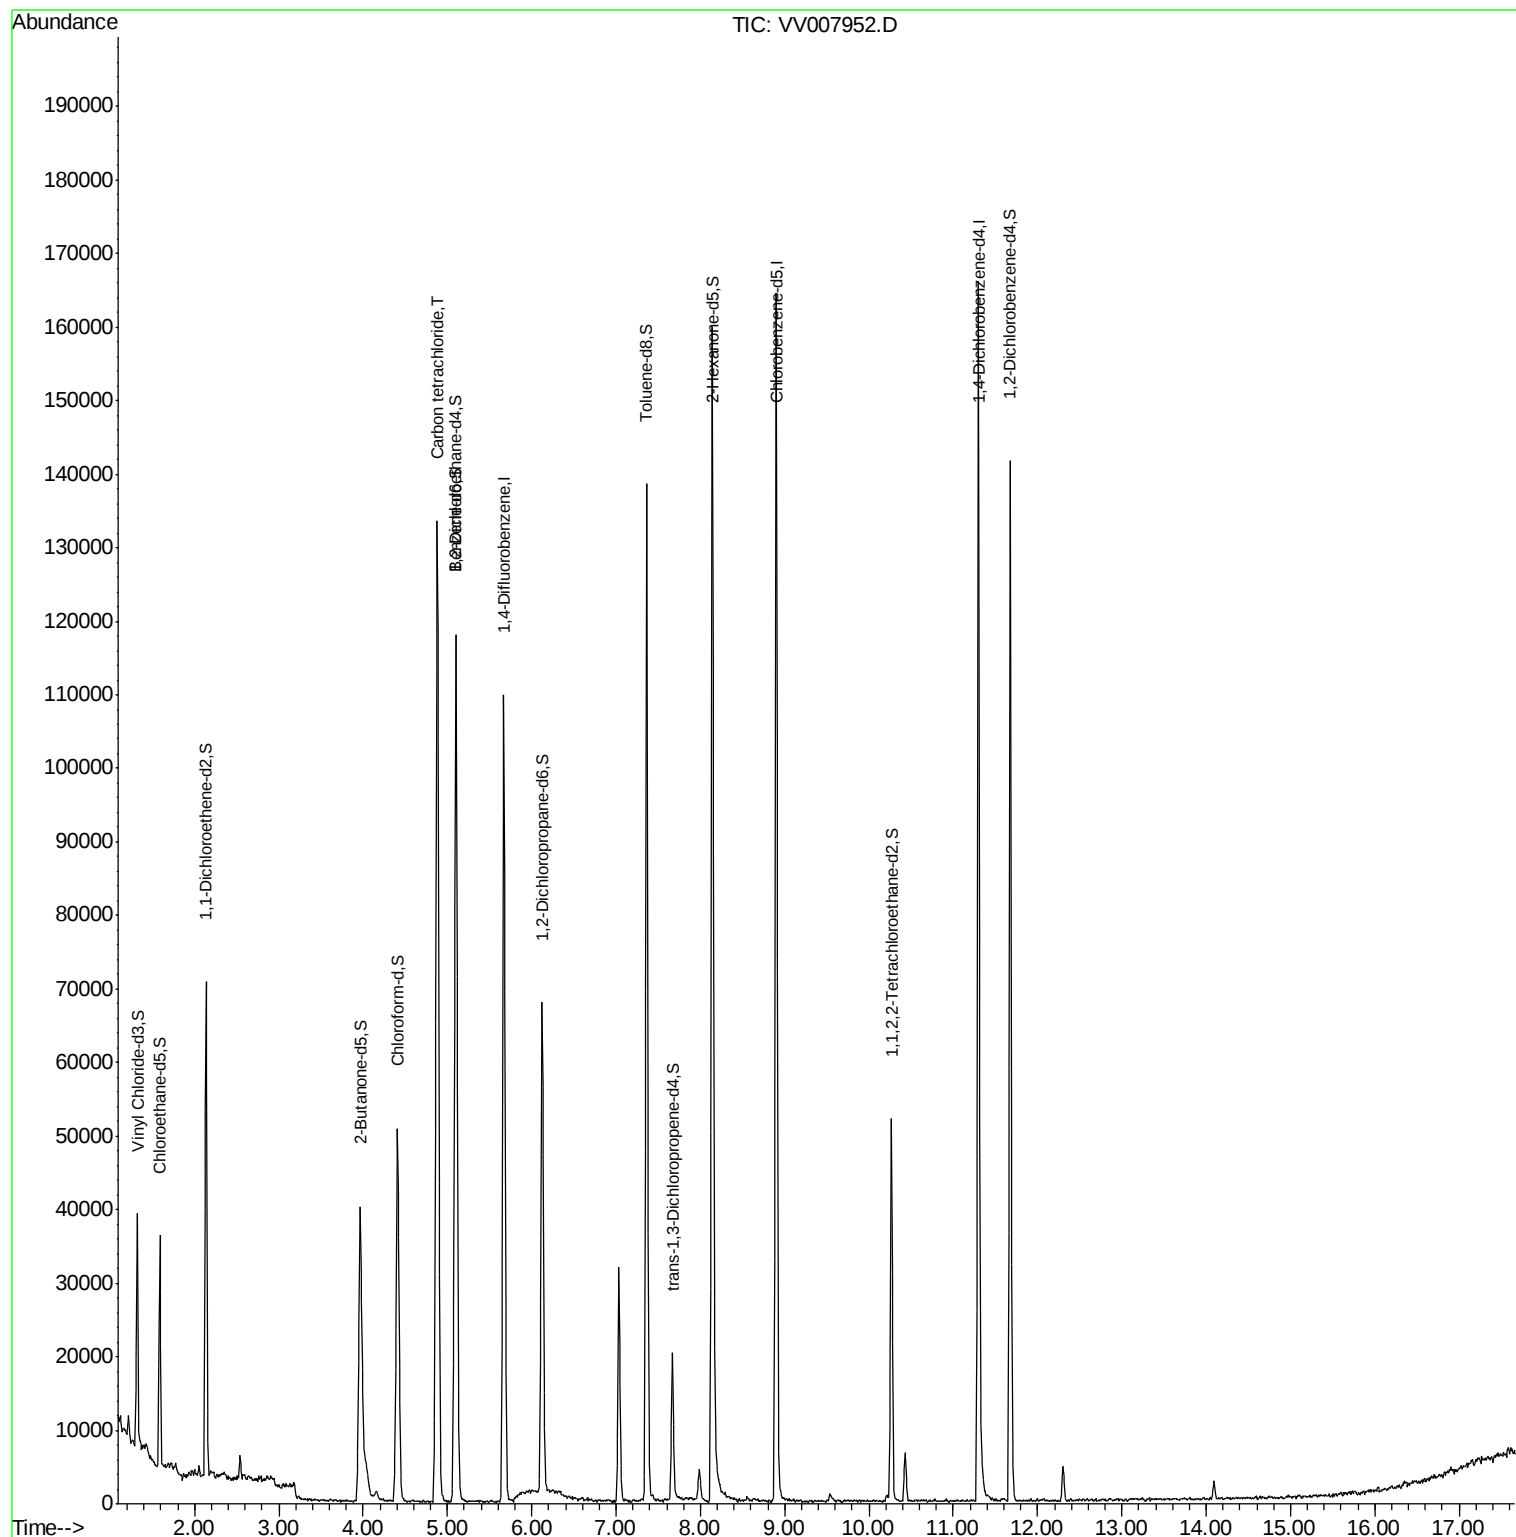

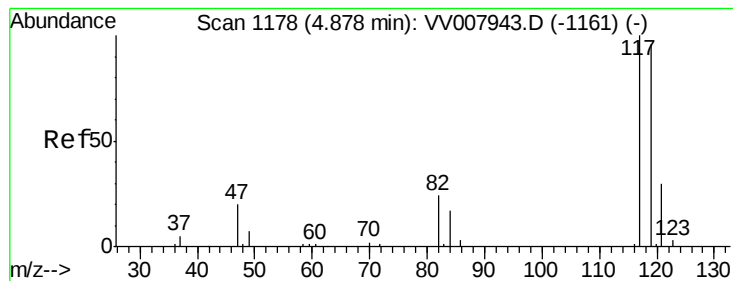

#31

Carbon tetrachloride

Concen: 10.197 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007952.D

Acq: 28 Sep 2018 14:28

Instrument :

MSVOA_V

ClientSampleId :

GAC22DL

Tot Ion:117 Resp: 96422

Ion Ratio Lower Upper

117 100

119 97.2 77.8 116.8

