

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007953.D
 Acq On : 28 Sep 2018 14:55
 Operator : SY/MD
 Sample : J5063-03DL 10X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC24DL

Quant Time: Oct 01 03:43:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 01:51:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	93719	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	89130	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43791	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20674	4.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.20%
7) Chloroethane-d5	1.59	69	19282	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.14	63	34726	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	3.96	46	68804	45.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.06%
24) Chloroform-d	4.41	84	51221	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.09	65	29102	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
32) Benzene-d6	5.10	84	99038	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.12	67	31269	4.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.60%
41) Toluene-d8	7.36	98	93752	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
43) trans-1,3-Dichloropropene-	7.67	79	10426	4.01	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.20%
46) 2-Hexanone-d5	8.14	63	54119	47.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.40%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	23867	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	40328	4.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.20%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	56345	5.963 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007953.D
Acq On : 28 Sep 2018 14:55
Operator : SY/MD
Sample : J5063-03DL 10X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC24DL

Quant Time: Oct 01 03:43:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 01:51:53 2018
Response via : Initial Calibration

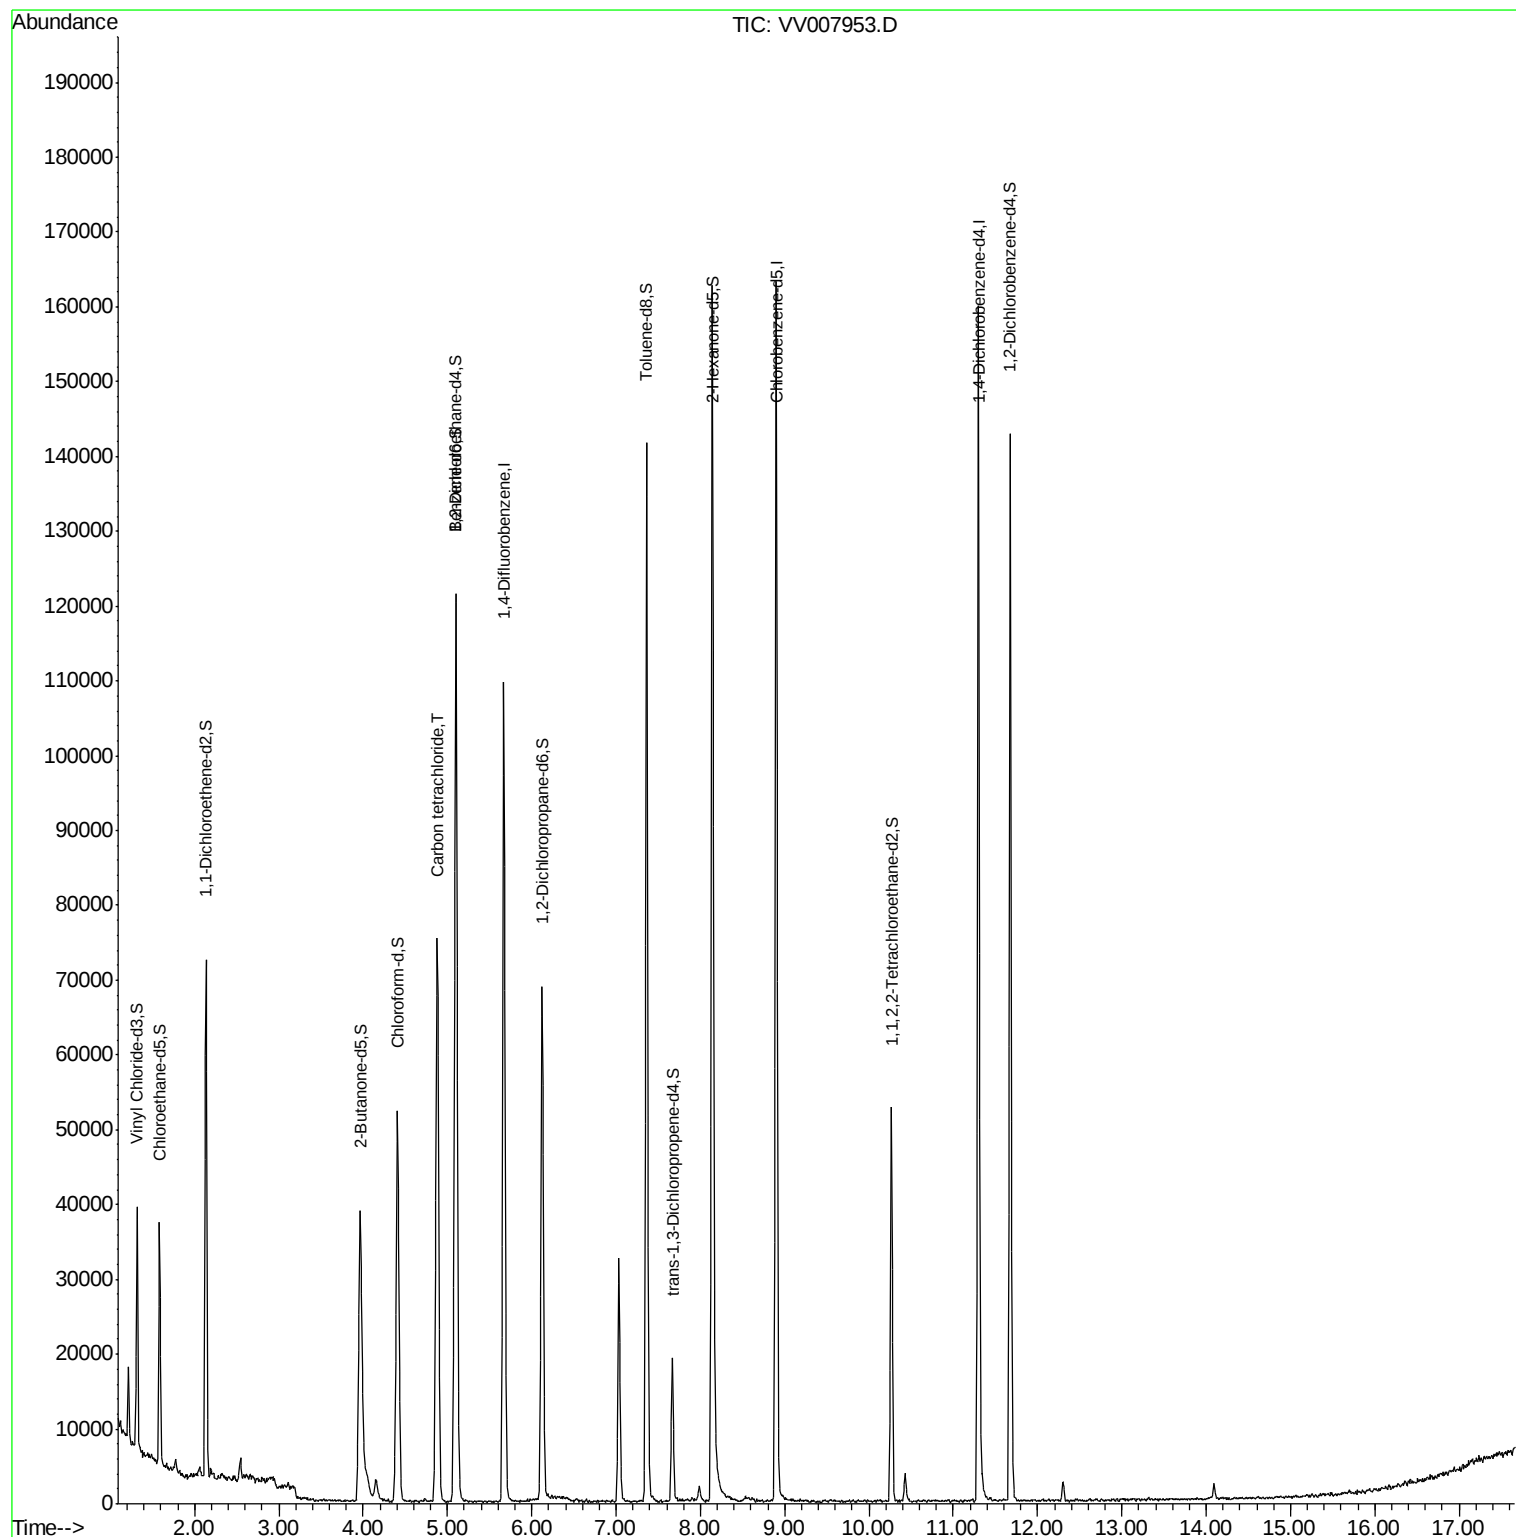

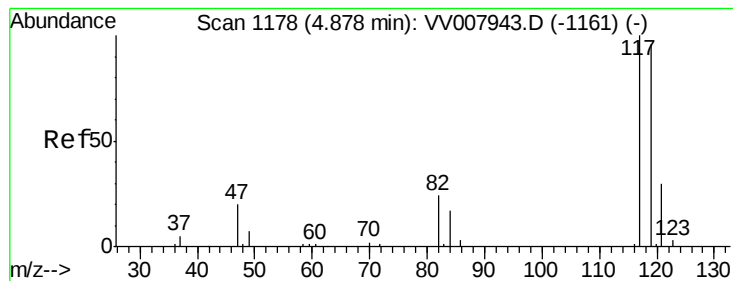

#31

Carbon tetrachloride

Concen: 5.963 ug/L

RT: 4.88 min Scan# 1178

Delta R.T. 0.00 min

Lab File: VV007953.D

Acq: 28 Sep 2018 14:55

Instrument :

MSVOA_V

ClientSampleId :

GAC24DL

Tot Ion:117 Resp: 56345

Ion Ratio Lower Upper

117 100

119 95.4 77.8 116.8

