

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007956.D
 Acq On : 28 Sep 2018 16:17
 Operator : SY/MD
 Sample : J5063-10DL 5X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC31DL

Quant Time: Oct 01 04:00:08 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 01:51:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91798	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	87847	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43756	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19377	3.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.80%
7) Chloroethane-d5	1.59	69	18990	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.14	63	34052	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	3.97	46	70996	47.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.92%
24) Chloroform-d	4.41	84	49090	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
26) 1,2-Dichloroethane-d4	5.09	65	28609	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.10	84	96629	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.12	67	30390	4.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.40%
41) Toluene-d8	7.36	98	88651	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	7.67	79	10043	3.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.40%
46) 2-Hexanone-d5	8.14	63	51823	45.86	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.72%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	23018	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	37792	4.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.20%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	56719	6.091 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007956.D
Acq On : 28 Sep 2018 16:17
Operator : SY/MD
Sample : J5063-10DL 5X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC31DL

Quant Time: Oct 01 04:00:08 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 01:51:53 2018
Response via : Initial Calibration

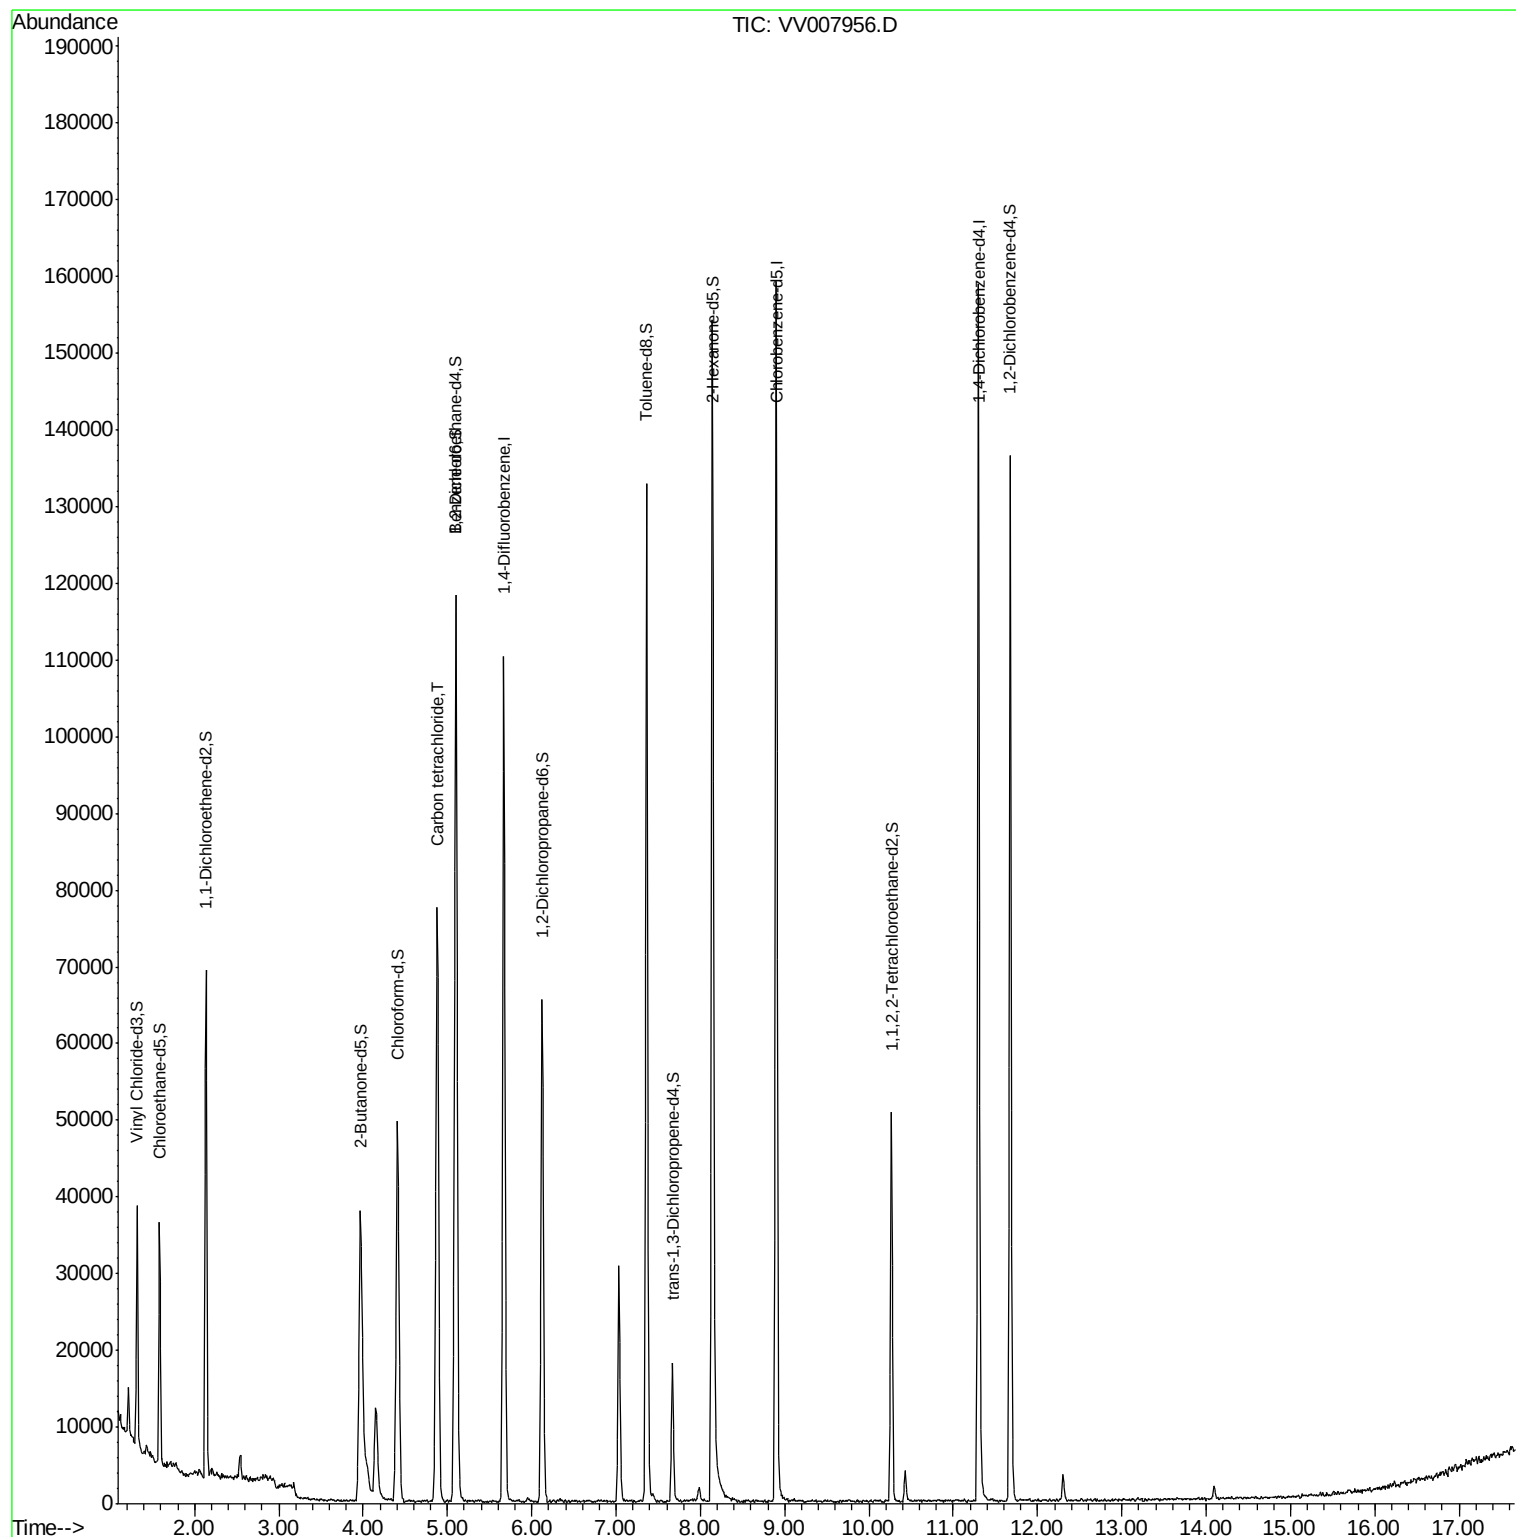

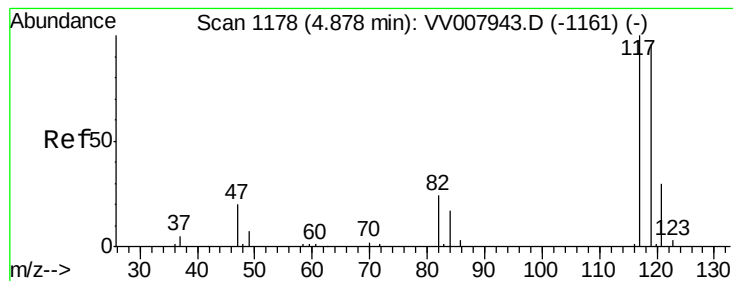

#31

Carbon tetrachloride

Concen: 6.091 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007956.D

Acq: 28 Sep 2018 16:17

Instrument :

MSVOA_V

ClientSampleId :

GAC31DL

Tot Ion:117 Resp: 56719

Ion Ratio Lower Upper

117 100

119 96.6 77.8 116.8

