

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007958.D
 Acq On : 28 Sep 2018 17:12
 Operator : SY/MD
 Sample : J5062-16
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC16

Quant Time: Oct 01 04:10:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 01:51:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91614	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88008	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	44291	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18157	3.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.00%
7) Chloroethane-d5	1.59	69	17800	4.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.80%
11) 1,1-Dichloroethene-d2	2.14	63	31351	2.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.60%#
20) 2-Butanone-d5	3.96	46	64871	43.91	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.82%
24) Chloroform-d	4.41	84	47688	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.20%
26) 1,2-Dichloroethane-d4	5.09	65	25916	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
32) Benzene-d6	5.10	84	88864	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.60%
36) 1,2-Dichloropropane-d6	6.12	67	28885	4.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.80%
41) Toluene-d8	7.36	98	82249	3.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.80%
43) trans-1,3-Dichloropropene-	7.67	79	9563	3.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.60%
46) 2-Hexanone-d5	8.14	63	47739	42.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.34%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21430	4.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	35743	4.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	3896	3.620 ug/L	96
31) Carbon tetrachloride	4.88	117	111059	11.904 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007958.D
Acq On : 28 Sep 2018 17:12
Operator : SY/MD
Sample : J5062-16
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC16

Quant Time: Oct 01 04:10:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 01:51:53 2018
Response via : Initial Calibration

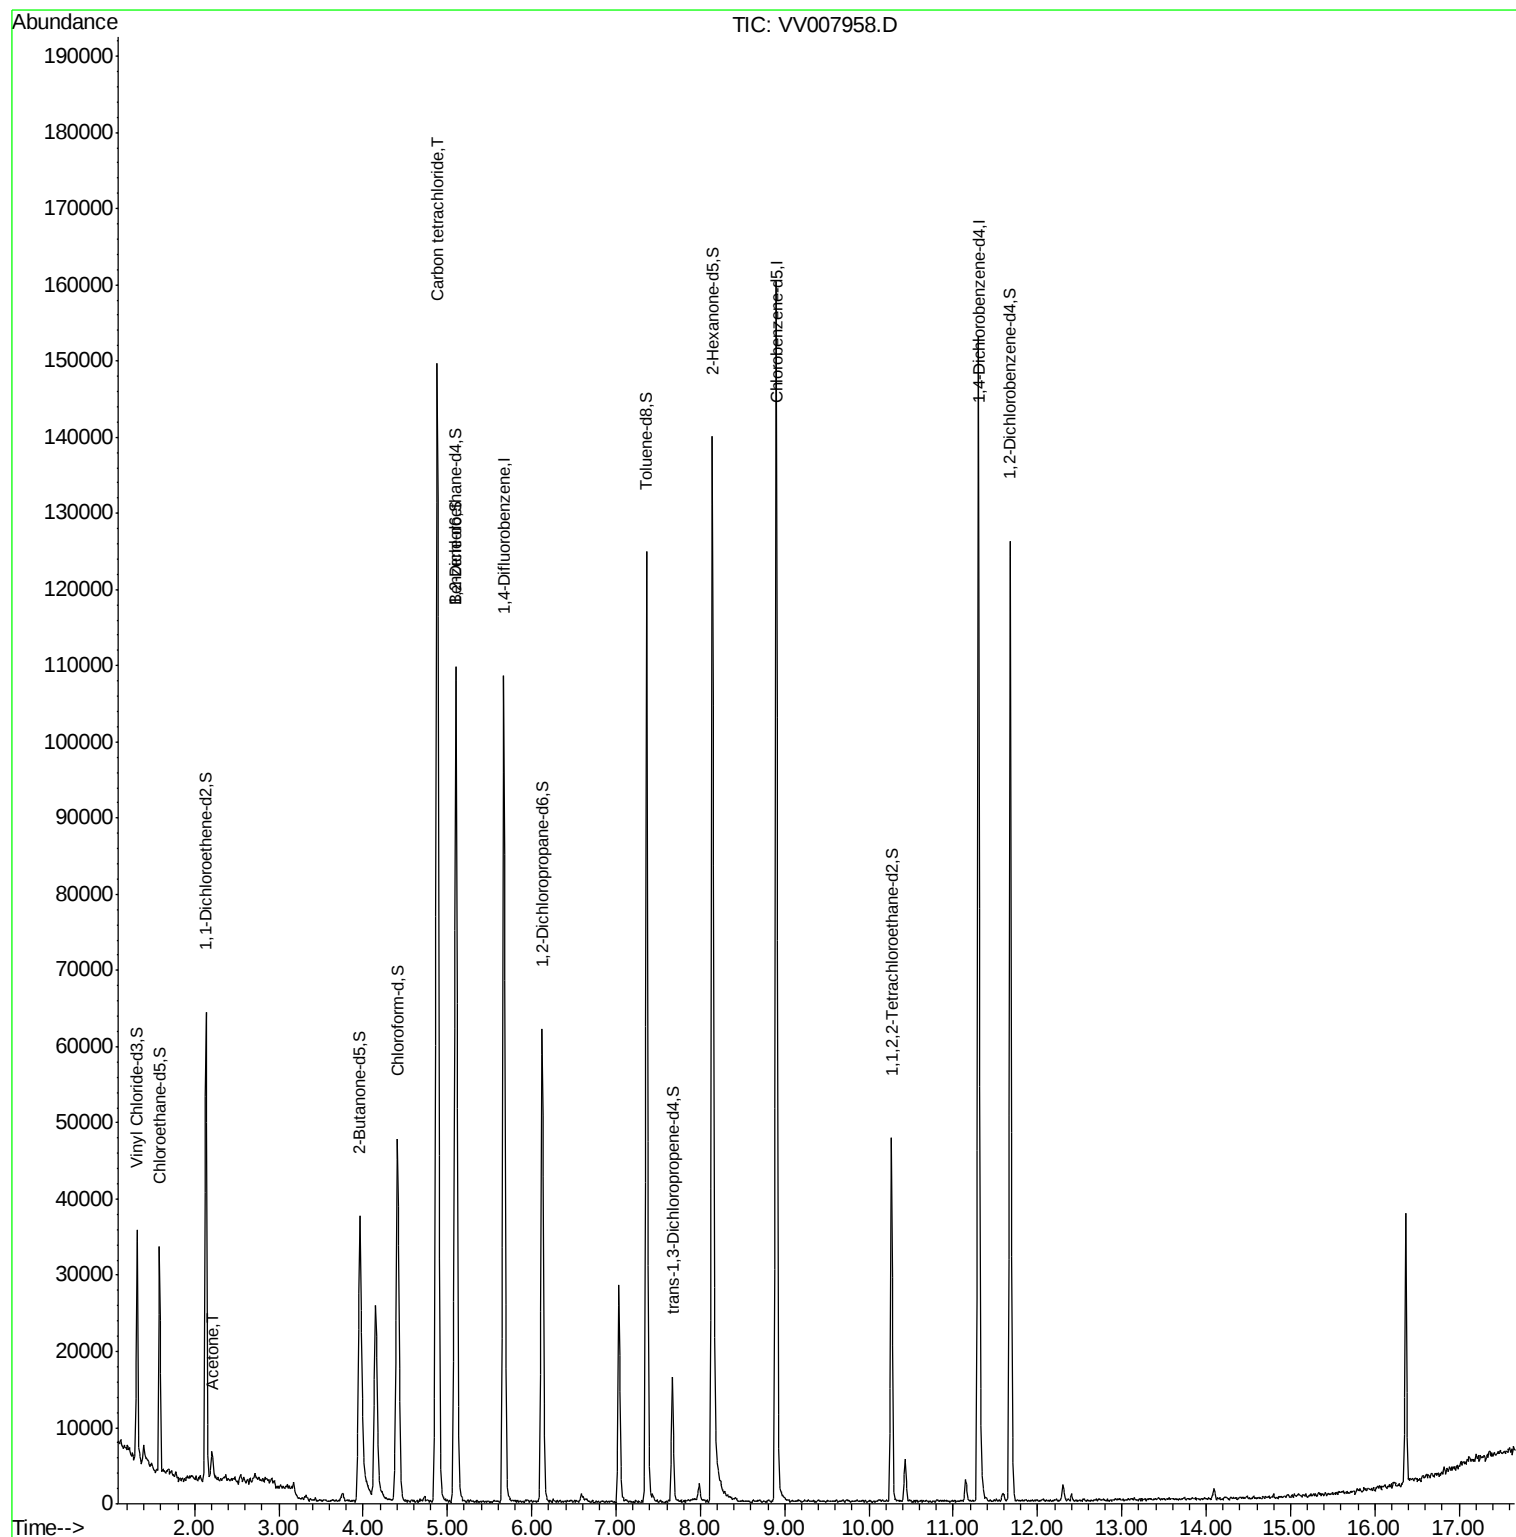

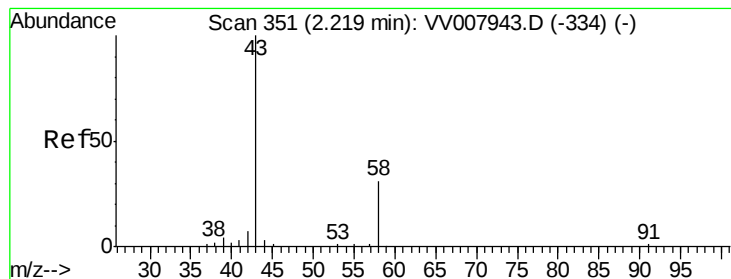

#13

Acetone

Concen: 3.620 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV007958.D

Acq: 28 Sep 2018 17:12

Instrument :

MSVOA_V

ClientSampleId :


GAC16

Tot Ion: 43 Resp: 3896

Ion Ratio Lower Upper

43 100

58 33.0 0.0 62.0

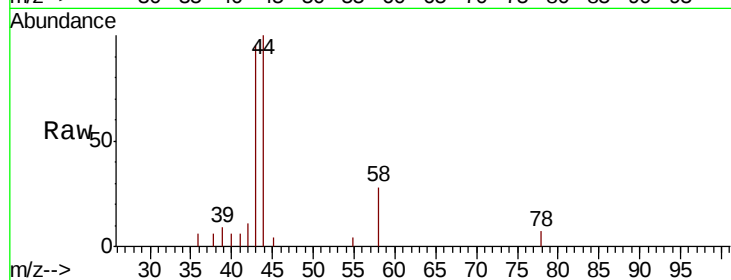

Abundance Ion 43.05 (42.75 to 43.75): VV007943.D (-334) (-)

Ion 58.05 (57.75 to 58.75): VV007943.D (-334) (-)

2.21

2500

2000



1500

1000

500

0

Time-->

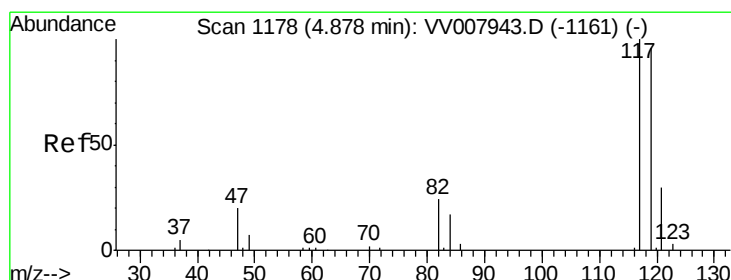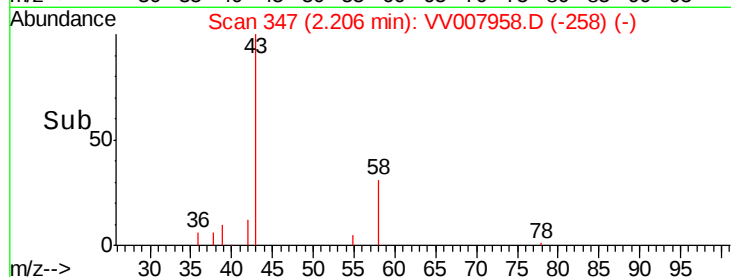

#31

Carbon tetrachloride

Concen: 11.904 ug/L

RT: 4.88 min Scan# 1178

Delta R.T. -0.00 min

Lab File: VV007958.D


Acq: 28 Sep 2018 17:12

Tgt Ion: 117 Resp: 111059

Ion Ratio Lower Upper

117 100

119 95.3 77.8 116.8

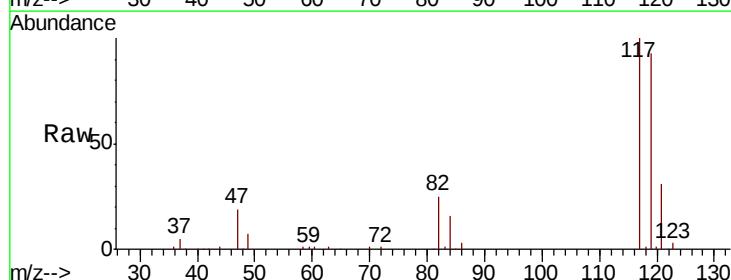

Abundance Ion 116.90 (116.60 to 117.60): VV007943.D (-1161) (-)

Ion 118.90 (118.60 to 119.60): VV007943.D (-1161) (-)

4.88

50000

40000

30000

20000

10000

0

Time-->

