

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007968.D
 Acq On : 28 Sep 2018 22:13
 Operator : SY/MD
 Sample : J5063-12DL 5X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC33DL

Quant Time: Oct 01 05:11:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 04:55:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	88900	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	84076	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41890	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18053	3.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.80%
7) Chloroethane-d5	1.59	69	18239	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.14	63	31669	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	3.96	46	67464	47.06	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.12%
24) Chloroform-d	4.41	84	48045	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.09	65	26468	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
32) Benzene-d6	5.10	84	91312	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.12	67	30108	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.36	98	83668	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
43) trans-1,3-Dichloropropene-	7.67	79	9148	3.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.60%
46) 2-Hexanone-d5	8.14	63	48071	44.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.90%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22393	4.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	36925	4.55	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.00%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	99067	11.115 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007968.D
Acq On : 28 Sep 2018 22:13
Operator : SY/MD
Sample : J5063-12DL 5X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
GAC33DL

Quant Time: Oct 01 05:11:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 04:55:39 2018
Response via : Initial Calibration

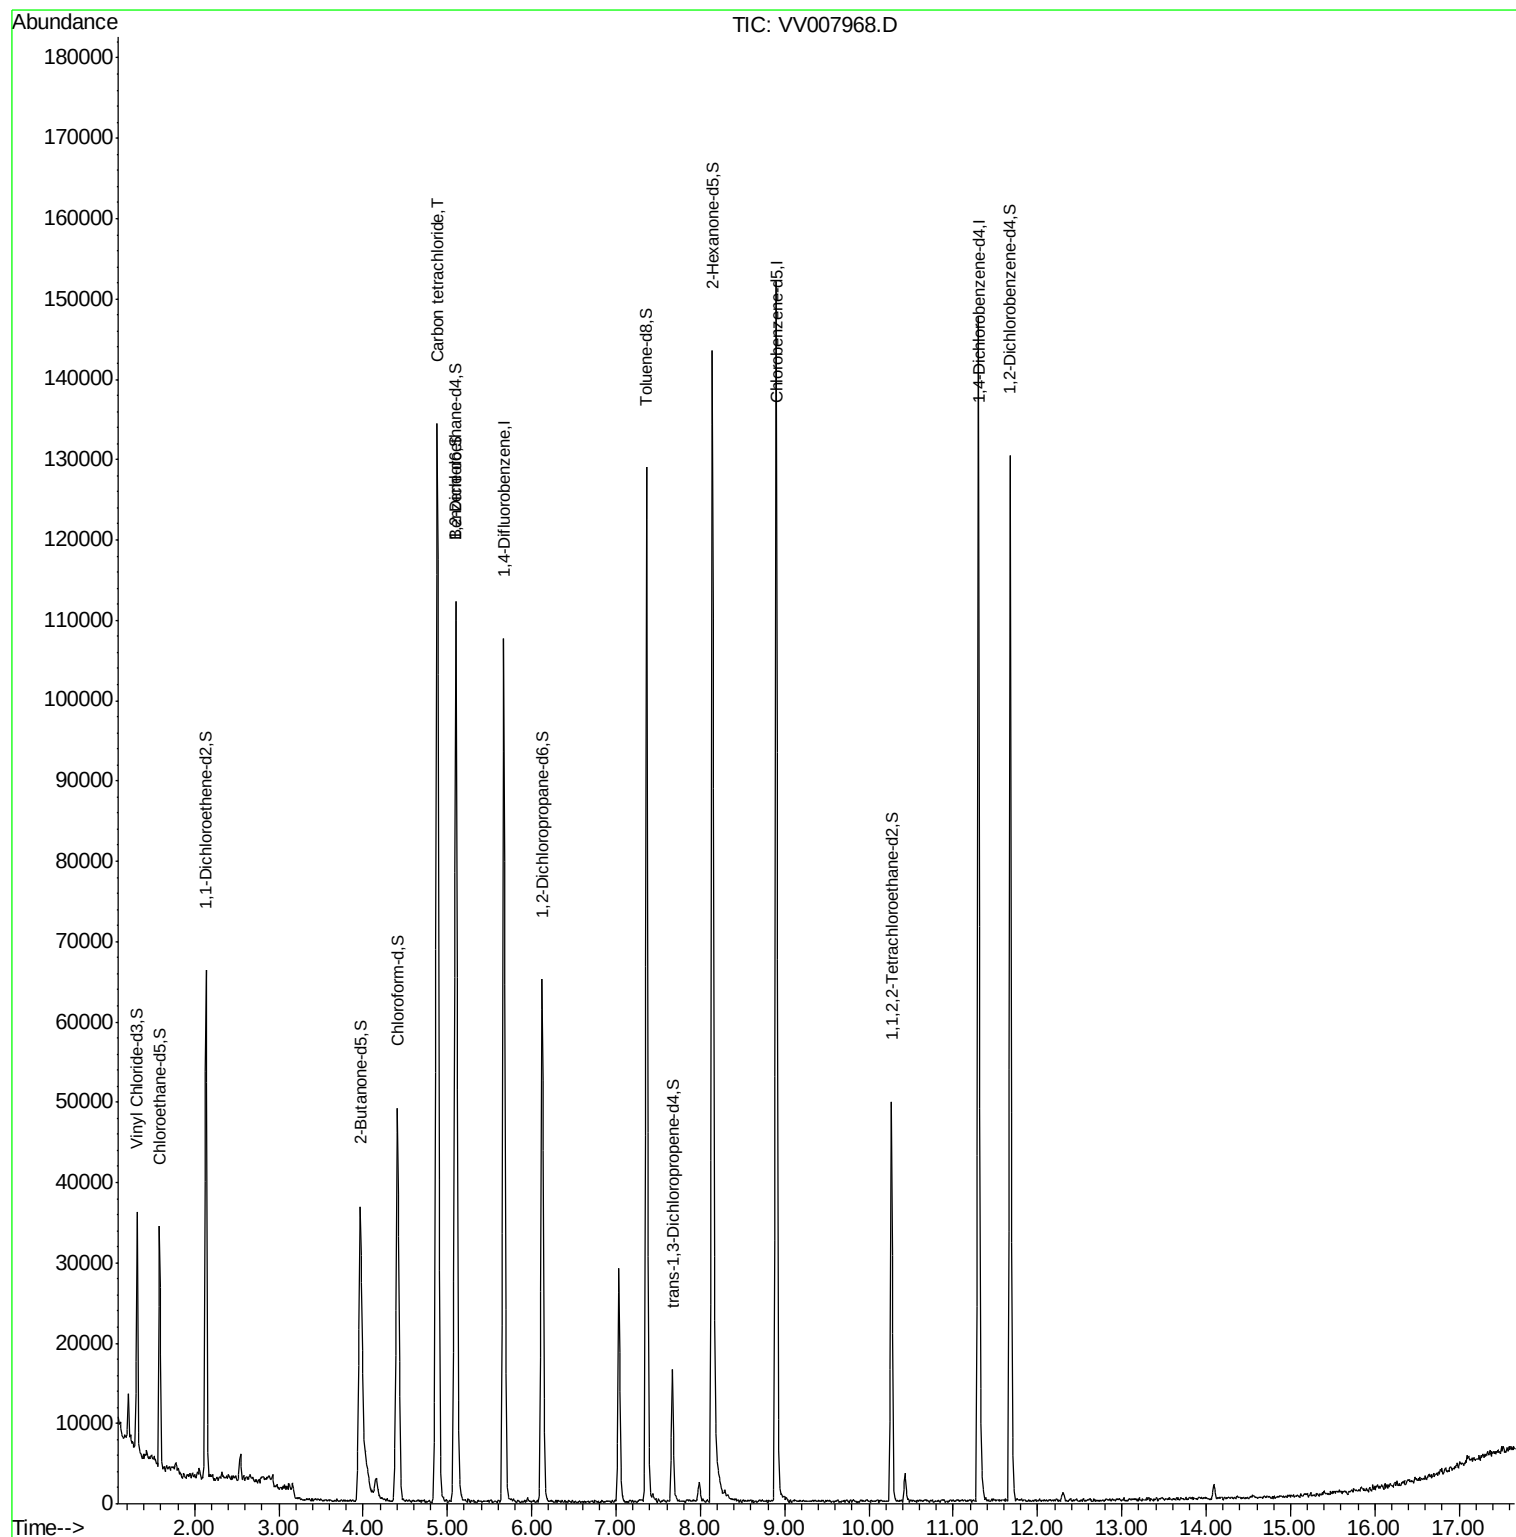

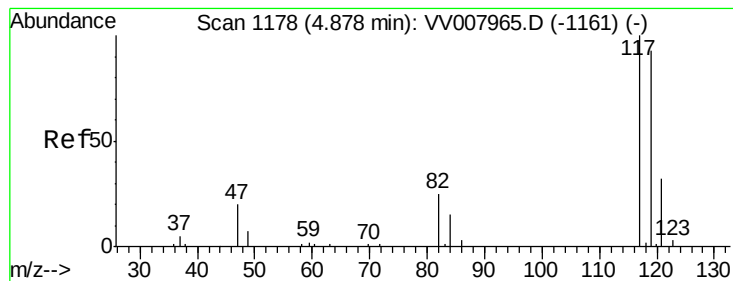

#31

Carbon tetrachloride

Concen: 11.115 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007968.D

Acq: 28 Sep 2018 22:13

Instrument :

MSVOA_V

ClientSampleId :

GAC33DL

Tot Ion:117 Resp: 99067

Ion Ratio Lower Upper

117 100

119 95.1 77.8 116.8

