

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007979.D
 Acq On : 29 Sep 2018 03:12
 Operator : SY/MD
 Sample : J5159-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC89

Quant Time: Oct 01 06:43:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 04:55:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	87765	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	83243	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40643	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	16825	3.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.60%
7) Chloroethane-d5	1.59	69	18037	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.14	63	30665	2.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.80%#
20) 2-Butanone-d5	3.97	46	69569	49.16	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.32%
24) Chloroform-d	4.41	84	47892	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.09	65	26771	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
32) Benzene-d6	5.10	84	90675	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
36) 1,2-Dichloropropane-d6	6.12	67	29705	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.36	98	82834	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
43) trans-1,3-Dichloropropene-	7.67	79	8459	3.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.80%
46) 2-Hexanone-d5	8.14	63	49725	46.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22413	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	35089	4.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.20%


Target Compounds					Ovalue
47) Tetrachloroethene	8.02	164	11795	1.865 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007979.D
Acq On : 29 Sep 2018 03:12
Operator : SY/MD
Sample : J5159-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC89

Quant Time: Oct 01 06:43:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 04:55:39 2018
Response via : Initial Calibration

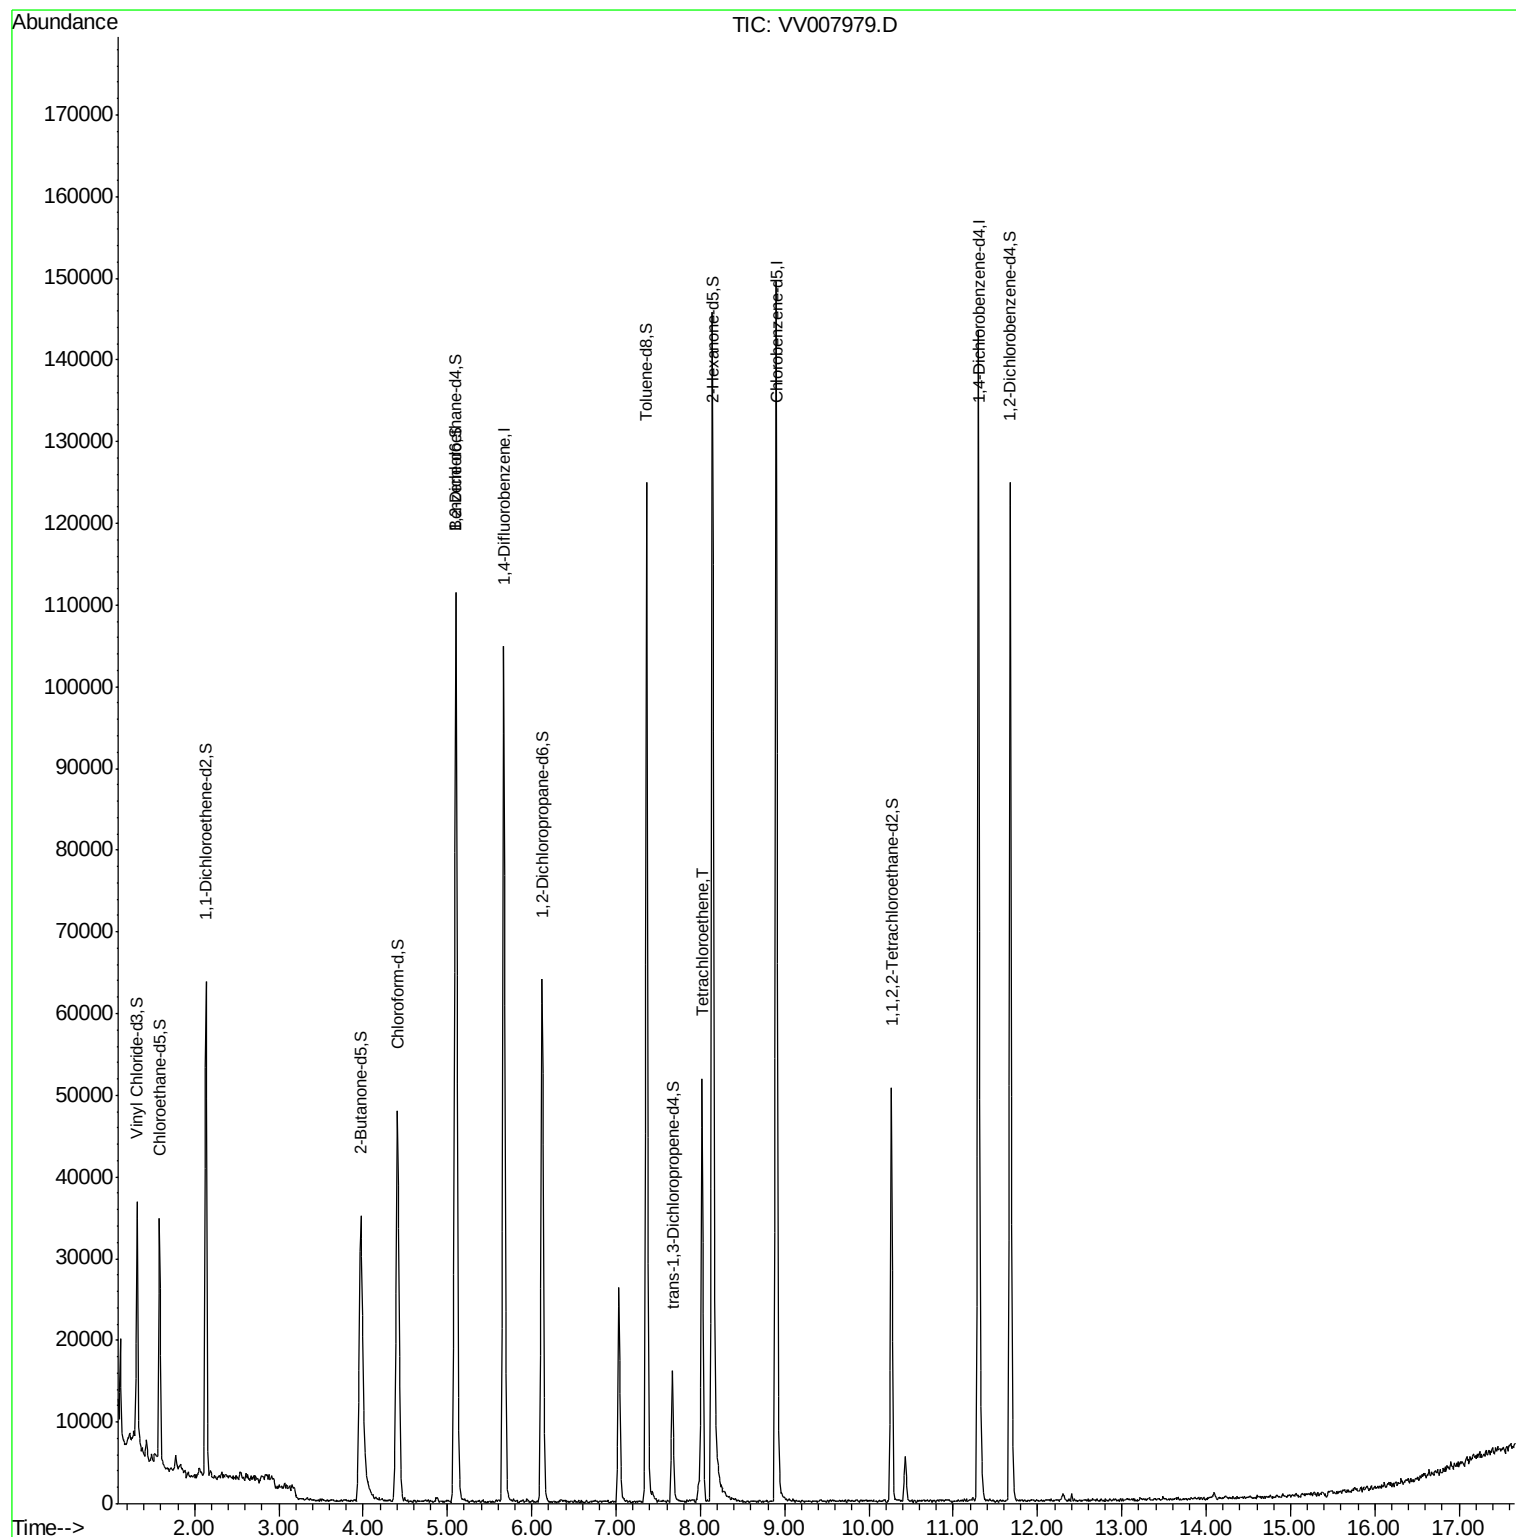

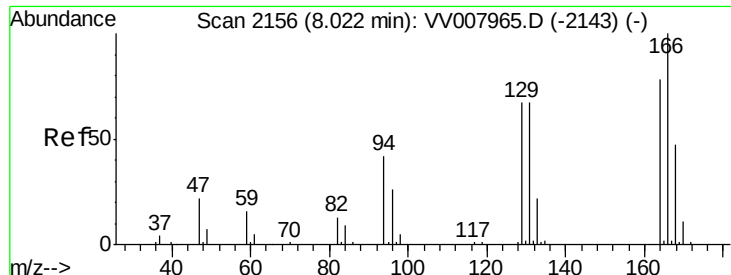

#47

Tetrachloroethene

Concen: 1.865 ug/L

RT: 8.02 min Scan# 2156

Delta R.T. 0.00 min

Lab File: VV007979.D


Acq: 29 Sep 2018 03:12

Instrument :

MSVOA_V

ClientSampleId :

GAC89

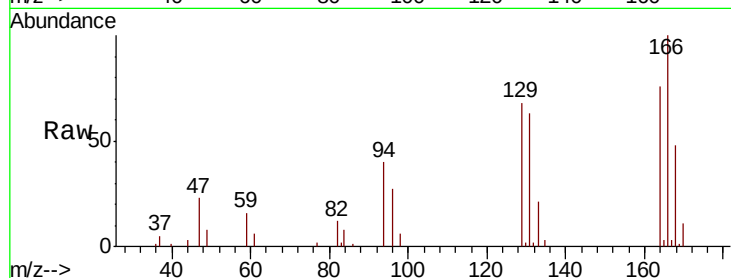

Tot Ion:164 Resp: 11795


Ion Ratio Lower Upper

164 100

129 89.7 59.2 110.0

131 83.0 57.1 106.1

166 131.6 88.6 164.6

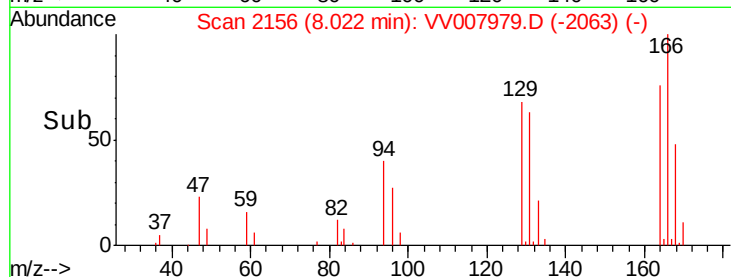

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

