

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
 Data File : VV007986.D
 Acq On : 29 Sep 2018 06:23
 Operator : SY/MD
 Sample : J5062-14DL 10X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC14DL

Quant Time: Oct 01 09:52:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 01 04:55:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89840	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	86784	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43331	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	20135	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.58	69	17690	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.00%
11) 1,1-Dichloroethene-d2	2.13	63	31158	2.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.20%#
20) 2-Butanone-d5	3.99	46	59432	41.03	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.06%
24) Chloroform-d	4.41	84	48551	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.09	65	26072	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
32) Benzene-d6	5.10	84	91444	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
36) 1,2-Dichloropropane-d6	6.12	67	29407	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.36	98	84900	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.40%
43) trans-1,3-Dichloropropene-	7.67	79	9396	3.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.40%
46) 2-Hexanone-d5	8.14	63	49071	43.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.92%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22553	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	37552	4.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.60%


Target Compounds					Ovalue
15) Methyl Acetate	2.48	43	10025	3.714 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007986.D
Acq On : 29 Sep 2018 06:23
Operator : SY/MD
Sample : J5062-14DL 10X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC14DL

Quant Time: Oct 01 09:52:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 01 04:55:39 2018
Response via : Initial Calibration

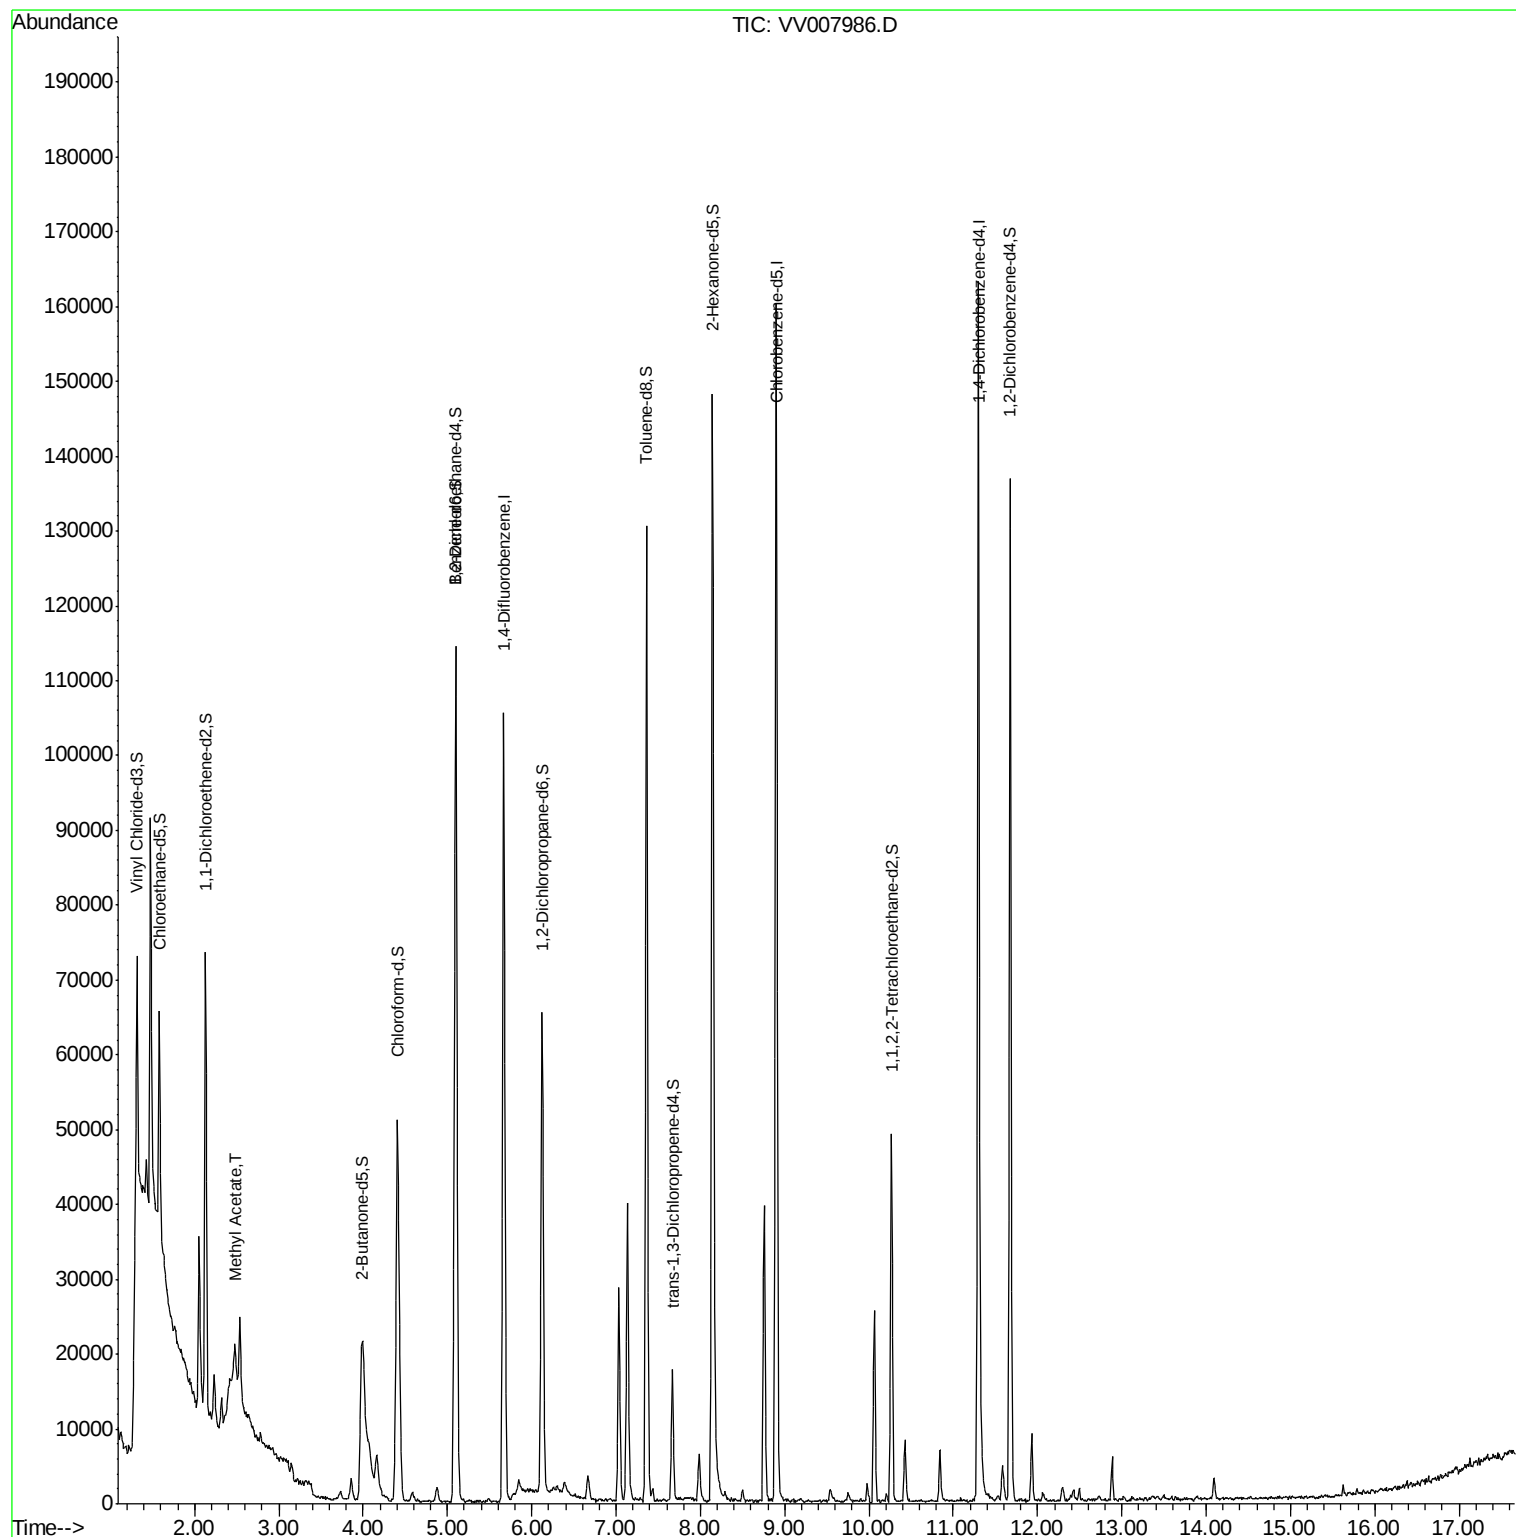

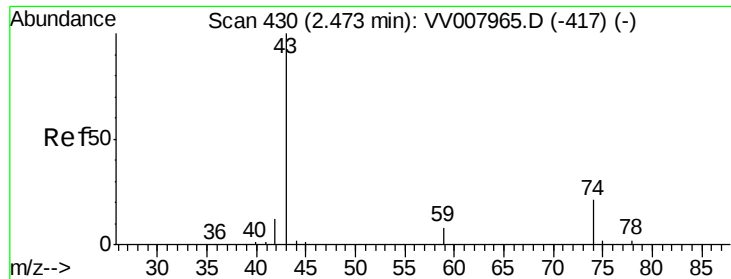

#15
Methyl Acetate
Concen: 3.714 ug/L
RT: 2.48 min Scan# 432
Delta R.T. 0.01 min
Lab File: VV007986.D
Acq: 29 Sep 2018 06:23

Instrument :
MSVOA_V
ClientSampleId :
GAC14DL

Tot Ion: 43 Resp: 10025
Ion Ratio Lower Upper
43 100
74 21.3 19.5 29.3

