


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092818\
Data File : VV007942.D
Acq On : 28 Sep 2018 09:18
Operator : SY/MD
Sample : BFB77
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 02 04:17:24 2018

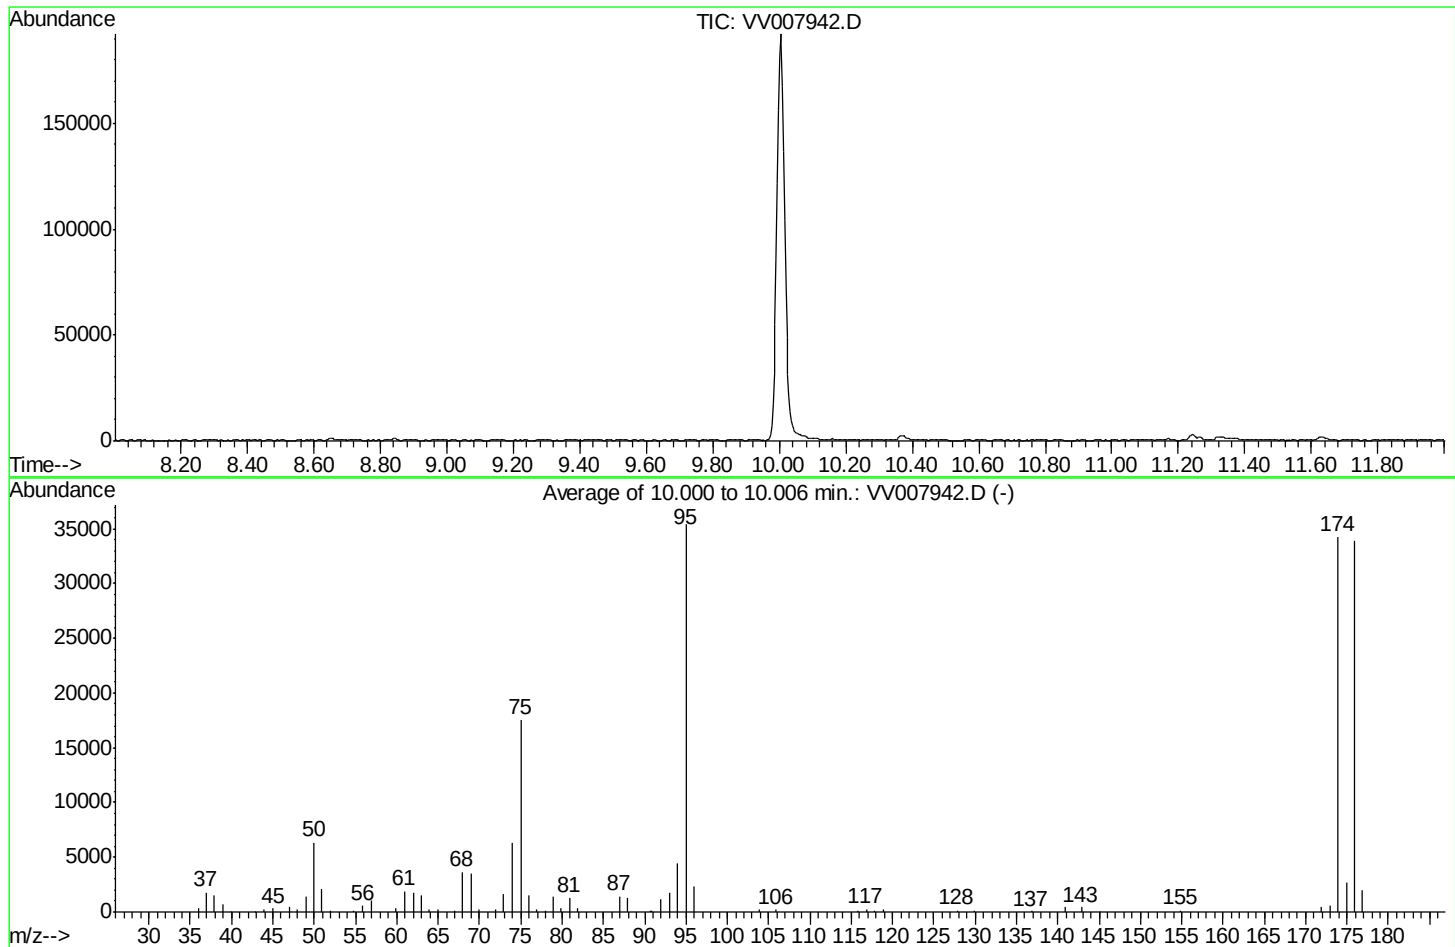

AutoFind: Scans 2771, 2772, 2773; Background Corrected with Scan 2759

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	6345	PASS
75	95	30	80	49.7	17589	PASS
95	95	100	100	100.0	35402	PASS
96	95	5	9	6.7	2366	PASS
173	174	0.00	2	1.8	607	PASS
174	95	50	120	96.9	34304	PASS
175	174	5	9	8.0	2737	PASS
176	174	95	101	98.7	33874	PASS
177	176	5	9	6.0	2047	PASS

Scan 2759 (9.961 min): VV007942.D
BFB77

m/z	Abundance
39.80	107.0
44.00	284.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	322.0
36.90	1770.0
37.90	1575.0
39.00	644.0
39.90	134.0
43.90	516.0
45.10	302.0
46.90	467.0
47.90	217.0
48.90	1333.0
50.00	6352.0
50.90	2156.0
51.90	108.0
54.80	119.0
55.90	577.0
57.00	1032.0
59.90	351.0
60.90	1841.0
62.00	1677.0
62.90	1453.0
63.90	181.0
65.00	263.0
67.00	168.0
67.90	3623.0
69.00	3516.0
69.90	263.0
72.00	230.0
73.00	1616.0
74.00	6320.0
75.00	17384.0
76.00	1426.0
76.80	232.0
78.00	111.0
78.80	1317.0
79.90	362.0
80.90	1335.0
81.90	326.0
86.90	1441.0
87.90	1232.0
90.70	192.0
92.00	1134.0
92.90	1701.0
94.00	4290.0
95.00	34424.0
96.00	2321.0
103.80	172.0
105.90	204.0
115.80	139.0
116.80	243.0
117.80	170.0
118.80	247.0
127.80	175.0
129.90	124.0
140.80	377.0
142.90	450.0
154.80	117.0
171.90	432.0
173.00	609.0
173.90	32968.0
174.90	2698.0
175.90	32088.0
176.90	1968.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	308.0
36.90	1722.0
37.90	1535.0
39.00	663.0
39.90	123.0
42.90	102.0
44.00	498.0
45.00	322.0
47.00	459.0
47.90	218.0
49.00	1460.0
50.00	6212.0
51.00	2036.0
51.90	127.0
54.80	149.0
55.90	571.0
57.00	1120.0
59.90	354.0
61.00	1852.0
62.00	1691.0
62.90	1482.0
63.80	220.0
64.90	260.0
66.90	180.0
67.90	3509.0
69.00	3416.0
69.90	309.0
71.80	175.0
72.90	1548.0
74.00	6242.0
75.00	17392.0
76.00	1598.0
76.90	231.0
77.90	121.0
78.90	1360.0
79.90	368.0
80.90	1252.0
81.80	286.0
87.00	1370.0
87.90	1289.0
90.90	214.0
91.90	1079.0
93.00	1649.0
94.00	4396.0
95.00	35408.0
96.00	2323.0
103.80	194.0
105.90	203.0
115.80	191.0
116.80	266.0
117.90	147.0
118.90	224.0
127.80	129.0
129.90	106.0
136.90	125.0
140.90	476.0
142.90	436.0
145.00	104.0
154.90	126.0
171.80	523.0
173.00	571.0
173.90	34832.0
174.90	2702.0
175.90	34552.0
176.90	2061.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	337.0
36.90	1838.0
37.90	1628.0
39.00	674.0
39.90	125.0
43.90	530.0
45.10	317.0
46.90	515.0
48.00	227.0
48.90	1493.0
50.00	6471.0
51.00	2239.0
51.90	116.0
54.80	143.0
55.90	589.0
57.00	1128.0
59.90	373.0
60.90	1966.0
62.00	1743.0
63.00	1577.0
63.90	207.0
65.00	278.0
67.00	184.0
67.90	3745.0
69.00	3578.0
70.00	300.0
71.90	186.0
73.00	1631.0
74.00	6523.0
75.00	17992.0
76.00	1567.0
76.90	241.0
78.00	119.0
78.90	1396.0
79.90	386.0
80.90	1354.0
81.90	329.0
87.00	1552.0
87.90	1295.0
90.90	220.0
91.90	1151.0
93.00	1764.0
94.00	4521.0
95.00	36376.0
96.00	2456.0
103.80	192.0
105.90	214.0
115.80	173.0
116.80	275.0
117.80	167.0
118.90	239.0
127.80	162.0
129.90	121.0
136.80	114.0
140.90	435.0
142.90	478.0
154.90	128.0
171.80	453.0
173.00	642.0
173.90	35112.0
174.90	2813.0
175.90	34984.0
176.90	2112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77