

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092820\
 Data File : VV018490.D
 Acq On : 28 Sep 2020 13:49
 Operator : SY/MD
 Sample : L4117-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	211618	209936	14.83%	1.910%
2	1.579	144	152	167	rBV	174286	197091	13.92%	1.793%
3	2.122	310	321	348	rVB	350208	535766	37.84%	4.875%
4	2.447	420	422	430	rVB	261	218	0.02%	0.002%
5	2.531	434	448	462	rBV4	4483	9367	0.66%	0.085%
6	2.782	516	526	536	rVB6	2279	4218	0.30%	0.038%
7	2.958	578	581	586	rVB	191	151	0.01%	0.001%
8	2.994	586	592	594	rBV	172	159	0.01%	0.001%
9	3.065	603	614	628	rVV2	6517	13101	0.93%	0.119%
10	3.116	628	630	636	rVB	209	168	0.01%	0.002%
11	3.145	636	639	647	rVB2	183	211	0.01%	0.002%
12	3.521	749	756	760	rBV	142	196	0.01%	0.002%
13	3.917	868	879	922	rBV	96062	293929	20.76%	2.675%
14	4.200	965	967	971	rVB2	262	157	0.01%	0.001%
15	4.376	1005	1022	1052	rVV	223611	548292	38.72%	4.989%
16	4.553	1075	1077	1082	rVB4	463	371	0.03%	0.003%
17	4.582	1082	1086	1090	rVB3	355	301	0.02%	0.003%
18	4.688	1114	1119	1121	rBV2	193	192	0.01%	0.002%
19	4.733	1130	1133	1137	rVB2	231	154	0.01%	0.001%
20	4.791	1146	1151	1159	rVB2	183	290	0.02%	0.003%
21	4.846	1166	1168	1176	rVB2	169	153	0.01%	0.001%
22	4.952	1197	1201	1204	rBV2	309	262	0.02%	0.002%
23	5.074	1221	1239	1271	rBV2	557681	1415918	100.00%	12.884%
24	5.302	1306	1310	1315	rVB4	250	272	0.02%	0.002%
25	5.383	1333	1335	1341	rVB2	256	187	0.01%	0.002%
26	5.434	1347	1351	1354	rBV	244	222	0.02%	0.002%
27	5.643	1403	1416	1444	rBV	268288	537065	37.93%	4.887%
28	5.939	1493	1508	1543	rBV	599310	1186985	83.83%	10.801%
29	6.093	1543	1556	1590	rVB	313025	633394	44.73%	5.763%
30	6.232	1595	1599	1601	rBV3	550	452	0.03%	0.004%
31	6.289	1615	1617	1620	rVB2	283	187	0.01%	0.002%
32	6.325	1624	1628	1632	rVB	335	270	0.02%	0.002%
33	6.576	1699	1706	1708	rBV2	137	178	0.01%	0.002%
34	7.010	1829	1841	1860	rBV	180212	324338	22.91%	2.951%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092820\
 Data File : VV018490.D
 Acq On : 28 Sep 2020 13:49
 Operator : SY/MD
 Sample : L4117-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 E0AA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	7.177	1890	1893	1901	rVB2	446	338	0.02%	0.003%
36	7.338	1930	1943	1969	rBV	667902	1142265	80.67%	10.394%
37	7.643	2028	2038	2064	rBV	130996	223980	15.82%	2.038%
38	7.891	2111	2115	2118	rBV2	224	163	0.01%	0.001%
39	7.958	2130	2136	2139	rBV2	272	351	0.02%	0.003%
40	8.109	2171	2183	2222	rBV2	317286	608457	42.97%	5.537%
41	8.482	2295	2299	2303	rBV2	234	194	0.01%	0.002%
42	8.505	2303	2306	2311	rVB2	215	148	0.01%	0.001%
43	8.592	2330	2333	2338	rBV3	216	174	0.01%	0.002%
44	8.691	2359	2364	2370	rVB3	221	265	0.02%	0.002%
45	8.875	2409	2421	2451	rBV	410078	663447	46.86%	6.037%
46	9.045	2471	2474	2478	rVB2	336	259	0.02%	0.002%
47	9.170	2510	2513	2517	rVB3	269	225	0.02%	0.002%
48	9.228	2522	2531	2538	rBV3	1358	1838	0.13%	0.017%
49	9.289	2544	2550	2553	rBV	185	226	0.02%	0.002%
50	9.569	2630	2637	2639	rBV2	212	256	0.02%	0.002%
51	9.646	2658	2661	2670	rVB2	122	169	0.01%	0.002%
52	9.736	2682	2689	2693	rVB3	646	660	0.05%	0.006%
53	9.868	2725	2730	2732	rBV2	220	190	0.01%	0.002%
54	10.032	2777	2781	2782	rBV2	274	162	0.01%	0.001%
55	10.109	2799	2805	2809	rBV4	1082	1104	0.08%	0.010%
56	10.141	2811	2815	2821	rVB4	975	985	0.07%	0.009%
57	10.238	2833	2845	2871	rBV	398367	618689	43.70%	5.630%
58	10.344	2875	2878	2884	rVB2	268	256	0.02%	0.002%
59	10.392	2884	2893	2896	rBV3	606	815	0.06%	0.007%
60	10.473	2912	2918	2923	rBV4	1375	1942	0.14%	0.018%
61	10.563	2942	2946	2950	rBV3	757	707	0.05%	0.006%
62	10.601	2950	2958	2971	rVB3	6891	10546	0.74%	0.096%
63	10.765	3004	3009	3015	rVB	270	328	0.02%	0.003%
64	10.794	3015	3018	3020	rBV3	468	268	0.02%	0.002%
65	10.846	3031	3034	3036	rBV2	249	154	0.01%	0.001%
66	10.897	3044	3050	3057	rBV4	1527	1979	0.14%	0.018%
67	10.942	3057	3064	3071	rVB3	2044	2892	0.20%	0.026%
68	11.026	3087	3090	3093	rBV2	195	153	0.01%	0.001%
69	11.048	3094	3097	3100	rVV3	524	425	0.03%	0.004%
70	11.116	3115	3118	3119	rBV	336	169	0.01%	0.002%
71	11.174	3131	3136	3143	rVB3	841	1126	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092820\
 Data File : VV018490.D
 Acq On : 28 Sep 2020 13:49
 Operator : SY/MD
 Sample : L4117-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3188	rBV	432889	666683	47.08%	6.066%
73	11.399	3199	3206	3212	rVB5	1547	2114	0.15%	0.019%
74	11.482	3228	3232	3239	rVB5	1344	1747	0.12%	0.016%
75	11.534	3245	3248	3254	rBV2	180	244	0.02%	0.002%
76	11.588	3263	3265	3268	rBV	432	290	0.02%	0.003%
77	11.646	3269	3283	3305	rVV	699943	1092659	77.17%	9.942%
78	11.810	3324	3334	3342	rBV3	7464	11107	0.78%	0.101%
79	11.903	3360	3363	3366	rBV2	230	176	0.01%	0.002%
80	11.948	3375	3377	3379	rBV2	350	190	0.01%	0.002%
81	11.961	3379	3381	3388	rVB2	858	789	0.06%	0.007%
82	11.993	3388	3391	3392	rBV2	292	149	0.01%	0.001%
83	12.009	3393	3396	3401	rVB4	420	372	0.03%	0.003%
84	12.103	3421	3425	3428	rBV3	356	299	0.02%	0.003%
85	12.196	3451	3454	3457	rBV	195	150	0.01%	0.001%
86	12.267	3474	3476	3484	rVB3	507	567	0.04%	0.005%
87	12.392	3508	3515	3520	rVB4	1035	1263	0.09%	0.011%
88	12.427	3520	3526	3528	rBV3	485	468	0.03%	0.004%
89	12.485	3542	3544	3548	rVV4	597	467	0.03%	0.004%
90	12.524	3551	3556	3562	rVB3	688	767	0.05%	0.007%
91	12.611	3580	3583	3584	rBV3	353	191	0.01%	0.002%
92	12.910	3668	3676	3685	rBV3	3025	4274	0.30%	0.039%
93	13.061	3719	3723	3725	rBV2	692	539	0.04%	0.005%
94	13.141	3745	3748	3753	rBV2	238	174	0.01%	0.002%
95	13.392	3824	3826	3830	rBV2	256	178	0.01%	0.002%
96	13.537	3865	3871	3872	rBV2	587	495	0.03%	0.005%
97	13.653	3902	3907	3913	rBV3	564	754	0.05%	0.007%
98	13.723	3927	3929	3933	rVB	329	168	0.01%	0.002%
99	13.771	3942	3944	3950	rVB2	420	343	0.02%	0.003%
100	13.919	3983	3990	3998	rBV6	1229	1725	0.12%	0.016%


Sum of corrected areas: 10989798

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092820\
Data File : VV018490.D
Acq On : 28 Sep 2020 13:49
Operator : SY/MD
Sample : L4117-06DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

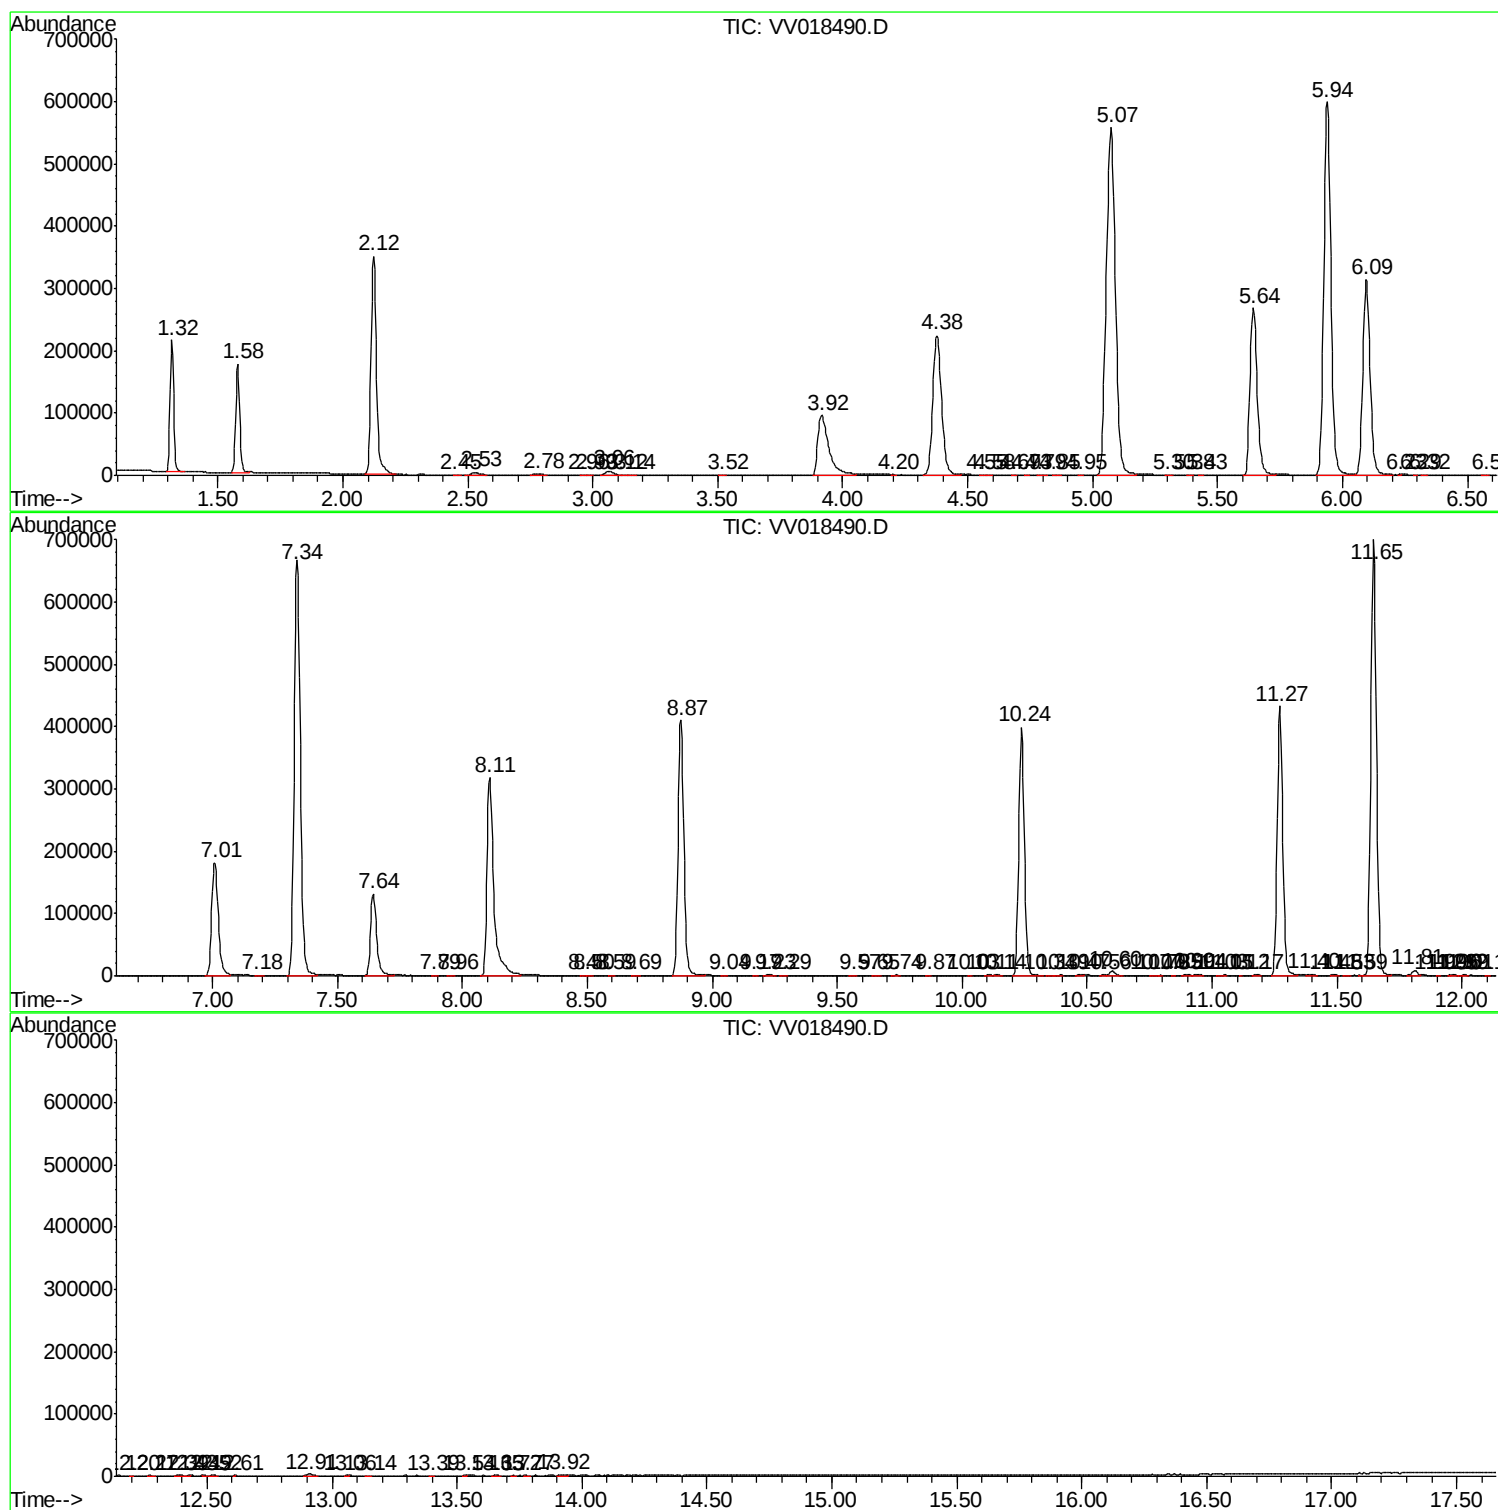

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092820\
Data File : VV018490.D
Acq On : 28 Sep 2020 13:49
Operator : SY/MD
Sample : L4117-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV092820\
Data File : VV018490.D
Acq On : 28 Sep 2020 13:49
Operator : SY/MD
Sample : L4117-06DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc