

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022360.D
 Acq On : 28 Sep 2021 11:03
 Operator : SY/MD
 Sample : VV0928WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 29 01:33:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 29 01:30:11 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	254077	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	242571	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	110751	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	101453	47.051	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	94.100%	
7) Chloroethane-d5	1.561	69	82691	48.486	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	96.980%	
11) 1,1-Dichloroethene-d2	2.105	63	138633	36.979	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	73.960%	
21) 2-Butanone-d5	3.870	46	149118	97.992	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	97.990%	
24) Chloroform-d	4.346	84	185799	47.720	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.440%	
26) 1,2-Dichloroethane-d4	5.027	65	118148	49.483	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.960%	
32) Benzene-d6	5.047	84	385899	50.570	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.140%	
36) 1,2-Dichloropropane-d6	6.066	67	125482	51.399	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	102.800%	
41) Toluene-d8	7.313	98	343728	49.212	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.420%	
43) trans-1,3-Dichloroprop...	7.622	79	52383	46.989	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	93.980%	
47) 2-Hexanone-d5	8.085	63	99723	100.528	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	100.530%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	171039	48.264	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	96.520%	
66) 1,2-Dichlorobenzene-d4	11.625	152	135662	55.087	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	110.180%	
Target Compounds						
44) trans-1,3-Dichloropropene	7.622	75	2588	0.969	ug/L	Qvalue 89
61) 1,2,3-Trichloropropane	11.249	75	12738	6.165	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022360.D
Acq On : 28 Sep 2021 11:03
Operator : SY/MD
Sample : VV0928WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 29 01:33:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 29 01:30:11 2021
Response via : Initial Calibration




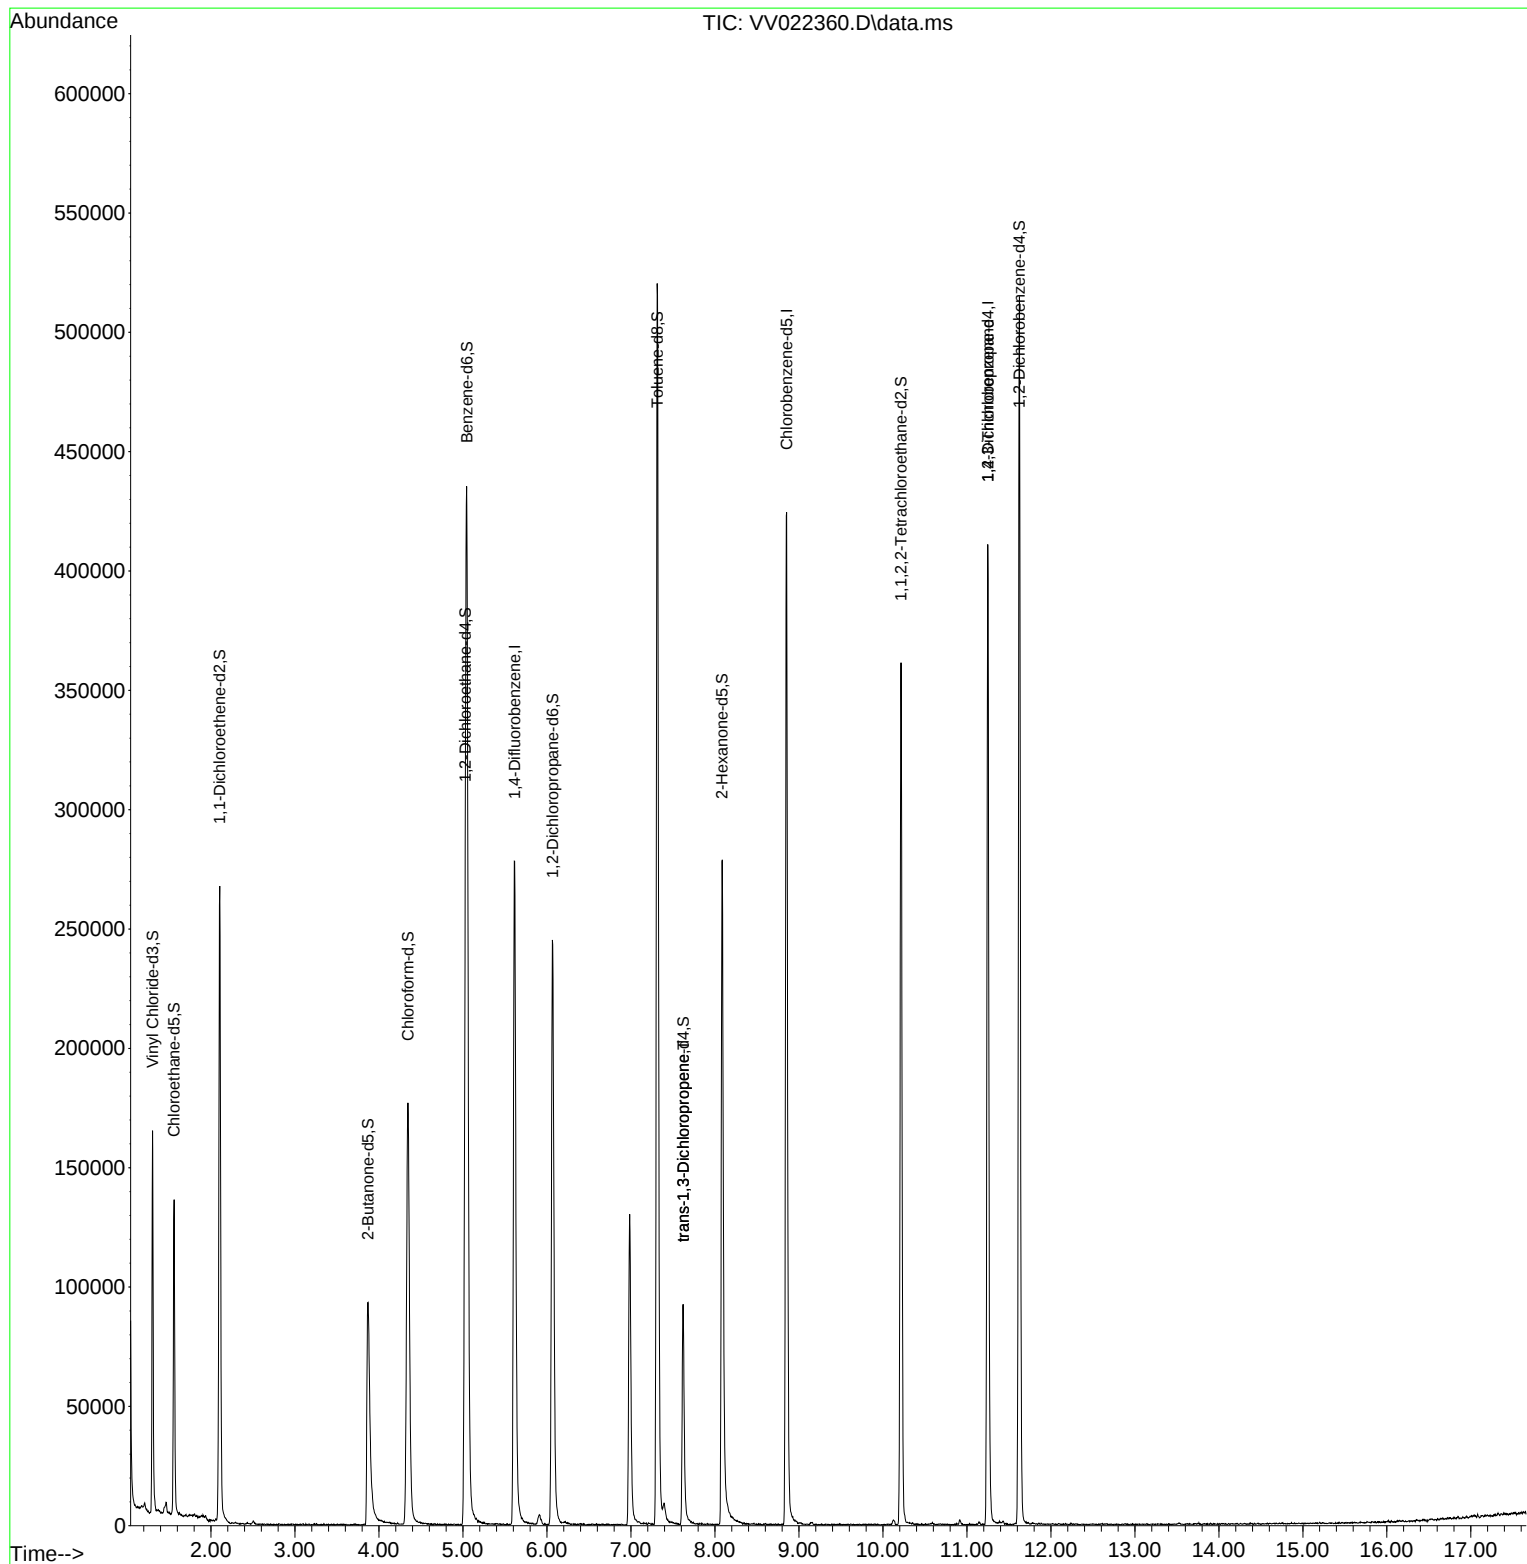


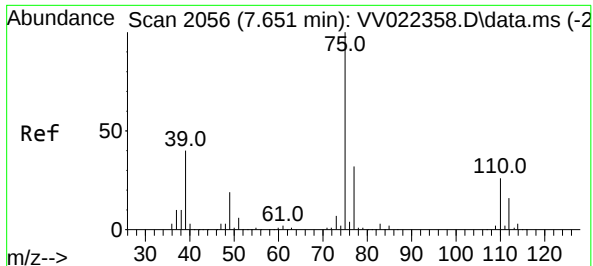

#44
trans-1,3-Dichloropropene
Concen: 0.969 ug/L
RT: 7.622 min Scan# 2047
Delta R.T. -0.029 min
Lab File: VV022360.D
Acq: 28 Sep 2021 11:03

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 2588
Ion Ratio Lower Upper
75 100
77 37.7 22.3 41.3

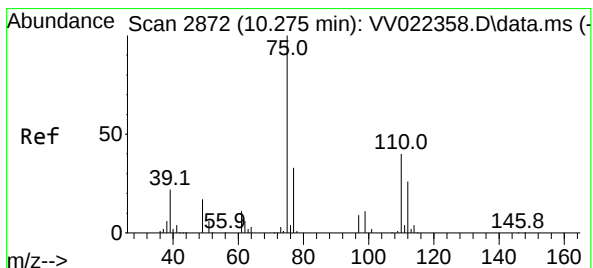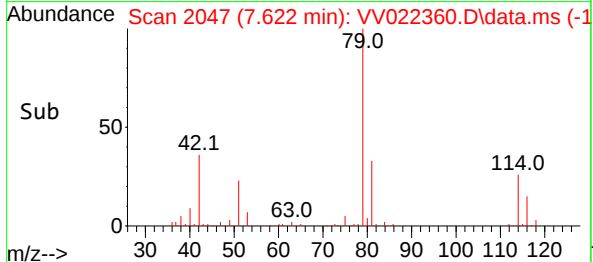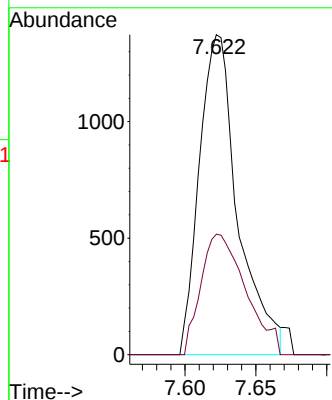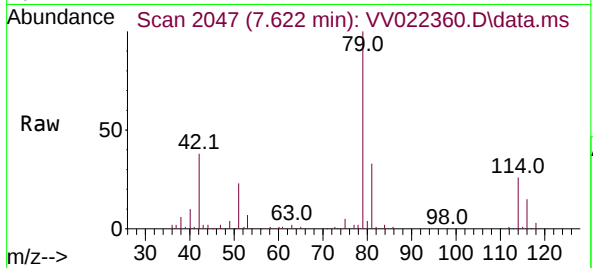

#61
1,2,3-Trichloropropane
Concen: 6.165 ug/L
RT: 11.249 min Scan# 3175
Delta R.T. 0.974 min
Lab File: VV022360.D
Acq: 28 Sep 2021 11:03

Tgt Ion: 75 Resp: 12738
Ion Ratio Lower Upper
75 100
77 28.7 25.4 38.0
110 2.4 32.6 48.8#

