

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Quant Time: Sep 29 01:33:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 29 01:30:11 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/29/2021 5:11:49 PM

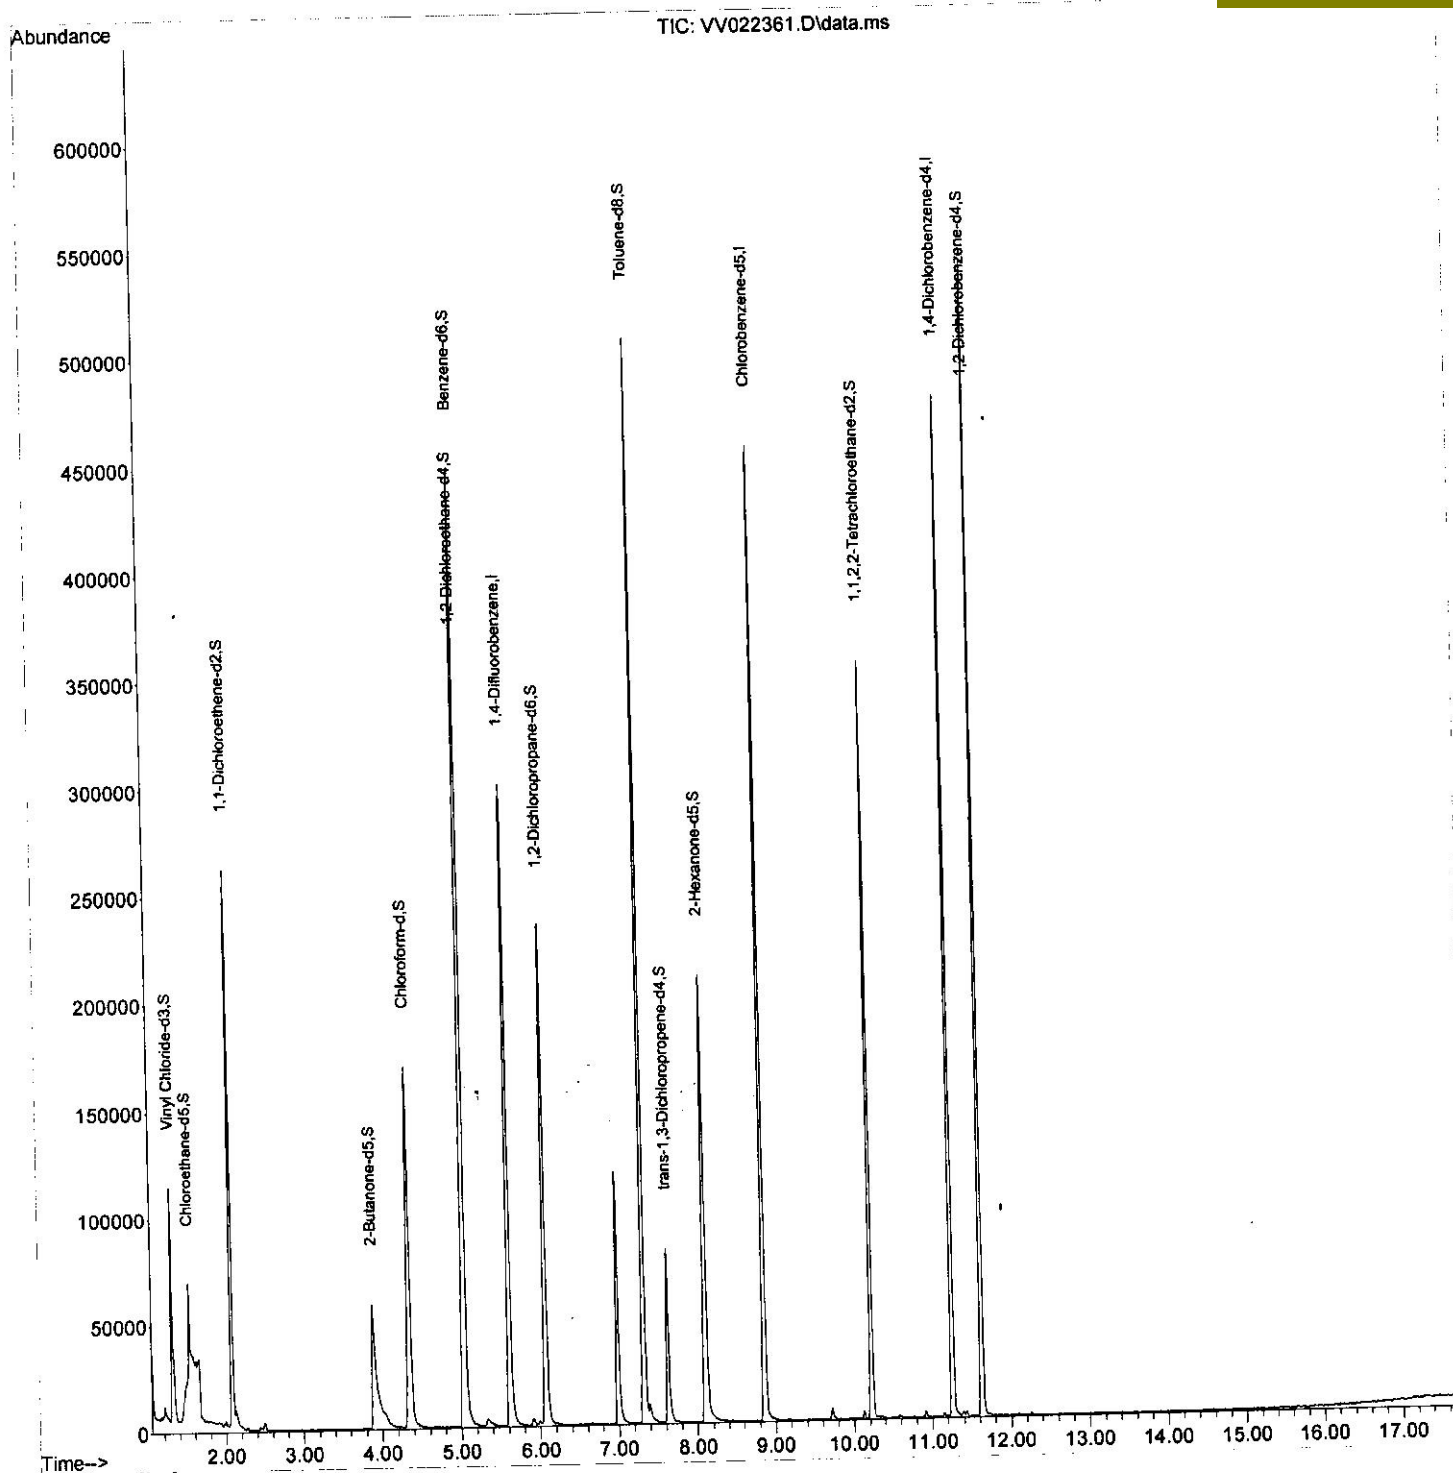

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100UL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Quant Time: Sep 29 01:33:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 29 01:30:11 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/29/2021 5:11:49 PM

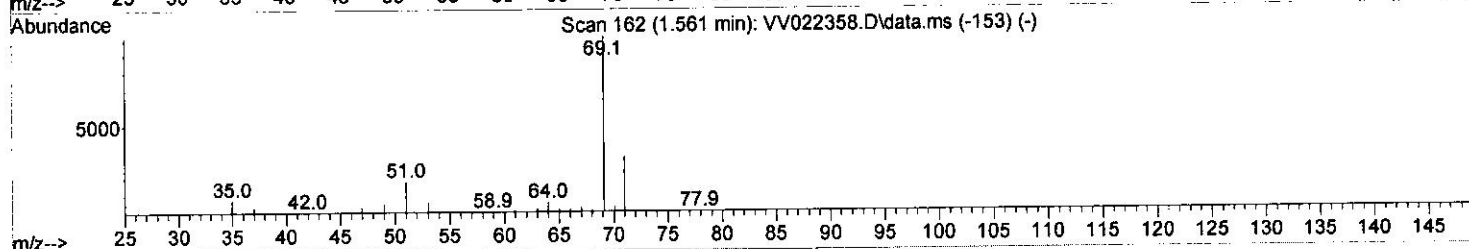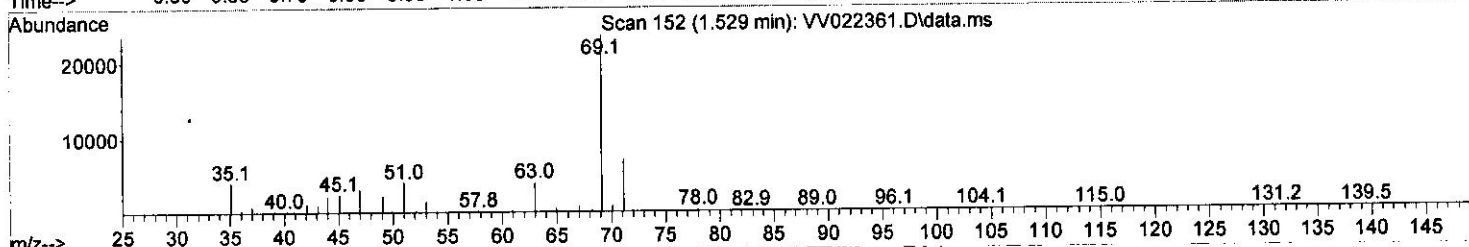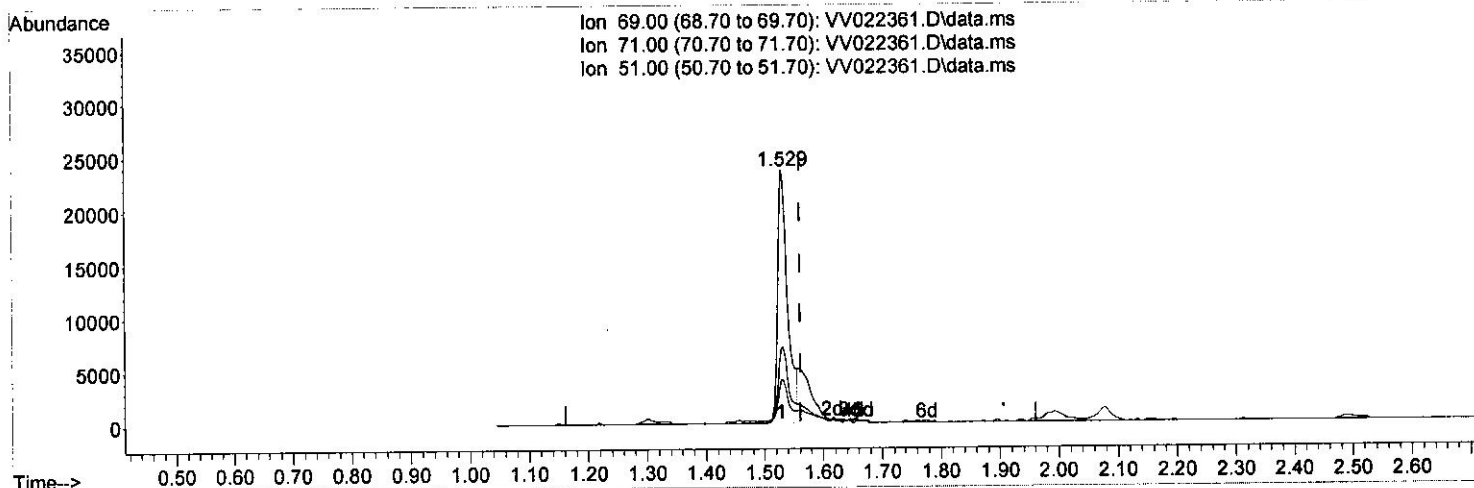

TIC: VV022361.D\data.ms

(7) Chloroethane-d5 (S)

1.529min (-0.032) 14.99 ug/L

response 28098

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	42.30#
51.00	24.90	16.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Manual Integrations
 APPROVED

MMDadoda
 9/29/2021 5:11:49 PM

Quant Time: Sep 29 01:33:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 29 01:30:11 2021
 Response via : Initial Calibration

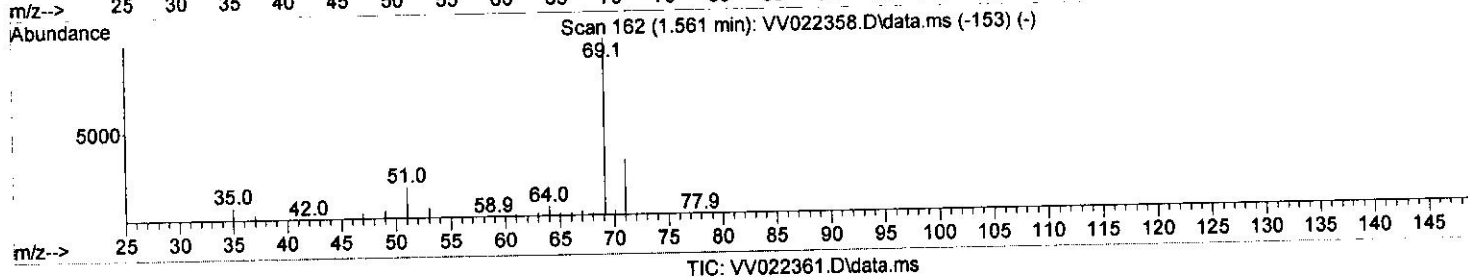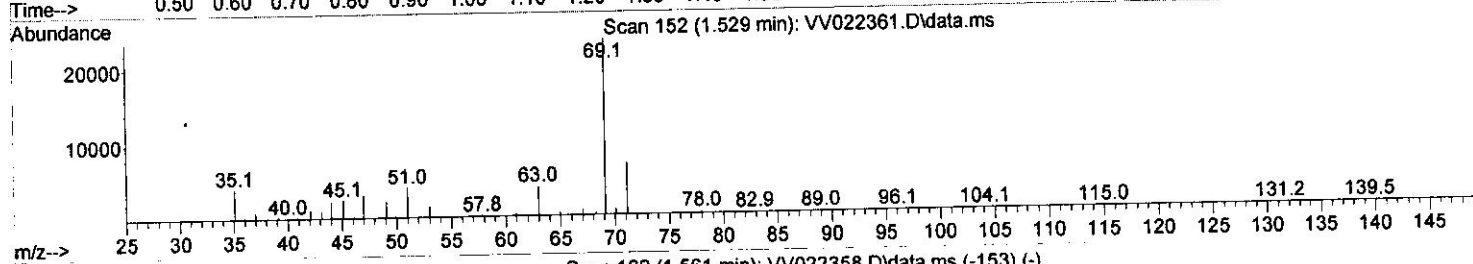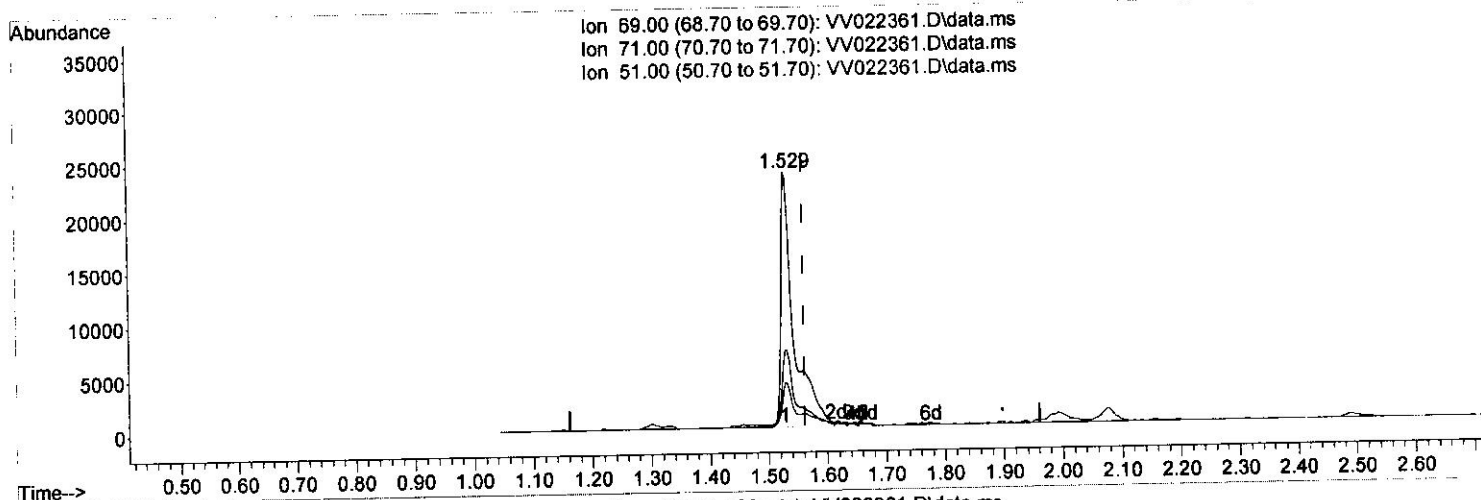

(7) Chloroethane-d5 (S)

1.529min (-0.032) 19.38 ug/L m

response 36330

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.30	32.71
51.00	24.90	13.07#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V092821\
 Data File : V022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Quant Time: Sep 29 01:33:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 29 01:30:11 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/29/2021 5:11:49 PM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	279262	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	267129	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	128604	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	101457	42.809	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	85.620%		
7) Chloroethane-d5	1.529	69	36330m	19.381	ug/L	-0.03
Spiked Amount	50.000	Range 70 - 130	Recovery =	38.760%#		
11) 1,1-Dichloroethene-d2	2.076	63	136117	33.034	ug/L	-0.03
Spiked Amount	50.000	Range 60 - 125	Recovery =	66.060%		
21) 2-Butanone-d5	3.883	46	137679	82.316	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	82.320%		
24) Chloroform-d	4.339	84	184711	43.162	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	86.320%		
26) 1,2-Dichloroethane-d4	5.024	65	119215	45.427	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	90.860%		
32) Benzene-d6	5.037	84	389272	46.322	ug/L	-0.01
Spiked Amount	50.000	Range 70 - 125	Recovery =	92.640%		
36) 1,2-Dichloropropane-d6	6.063	67	122429	45.538	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	91.080%		
41) Toluene-d8	7.313	98	346561	45.056	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	90.120%		
43) trans-1,3-Dichloroprop...	7.622	79	53224	43.354	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	86.700%		
47) 2-Hexanone-d5	8.101	63	104278	95.455	ug/L	0.01
Spiked Amount	100.000	Range 45 - 130	Recovery =	95.460%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	176798	45.302	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	90.600%		
66) 1,2-Dichlorobenzene-d4	11.628	152	146764	51.322	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	102.640%		

m.3
10/1/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed