

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022342.D
 Acq On : 27 Sep 2021 19:22
 Operator : SY/MD
 Sample : VV0928MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rBV	171534	171660	14.71%	2.013%
2	1.561	155	162	177	rVB	132314	157553	13.50%	1.847%
3	2.105	321	331	350	rBV	278249	410636	35.19%	4.814%
4	2.429	429	432	438	rBV4	888	862	0.07%	0.010%
5	2.619	488	491	493	rVB3	571	332	0.03%	0.004%
6	2.648	498	500	503	rBV2	335	254	0.02%	0.003%
7	2.751	530	532	533	rBV2	530	212	0.02%	0.002%
8	2.928	583	587	590	rBV2	311	276	0.02%	0.003%
9	3.118	641	646	650	rVB2	459	442	0.04%	0.005%
10	3.153	650	657	659	rBV2	438	405	0.03%	0.005%
11	3.230	679	681	685	rVB2	588	287	0.02%	0.003%
12	3.256	685	689	693	rBV3	392	353	0.03%	0.004%
13	3.375	724	726	732	rVB2	376	339	0.03%	0.004%
14	3.407	732	736	743	rBV4	583	543	0.05%	0.006%
15	3.474	755	757	761	rBV2	289	244	0.02%	0.003%
16	3.555	778	782	784	rBV2	356	273	0.02%	0.003%
17	3.777	849	851	856	rVB2	364	206	0.02%	0.002%
18	3.876	871	882	923	rBV	97495	273042	23.40%	3.201%
19	4.349	1012	1029	1062	rVV	180961	462840	39.67%	5.426%
20	4.654	1121	1124	1126	rBV3	460	298	0.03%	0.003%
21	4.838	1177	1181	1184	rVB4	344	278	0.02%	0.003%
22	5.047	1228	1246	1275	rBV2	455815	1166871	100.00%	13.680%
23	5.371	1344	1347	1350	rVB2	563	344	0.03%	0.004%
24	5.519	1390	1393	1396	rVB4	691	338	0.03%	0.004%
25	5.535	1396	1398	1403	rVB5	655	482	0.04%	0.006%
26	5.616	1411	1423	1448	rBV	303718	612945	52.53%	7.186%
27	5.915	1510	1516	1524	rVB6	2594	3826	0.33%	0.045%
28	5.986	1533	1538	1543	rVB2	453	488	0.04%	0.006%
29	6.008	1543	1545	1549	rBV3	522	361	0.03%	0.004%
30	6.069	1550	1564	1592	rBV	254317	528884	45.32%	6.201%
31	6.333	1643	1646	1647	rBV	588	301	0.03%	0.004%
32	6.352	1650	1652	1655	rVB2	458	222	0.02%	0.003%
33	6.378	1656	1660	1662	rBV	553	319	0.03%	0.004%
34	6.645	1737	1743	1747	rBV3	687	700	0.06%	0.008%
35	6.699	1758	1760	1762	rBV	569	253	0.02%	0.003%
36	6.789	1783	1788	1795	rVB3	437	406	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022342.D
 Acq On : 27 Sep 2021 19:22
 Operator : SY/MD
 Sample : VV0928MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.889	1816	1819	1822	rVB	326	233	0.02%	0.003%
38	6.989	1838	1850	1879	rBV	133421	248780	21.32%	2.917%
39	7.191	1912	1913	1916	rBV	456	207	0.02%	0.002%
40	7.246	1924	1930	1936	rVB4	782	1010	0.09%	0.012%
41	7.317	1936	1952	1971	rBV	538332	928155	79.54%	10.881%
42	7.622	2037	2047	2066	rBV	94266	164737	14.12%	1.931%
43	7.850	2114	2118	2120	rBV2	571	376	0.03%	0.004%
44	7.928	2139	2142	2143	rBV2	370	216	0.02%	0.003%
45	7.973	2153	2156	2157	rBV2	906	451	0.04%	0.005%
46	8.040	2174	2177	2182	rBV3	413	406	0.03%	0.005%
47	8.088	2182	2192	2221	rBV	312032	547910	46.96%	6.424%
48	8.651	2364	2367	2371	rVB	379	240	0.02%	0.003%
49	8.680	2374	2376	2378	rBV2	381	220	0.02%	0.003%
50	8.735	2386	2393	2395	rBV4	386	342	0.03%	0.004%
51	8.802	2411	2414	2419	rBV3	598	506	0.04%	0.006%
52	8.854	2419	2430	2449	rBV	458661	744126	63.77%	8.724%
53	9.021	2478	2482	2485	rBV2	1153	1097	0.09%	0.013%
54	9.149	2515	2522	2533	rBV5	1445	2567	0.22%	0.030%
55	9.249	2549	2553	2555	rVB3	449	320	0.03%	0.004%
56	9.265	2556	2558	2563	rVV2	428	387	0.03%	0.005%
57	9.284	2563	2564	2570	rVB3	471	313	0.03%	0.004%
58	9.352	2580	2585	2588	rBV3	450	350	0.03%	0.004%
59	9.391	2594	2597	2602	rVB3	537	369	0.03%	0.004%
60	9.490	2624	2628	2634	rBV3	488	312	0.03%	0.004%
61	9.551	2641	2647	2649	rBV2	1237	1152	0.10%	0.014%
62	9.680	2684	2687	2691	rBV3	358	249	0.02%	0.003%
63	9.719	2696	2699	2702	rBV2	317	286	0.02%	0.003%
64	9.895	2749	2754	2756	rBV2	344	292	0.03%	0.003%
65	9.921	2759	2762	2764	rBV2	525	296	0.03%	0.003%
66	10.101	2816	2818	2819	rBV	571	245	0.02%	0.003%
67	10.217	2842	2854	2878	rVV	369602	586859	50.29%	6.880%
68	10.384	2903	2906	2911	rVB5	809	702	0.06%	0.008%
69	10.432	2916	2921	2927	rBV4	355	480	0.04%	0.006%
70	10.461	2927	2930	2932	rVB2	275	193	0.02%	0.002%
71	10.481	2932	2936	2937	rBV	325	203	0.02%	0.002%
72	10.532	2950	2952	2953	rBV	566	223	0.02%	0.003%
73	10.600	2971	2973	2976	rBV3	471	263	0.02%	0.003%
74	10.773	3023	3027	3030	rBV3	423	266	0.02%	0.003%
75	10.789	3030	3032	3037	rVB3	366	314	0.03%	0.004%
76	10.921	3062	3073	3080	rBV9	2617	4794	0.41%	0.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022342.D
 Acq On : 27 Sep 2021 19:22
 Operator : SY/MD
 Sample : VV0928MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.043	3110	3111	3115	rVB	480	199	0.02%	0.002%
78	11.149	3138	3144	3150	rBV5	1282	1545	0.13%	0.018%
79	11.188	3150	3156	3164	rVB5	1795	2613	0.22%	0.031%
80	11.252	3164	3176	3194	rBV	424273	666514	57.12%	7.814%
81	11.542	3263	3266	3271	rBV	457	264	0.02%	0.003%
82	11.625	3280	3292	3314	rBV	508418	804622	68.96%	9.433%
83	11.844	3358	3360	3364	rBV3	425	296	0.03%	0.003%
84	12.484	3555	3559	3563	rBV3	285	297	0.03%	0.003%
85	12.529	3571	3573	3579	rVB3	640	483	0.04%	0.006%
86	12.609	3595	3598	3601	rBV2	304	227	0.02%	0.003%
87	12.622	3601	3602	3605	rVV2	347	214	0.02%	0.003%
88	12.651	3605	3611	3620	rVB6	2978	4089	0.35%	0.048%
89	12.686	3620	3622	3624	rBV2	519	268	0.02%	0.003%
90	12.770	3646	3648	3655	rBV	291	247	0.02%	0.003%
91	12.898	3686	3688	3691	rBV2	407	229	0.02%	0.003%
92	12.989	3713	3716	3720	rBV2	312	239	0.02%	0.003%
93	13.268	3796	3803	3811	rVV9	2458	3478	0.30%	0.041%
94	13.336	3820	3824	3826	rBV2	293	219	0.02%	0.003%
95	13.513	3872	3879	3888	rBV6	2726	3443	0.30%	0.040%
96	13.850	3982	3984	3989	rBV3	287	228	0.02%	0.003%
97	13.873	3989	3991	3996	rVV4	495	385	0.03%	0.005%
98	14.075	4051	4054	4055	rBV2	421	227	0.02%	0.003%
99	14.435	4161	4166	4169	rBV2	565	580	0.05%	0.007%
100	14.580	4209	4211	4213	rBV	511	253	0.02%	0.003%


Sum of corrected areas: 8529681

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022342.D
Acq On : 27 Sep 2021 19:22
Operator : SY/MD
Sample : VV0928MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK260

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

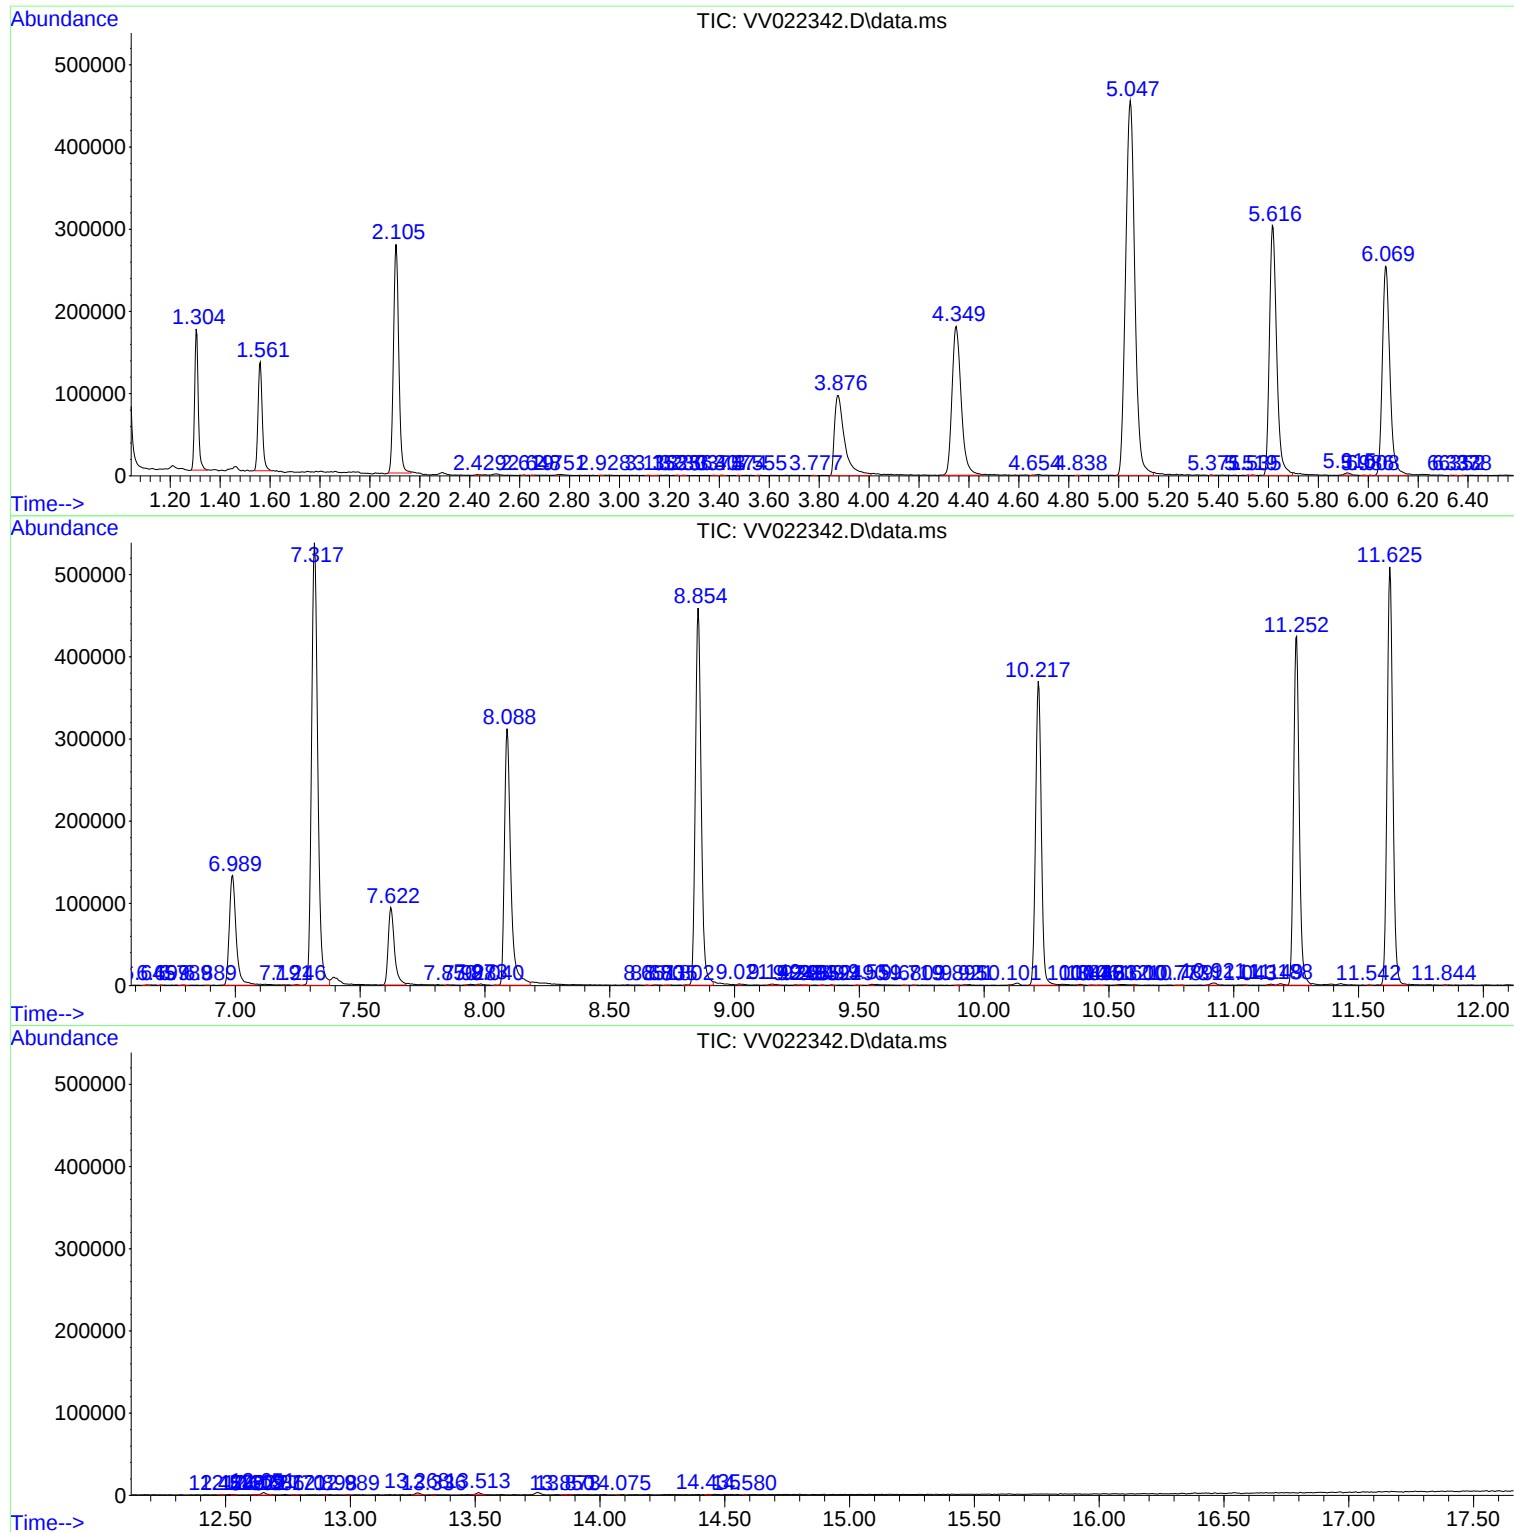

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022342.D
Acq On : 27 Sep 2021 19:22
Operator : SY/MD
Sample : VV0928MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK260

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022342.D
Acq On : 27 Sep 2021 19:22
Operator : SY/MD
Sample : VV0928MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK260

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
