

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022345.D
 Acq On : 27 Sep 2021 20:34
 Operator : SY/MD
 Sample : M3837-06ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7T6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	104	rVB	111036	175730	14.58%	2.014%
2	2.072	312	321	332	rBV	273180	387115	32.12%	4.436%
3	2.490	444	451	465	rVB3	6496	10999	0.91%	0.126%
4	2.732	524	526	528	rBV	616	324	0.03%	0.004%
5	2.751	530	532	535	rVB2	524	222	0.02%	0.003%
6	2.931	585	588	590	rBV2	296	210	0.02%	0.002%
7	3.185	664	667	671	rVB3	396	255	0.02%	0.003%
8	3.278	694	696	701	rVB2	416	164	0.01%	0.002%
9	3.301	701	703	704	rBV2	225	79	0.01%	0.001%
10	3.645	808	810	815	rVB	478	278	0.02%	0.003%
11	3.680	819	821	824	rVB	257	122	0.01%	0.001%
12	3.757	843	845	847	rVB	357	116	0.01%	0.001%
13	3.889	874	886	920	rBV	71124	251179	20.84%	2.878%
14	4.342	1012	1027	1059	rBV	175613	455761	37.81%	5.222%
15	4.641	1119	1120	1122	rBV	292	137	0.01%	0.002%
16	4.719	1142	1144	1146	rBV	450	247	0.02%	0.003%
17	4.789	1164	1166	1167	rBV	265	93	0.01%	0.001%
18	4.834	1176	1180	1183	rBV3	631	488	0.04%	0.006%
19	4.889	1195	1197	1198	rBV	395	207	0.02%	0.002%
20	4.966	1219	1221	1226	rBV2	153	126	0.01%	0.001%
21	5.037	1227	1243	1281	rBV2	479149	1205260	100.00%	13.810%
22	5.612	1410	1422	1452	rBV	309678	651771	54.08%	7.468%
23	5.915	1505	1516	1526	rBV	4192	8120	0.67%	0.093%
24	5.989	1532	1539	1544	rBV6	2453	3549	0.29%	0.041%
25	6.069	1551	1564	1597	rVB	249261	542376	45.00%	6.215%
26	6.358	1651	1654	1656	rBV	494	292	0.02%	0.003%
27	6.432	1675	1677	1679	rBV	336	122	0.01%	0.001%
28	6.477	1688	1691	1693	rBV2	261	137	0.01%	0.002%
29	6.490	1693	1695	1697	rVB2	340	110	0.01%	0.001%
30	6.574	1719	1721	1726	rVB2	440	284	0.02%	0.003%
31	6.596	1726	1728	1730	rBV	417	171	0.01%	0.002%
32	6.619	1731	1735	1737	rBV4	470	357	0.03%	0.004%
33	6.770	1780	1782	1784	rBV3	423	189	0.02%	0.002%
34	6.821	1795	1798	1800	rBV	355	202	0.02%	0.002%
35	6.924	1827	1830	1834	rBV3	668	541	0.04%	0.006%
36	6.985	1837	1849	1874	rBV	124138	247841	20.56%	2.840%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022345.D
 Acq On : 27 Sep 2021 20:34
 Operator : SY/MD
 Sample : M3837-06ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7T6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	7.313	1940	1951	1971	rBV	538529	960980	79.73%	11.011%
38	7.622	2037	2047	2073	rBV	82754	168275	13.96%	1.928%
39	7.972	2154	2156	2158	rBV3	517	209	0.02%	0.002%
40	8.008	2164	2167	2170	rBV2	289	159	0.01%	0.002%
41	8.101	2184	2196	2244	rBV2	215296	583875	48.44%	6.690%
42	8.606	2351	2353	2356	rBV2	217	120	0.01%	0.001%
43	8.718	2387	2388	2390	rBV2	347	167	0.01%	0.002%
44	8.783	2405	2408	2409	rBV2	252	128	0.01%	0.001%
45	8.853	2419	2430	2454	rBV	455207	787096	65.31%	9.019%
46	9.085	2497	2502	2505	rBV2	355	285	0.02%	0.003%
47	9.107	2505	2509	2512	rBV4	522	496	0.04%	0.006%
48	9.133	2513	2517	2518	rBV2	753	524	0.04%	0.006%
49	9.249	2551	2553	2557	rBV3	330	254	0.02%	0.003%
50	9.329	2575	2578	2580	rBV	200	117	0.01%	0.001%
51	9.378	2591	2593	2594	rBV	289	118	0.01%	0.001%
52	9.458	2616	2618	2622	rBV2	254	188	0.02%	0.002%
53	9.493	2627	2629	2632	rVB	300	145	0.01%	0.002%
54	9.513	2632	2635	2636	rBV2	352	215	0.02%	0.002%
55	9.538	2639	2643	2645	rBV3	553	357	0.03%	0.004%
56	9.554	2645	2648	2652	rBV3	902	674	0.06%	0.008%
57	9.632	2670	2672	2673	rBV	339	136	0.01%	0.002%
58	9.802	2719	2725	2726	rBV	548	447	0.04%	0.005%
59	9.860	2741	2743	2748	rBV	305	231	0.02%	0.003%
60	9.886	2748	2751	2752	rBV	313	174	0.01%	0.002%
61	9.927	2762	2764	2767	rBV3	569	360	0.03%	0.004%
62	9.963	2773	2775	2777	rBV	354	110	0.01%	0.001%
63	10.040	2796	2799	2801	rBV2	388	203	0.02%	0.002%
64	10.056	2801	2804	2806	rVB	385	191	0.02%	0.002%
65	10.101	2815	2818	2819	rBV	349	165	0.01%	0.002%
66	10.130	2819	2827	2837	rVB4	4168	6278	0.52%	0.072%
67	10.223	2843	2856	2877	rBV	364181	616618	51.16%	7.066%
68	10.497	2938	2941	2942	rBV	308	151	0.01%	0.002%
69	10.670	2992	2995	2997	rVB2	630	314	0.03%	0.004%
70	10.696	3001	3003	3005	rBV2	328	199	0.02%	0.002%
71	10.744	3013	3018	3025	rBV2	462	561	0.05%	0.006%
72	10.779	3025	3029	3032	rBV2	245	257	0.02%	0.003%
73	10.802	3032	3036	3039	rBV2	692	426	0.04%	0.005%
74	10.879	3058	3060	3063	rVB3	643	317	0.03%	0.004%
75	10.918	3063	3072	3080	rBV5	4412	7151	0.59%	0.082%
76	11.030	3104	3107	3109	rBV4	591	477	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022345.D
 Acq On : 27 Sep 2021 20:34
 Operator : SY/MD
 Sample : M3837-06ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7T6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.066	3116	3118	3120	rBV2	403	229	0.02%	0.003%
78	11.091	3124	3126	3128	rVB	444	150	0.01%	0.002%
79	11.146	3136	3143	3152	rBV7	2148	2878	0.24%	0.033%
80	11.191	3154	3157	3161	rBV2	932	730	0.06%	0.008%
81	11.252	3165	3176	3196	rBV	479922	747564	62.03%	8.566%
82	11.471	3242	3244	3247	rBV2	544	355	0.03%	0.004%
83	11.628	3281	3293	3318	rBV	562406	884218	73.36%	10.132%
84	11.786	3337	3342	3351	rVB5	2204	3044	0.25%	0.035%
85	11.972	3398	3400	3401	rBV5	331	117	0.01%	0.001%
86	12.271	3491	3493	3499	rVB4	545	359	0.03%	0.004%
87	12.422	3537	3540	3541	rBV	498	326	0.03%	0.004%
88	12.487	3558	3560	3562	rBV	405	216	0.02%	0.002%
89	12.541	3575	3577	3581	rBV2	405	228	0.02%	0.003%
90	12.586	3587	3591	3592	rBV2	551	401	0.03%	0.005%
91	12.715	3628	3631	3634	rBV2	470	271	0.02%	0.003%
92	12.828	3662	3666	3669	rVB3	355	290	0.02%	0.003%
93	12.847	3669	3672	3674	rBV	401	226	0.02%	0.003%
94	12.873	3678	3680	3681	rBV	353	187	0.02%	0.002%
95	12.934	3697	3699	3700	rBV	274	114	0.01%	0.001%
96	12.969	3708	3710	3711	rBV	229	84	0.01%	0.001%
97	13.207	3781	3784	3787	rBV2	350	239	0.02%	0.003%
98	13.332	3821	3823	3826	rBV	310	185	0.02%	0.002%
99	13.471	3864	3866	3867	rBV	376	120	0.01%	0.001%
100	13.750	3949	3953	3955	rBV4	475	307	0.03%	0.004%




Sum of corrected areas: 8727160

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022345.D
Acq On : 27 Sep 2021 20:34
Operator : SY/MD
Sample : M3837-06ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7T6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

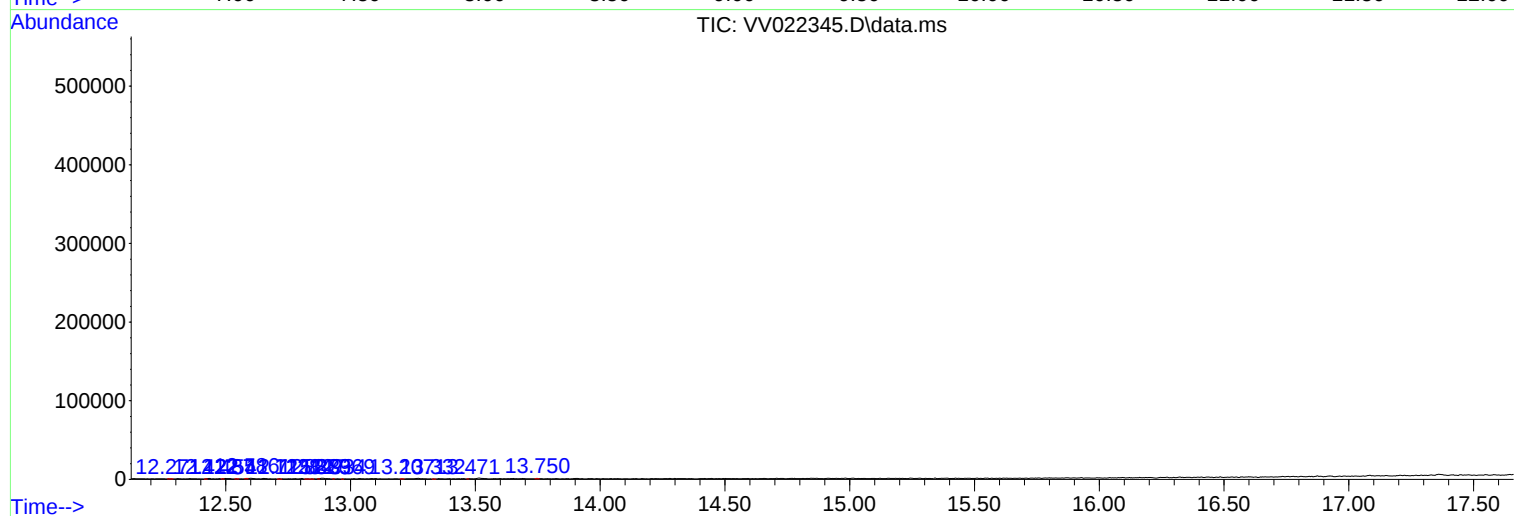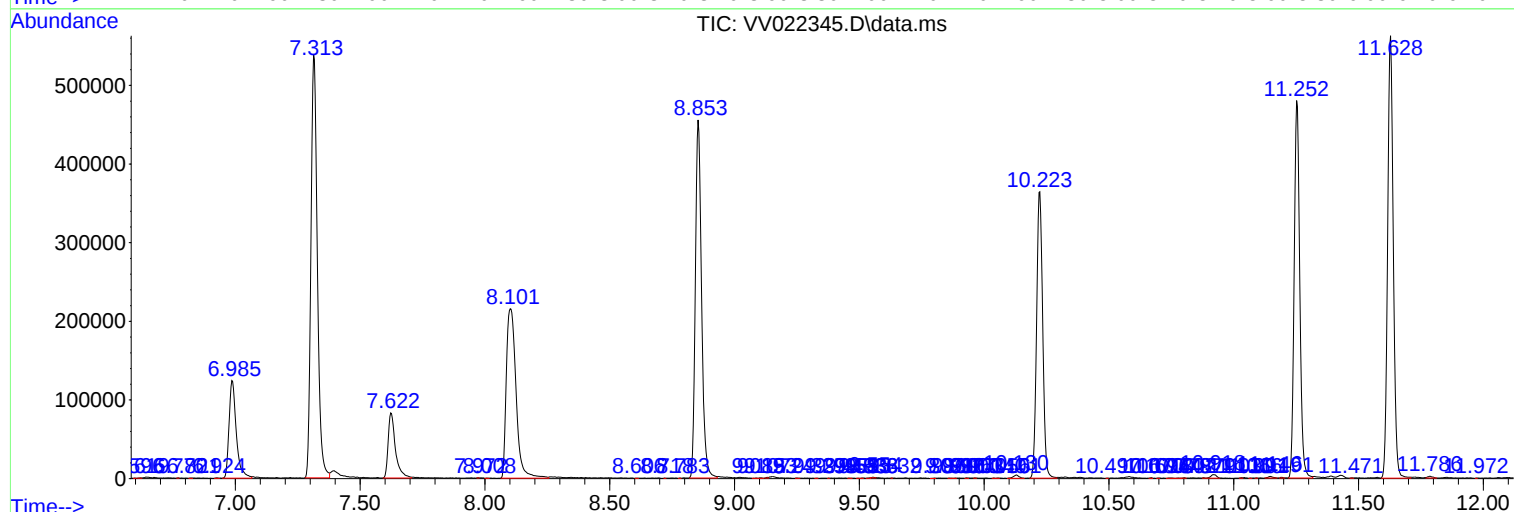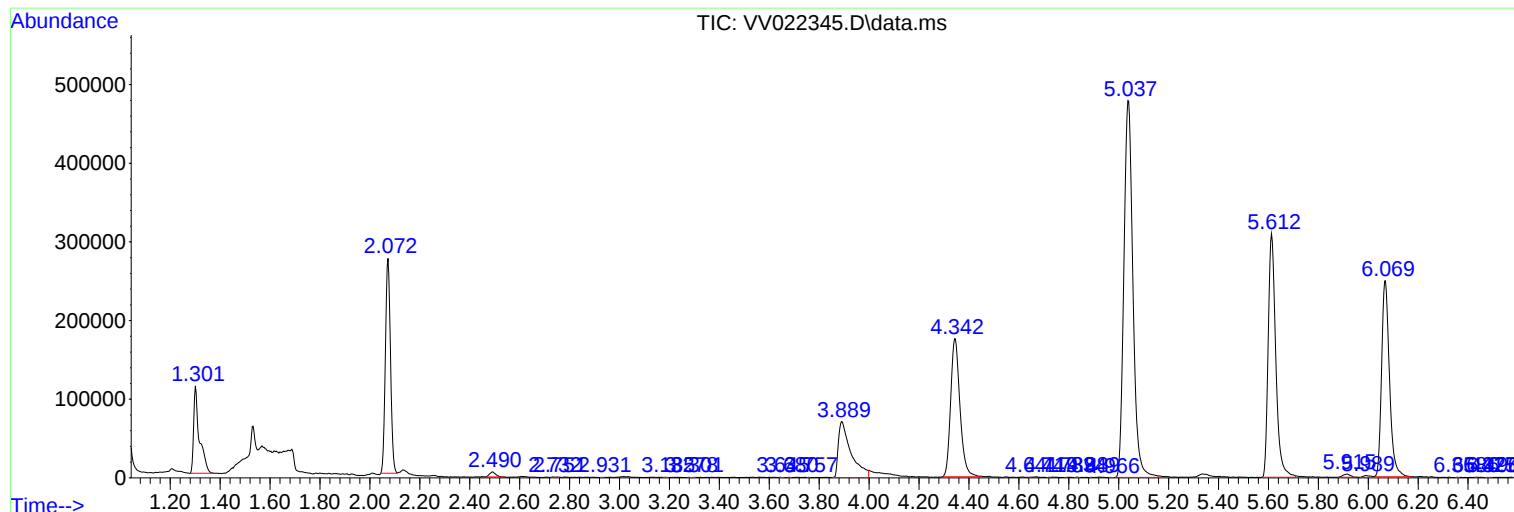

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022345.D
Acq On : 27 Sep 2021 20:34
Operator : SY/MD
Sample : M3837-06ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7T6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022345.D
Acq On : 27 Sep 2021 20:34
Operator : SY/MD
Sample : M3837-06ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7T6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc