

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022348.D
 Acq On : 27 Sep 2021 21:47
 Operator : SY/MD
 Sample : M3834-05ME
 Misc : 4.58g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW406ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	123404	172831	14.50%	1.987%
2	2.076	312	322	334	rBV	270752	390408	32.76%	4.489%
3	2.368	410	413	415	rBV2	651	430	0.04%	0.005%
4	2.378	415	416	421	rVV4	415	312	0.03%	0.004%
5	2.609	484	488	490	rBV3	664	497	0.04%	0.006%
6	2.661	503	504	507	rBV2	284	182	0.02%	0.002%
7	2.738	525	528	530	rBV2	594	350	0.03%	0.004%
8	2.796	542	546	548	rVB2	578	336	0.03%	0.004%
9	3.037	619	621	625	rBV	480	355	0.03%	0.004%
10	3.198	669	671	675	rVB	351	179	0.02%	0.002%
11	3.259	688	690	693	rVB	302	168	0.01%	0.002%
12	3.281	693	697	699	rBV2	359	280	0.02%	0.003%
13	3.349	715	718	720	rVV2	522	271	0.02%	0.003%
14	3.490	760	762	764	rBV2	396	198	0.02%	0.002%
15	3.551	778	781	784	rBV2	365	239	0.02%	0.003%
16	3.632	804	806	810	rBV3	272	183	0.02%	0.002%
17	3.731	834	837	840	rBV2	352	230	0.02%	0.003%
18	3.793	853	856	859	rBV2	243	175	0.01%	0.002%
19	3.889	875	886	927	rBV	70052	261576	21.95%	3.008%
20	4.217	985	988	993	rVB4	574	522	0.04%	0.006%
21	4.342	1010	1027	1053	rBV2	176205	458608	38.48%	5.273%
22	4.622	1111	1114	1115	rBV2	304	174	0.01%	0.002%
23	4.664	1124	1127	1130	rBV4	504	311	0.03%	0.004%
24	4.841	1177	1182	1183	rVB2	339	220	0.02%	0.003%
25	4.857	1183	1187	1188	rBV	390	230	0.02%	0.003%
26	4.879	1192	1194	1197	rBV3	392	223	0.02%	0.003%
27	5.037	1227	1243	1278	rBV2	477605	1191830	100.00%	13.704%
28	5.333	1325	1335	1340	rBV8	4092	7413	0.62%	0.085%
29	5.474	1377	1379	1381	rBV3	568	188	0.02%	0.002%
30	5.551	1401	1403	1406	rVB2	439	169	0.01%	0.002%
31	5.612	1410	1422	1445	rBV	312074	646262	54.22%	7.431%
32	5.911	1505	1515	1527	rVB8	3756	8080	0.68%	0.093%
33	6.069	1550	1564	1591	rBV	244995	532031	44.64%	6.117%
34	6.288	1630	1632	1639	rVB4	723	613	0.05%	0.007%
35	6.326	1639	1644	1648	rBV3	410	425	0.04%	0.005%
36	6.346	1648	1650	1655	rVB2	298	199	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022348.D
 Acq On : 27 Sep 2021 21:47
 Operator : SY/MD
 Sample : M3834-05ME
 Misc : 4.58g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW406ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.413	1669	1671	1675	rBV	345	230	0.02%	0.003%
38	6.448	1681	1682	1685	rVV	523	341	0.03%	0.004%
39	6.497	1694	1697	1699	rVB2	483	291	0.02%	0.003%
40	6.702	1759	1761	1762	rBV2	506	261	0.02%	0.003%
41	6.764	1776	1780	1781	rBV2	314	199	0.02%	0.002%
42	6.937	1831	1834	1836	rBV	359	212	0.02%	0.002%
43	6.985	1838	1849	1873	rBV	122154	241720	20.28%	2.779%
44	7.162	1902	1904	1907	rBV3	366	181	0.02%	0.002%
45	7.313	1939	1951	1971	rBV	530903	955048	80.13%	10.981%
46	7.622	2037	2047	2080	rBV	85478	168055	14.10%	1.932%
47	7.992	2159	2162	2164	rBV3	325	249	0.02%	0.003%
48	8.008	2164	2167	2171	rVB2	505	385	0.03%	0.004%
49	8.101	2184	2196	2227	rBV2	241840	575381	48.28%	6.616%
50	8.439	2299	2301	2303	rBV	580	295	0.02%	0.003%
51	8.686	2376	2378	2380	rBV2	493	235	0.02%	0.003%
52	8.734	2390	2393	2397	rVB3	370	188	0.02%	0.002%
53	8.853	2418	2430	2457	rBV	458124	786704	66.01%	9.046%
54	9.111	2508	2510	2512	rBV2	400	260	0.02%	0.003%
55	9.149	2518	2522	2524	rBV2	589	487	0.04%	0.006%
56	9.217	2539	2543	2546	rBV2	382	312	0.03%	0.004%
57	9.275	2560	2561	2564	rBV2	286	172	0.01%	0.002%
58	9.352	2581	2585	2588	rVV3	423	323	0.03%	0.004%
59	9.397	2596	2599	2602	rVB	442	204	0.02%	0.002%
60	9.596	2656	2661	2664	rBV4	619	536	0.04%	0.006%
61	9.632	2669	2672	2674	rBV	560	276	0.02%	0.003%
62	9.664	2679	2682	2684	rBV	362	182	0.02%	0.002%
63	9.805	2724	2726	2730	rVV3	387	245	0.02%	0.003%
64	9.828	2730	2733	2735	rVV2	441	208	0.02%	0.002%
65	9.860	2738	2743	2747	rVV2	455	386	0.03%	0.004%
66	9.947	2768	2770	2772	rVB	460	188	0.02%	0.002%
67	10.130	2819	2827	2837	rVB3	4443	6769	0.57%	0.078%
68	10.223	2843	2856	2873	rBV	370923	615882	51.68%	7.081%
69	10.426	2915	2919	2920	rBV	328	177	0.01%	0.002%
70	10.477	2932	2935	2936	rBV	382	207	0.02%	0.002%
71	10.538	2948	2954	2955	rBV3	354	261	0.02%	0.003%
72	10.580	2958	2967	2971	rBV4	1496	2135	0.18%	0.025%
73	10.657	2989	2991	2994	rVB2	582	369	0.03%	0.004%
74	10.921	3067	3073	3080	rVB5	3511	4769	0.40%	0.055%
75	10.972	3087	3089	3092	rBV3	562	400	0.03%	0.005%
76	11.082	3119	3123	3128	rVB2	391	435	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022348.D
 Acq On : 27 Sep 2021 21:47
 Operator : SY/MD
 Sample : M3834-05ME
 Misc : 4.58g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW406ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.104	3128	3130	3134	rVB2	327	247	0.02%	0.003%
78	11.146	3134	3143	3154	rBV6	2756	4800	0.40%	0.055%
79	11.252	3165	3176	3194	rBV	485067	755180	63.36%	8.683%
80	11.381	3212	3216	3217	rBV4	1530	1231	0.10%	0.014%
81	11.541	3261	3266	3268	rBV3	637	640	0.05%	0.007%
82	11.628	3281	3293	3310	rBV	555712	887334	74.45%	10.203%
83	11.844	3354	3360	3362	rBV3	902	870	0.07%	0.010%
84	12.303	3499	3503	3504	rBV3	410	299	0.03%	0.003%
85	12.426	3536	3541	3544	rBV2	559	470	0.04%	0.005%
86	12.490	3558	3561	3566	rVB4	841	596	0.05%	0.007%
87	12.516	3567	3569	3571	rBV2	331	206	0.02%	0.002%
88	12.590	3590	3592	3593	rBV	567	265	0.02%	0.003%
89	12.651	3607	3611	3614	rBV2	475	411	0.03%	0.005%
90	12.747	3638	3641	3643	rBV	305	212	0.02%	0.002%
91	12.908	3688	3691	3693	rBV2	464	231	0.02%	0.003%
92	13.040	3728	3732	3735	rVB2	415	349	0.03%	0.004%
93	13.062	3735	3739	3744	rBV2	493	336	0.03%	0.004%
94	13.127	3757	3759	3761	rVV	401	234	0.02%	0.003%
95	13.143	3762	3764	3767	rVB2	527	233	0.02%	0.003%
96	13.268	3801	3803	3808	rBV4	455	360	0.03%	0.004%
97	13.676	3928	3930	3933	rVB	380	204	0.02%	0.002%
98	13.969	4019	4021	4022	rBV	361	172	0.01%	0.002%
99	14.037	4041	4042	4045	rBV	392	232	0.02%	0.003%
100	14.201	4091	4093	4095	rBV2	378	209	0.02%	0.002%




Sum of corrected areas: 8697177

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022348.D
Acq On : 27 Sep 2021 21:47
Operator : SY/MD
Sample : M3834-05ME
Misc : 4.58g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW406ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

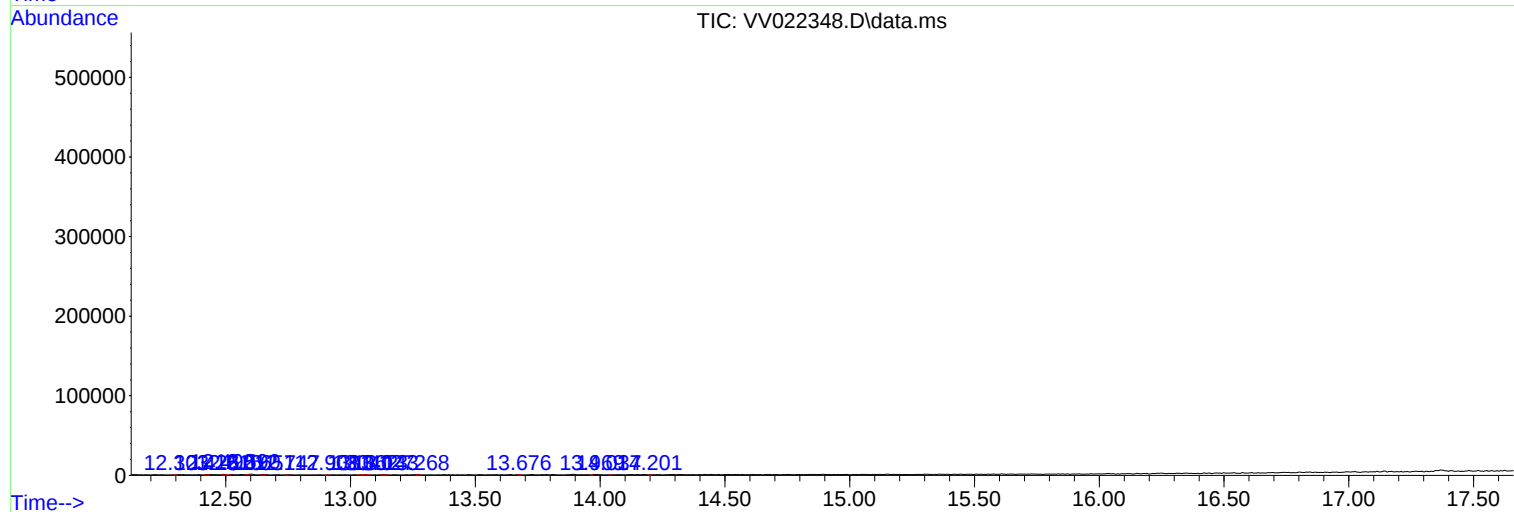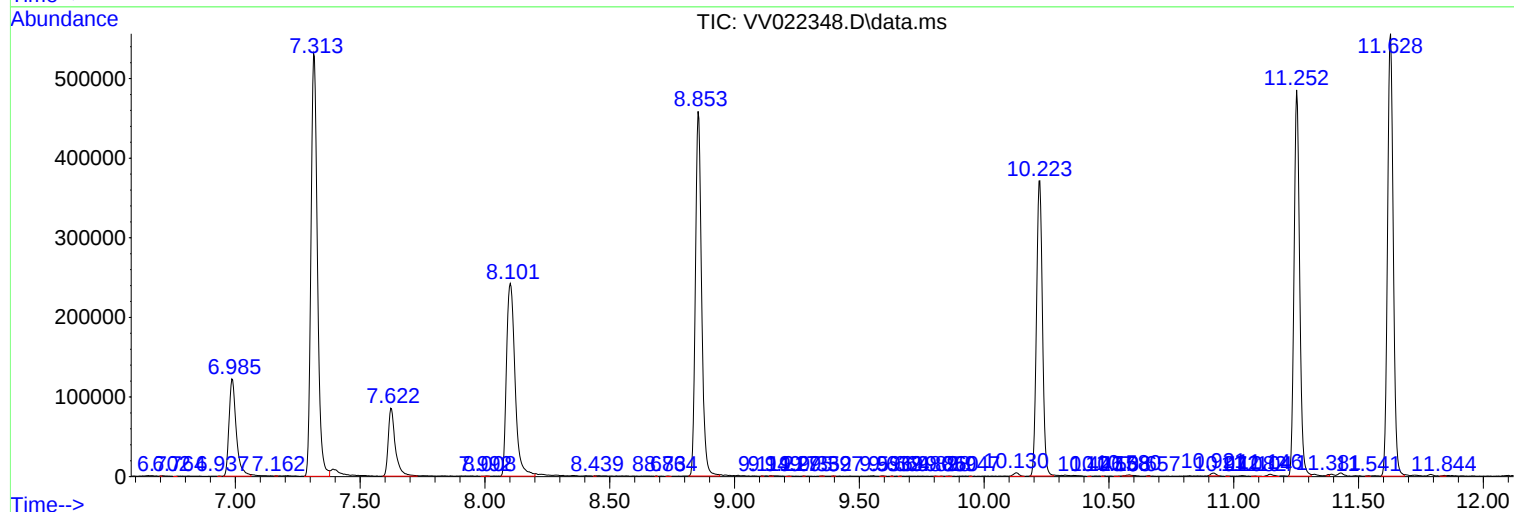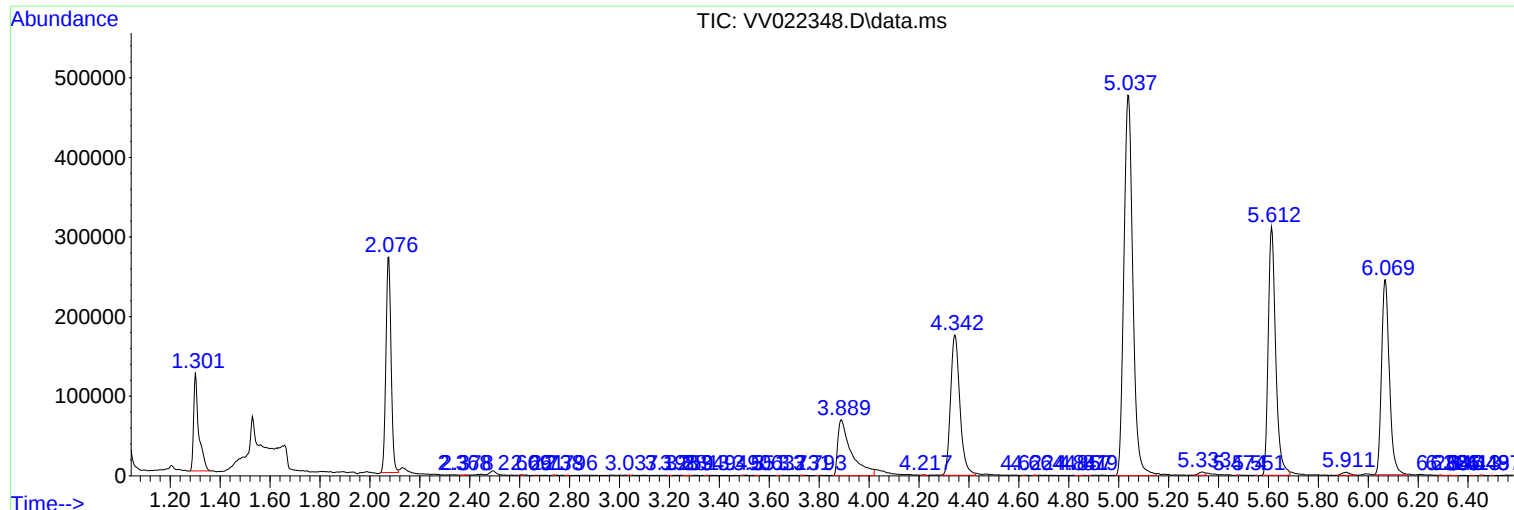

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022348.D
Acq On : 27 Sep 2021 21:47
Operator : SY/MD
Sample : M3834-05ME
Misc : 4.58g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW406ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022348.D
Acq On : 27 Sep 2021 21:47
Operator : SY/MD
Sample : M3834-05ME
Misc : 4.58g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW406ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc