

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022360.D
 Acq On : 28 Sep 2021 11:03
 Operator : SY/MD
 Sample : VV0928WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	159370	160857	14.32%	1.971%
2	1.561	155	162	178	rVB	131890	152214	13.55%	1.865%
3	2.105	321	331	364	rVB	266653	401491	35.75%	4.919%
4	2.571	473	476	479	rBV3	349	252	0.02%	0.003%
5	2.638	492	497	500	rBV	377	383	0.03%	0.005%
6	2.709	515	519	525	rBV3	415	408	0.04%	0.005%
7	2.806	546	549	550	rBV	378	184	0.02%	0.002%
8	2.960	595	597	601	rBV2	383	300	0.03%	0.004%
9	3.230	678	681	684	rBV3	427	234	0.02%	0.003%
10	3.256	687	689	693	rVB2	560	292	0.03%	0.004%
11	3.346	715	717	722	rVB	470	243	0.02%	0.003%
12	3.436	742	745	747	rVV2	328	225	0.02%	0.003%
13	3.462	751	753	755	rBV2	407	210	0.02%	0.003%
14	3.503	764	766	772	rVB2	405	276	0.02%	0.003%
15	3.574	785	788	791	rBV2	447	185	0.02%	0.002%
16	3.870	870	880	919	rBV	93103	250293	22.29%	3.067%
17	4.153	966	968	972	rBV3	433	258	0.02%	0.003%
18	4.346	1012	1028	1055	rBV	176323	437936	38.99%	5.366%
19	4.629	1114	1116	1120	rVB2	533	367	0.03%	0.004%
20	4.648	1120	1122	1123	rBV2	447	203	0.02%	0.002%
21	4.696	1134	1137	1139	rBV3	419	201	0.02%	0.002%
22	4.828	1176	1178	1182	rBV2	365	223	0.02%	0.003%
23	5.043	1226	1245	1271	rBV2	435183	1123128	100.00%	13.761%
24	5.249	1305	1309	1311	rBV3	623	363	0.03%	0.004%
25	5.439	1365	1368	1372	rVB4	465	370	0.03%	0.005%
26	5.461	1372	1375	1378	rBV	289	210	0.02%	0.003%
27	5.526	1391	1395	1400	rVB4	469	484	0.04%	0.006%
28	5.555	1400	1404	1406	rBV2	331	253	0.02%	0.003%
29	5.613	1410	1422	1448	rBV	277702	571691	50.90%	7.004%
30	5.908	1505	1514	1520	rBV9	3686	7098	0.63%	0.087%
31	5.976	1532	1535	1537	rBV2	686	399	0.04%	0.005%
32	6.066	1549	1563	1596	rBV	245028	512205	45.61%	6.276%
33	6.439	1677	1679	1688	rVB2	640	429	0.04%	0.005%
34	6.529	1705	1707	1709	rBV	380	192	0.02%	0.002%
35	6.584	1720	1724	1725	rBV2	405	222	0.02%	0.003%
36	6.834	1799	1802	1806	rVB2	384	316	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022360.D
 Acq On : 28 Sep 2021 11:03
 Operator : SY/MD
 Sample : VV0928WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.857	1806	1809	1814	rBV3	254	239	0.02%	0.003%
38	6.889	1814	1819	1828	rBV4	352	510	0.05%	0.006%
39	6.986	1838	1849	1871	rBV	130222	242589	21.60%	2.972%
40	7.207	1915	1918	1920	rBV3	581	341	0.03%	0.004%
41	7.252	1929	1932	1935	rBV3	463	231	0.02%	0.003%
42	7.313	1939	1951	1969	rBV	519990	894717	79.66%	10.962%
43	7.622	2037	2047	2074	rBV	92274	165389	14.73%	2.026%
44	7.812	2103	2106	2109	rBV2	570	297	0.03%	0.004%
45	8.088	2182	2192	2225	rBV	278262	505161	44.98%	6.189%
46	8.580	2341	2345	2347	rBV2	444	285	0.03%	0.003%
47	8.654	2365	2368	2369	rBV	416	199	0.02%	0.002%
48	8.719	2386	2388	2393	rVB3	484	414	0.04%	0.005%
49	8.854	2418	2430	2459	rBV	424027	703104	62.60%	8.615%
50	9.137	2514	2518	2519	rBV	746	438	0.04%	0.005%
51	9.204	2537	2539	2544	rVB2	415	280	0.02%	0.003%
52	9.230	2544	2547	2551	rBV	207	192	0.02%	0.002%
53	9.391	2595	2597	2602	rVB2	436	332	0.03%	0.004%
54	9.416	2602	2605	2606	rBV2	347	196	0.02%	0.002%
55	9.484	2625	2626	2629	rVB	445	213	0.02%	0.003%
56	9.526	2638	2639	2645	rBV2	259	203	0.02%	0.002%
57	9.616	2665	2667	2675	rVB3	364	357	0.03%	0.004%
58	9.648	2675	2677	2680	rVB2	339	188	0.02%	0.002%
59	9.719	2696	2699	2706	rVB3	417	397	0.04%	0.005%
60	9.899	2751	2755	2758	rBV	324	259	0.02%	0.003%
61	10.124	2819	2825	2835	rVB5	1972	3268	0.29%	0.040%
62	10.217	2840	2854	2873	rBV	361175	563687	50.19%	6.906%
63	10.352	2894	2896	2900	rVB2	596	338	0.03%	0.004%
64	10.509	2941	2945	2948	rVB	348	242	0.02%	0.003%
65	10.664	2990	2993	2996	rBV3	305	236	0.02%	0.003%
66	10.857	3048	3053	3056	rBV2	403	319	0.03%	0.004%
67	10.915	3066	3071	3079	rBV6	1881	2297	0.20%	0.028%
68	11.034	3106	3108	3112	rVB	567	306	0.03%	0.004%
69	11.143	3137	3142	3150	rVB5	1171	1491	0.13%	0.018%
70	11.181	3150	3154	3156	rBV	222	187	0.02%	0.002%
71	11.249	3163	3175	3194	rBV	410663	637852	56.79%	7.815%
72	11.461	3237	3241	3243	rBV2	495	352	0.03%	0.004%
73	11.480	3245	3247	3252	rVB2	447	236	0.02%	0.003%
74	11.625	3280	3292	3312	rBV	514085	802863	71.48%	9.837%
75	11.712	3317	3319	3322	rBV2	588	252	0.02%	0.003%
76	11.763	3332	3335	3337	rBV2	466	323	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022360.D
 Acq On : 28 Sep 2021 11:03
 Operator : SY/MD
 Sample : VV0928WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.853	3359	3363	3364	rBV3	495	335	0.03%	0.004%
78	11.886	3371	3373	3377	rVB2	487	259	0.02%	0.003%
79	12.146	3450	3454	3455	rBV2	372	202	0.02%	0.002%
80	12.239	3479	3483	3488	rBV3	680	469	0.04%	0.006%
81	12.265	3488	3491	3496	rVB2	395	290	0.03%	0.004%
82	12.294	3496	3500	3501	rBV	368	242	0.02%	0.003%
83	12.715	3627	3631	3633	rBV	265	193	0.02%	0.002%
84	12.751	3640	3642	3646	rBV2	359	281	0.03%	0.003%
85	12.847	3670	3672	3676	rVB3	288	213	0.02%	0.003%
86	12.915	3692	3693	3698	rVB	414	216	0.02%	0.003%
87	12.943	3698	3702	3707	rBV	293	297	0.03%	0.004%
88	12.972	3708	3711	3713	rVV	464	227	0.02%	0.003%
89	12.988	3713	3716	3721	rVB2	241	201	0.02%	0.002%
90	13.214	3785	3786	3794	rVB5	361	323	0.03%	0.004%
91	13.400	3841	3844	3846	rBV	425	223	0.02%	0.003%
92	13.445	3855	3858	3861	rBV2	285	198	0.02%	0.002%
93	13.751	3949	3953	3956	rBV2	517	462	0.04%	0.006%
94	14.005	4030	4032	4036	rVB2	388	219	0.02%	0.003%
95	14.027	4036	4039	4042	rBV	412	312	0.03%	0.004%
96	14.082	4054	4056	4061	rVB3	419	241	0.02%	0.003%
97	14.114	4064	4066	4071	rVB2	399	324	0.03%	0.004%
98	14.217	4097	4098	4104	rVB3	473	327	0.03%	0.004%
99	14.345	4135	4138	4141	rBV	340	221	0.02%	0.003%
100	14.423	4160	4162	4164	rBV2	404	194	0.02%	0.002%




Sum of corrected areas: 8161844

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022360.D
Acq On : 28 Sep 2021 11:03
Operator : SY/MD
Sample : VV0928WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

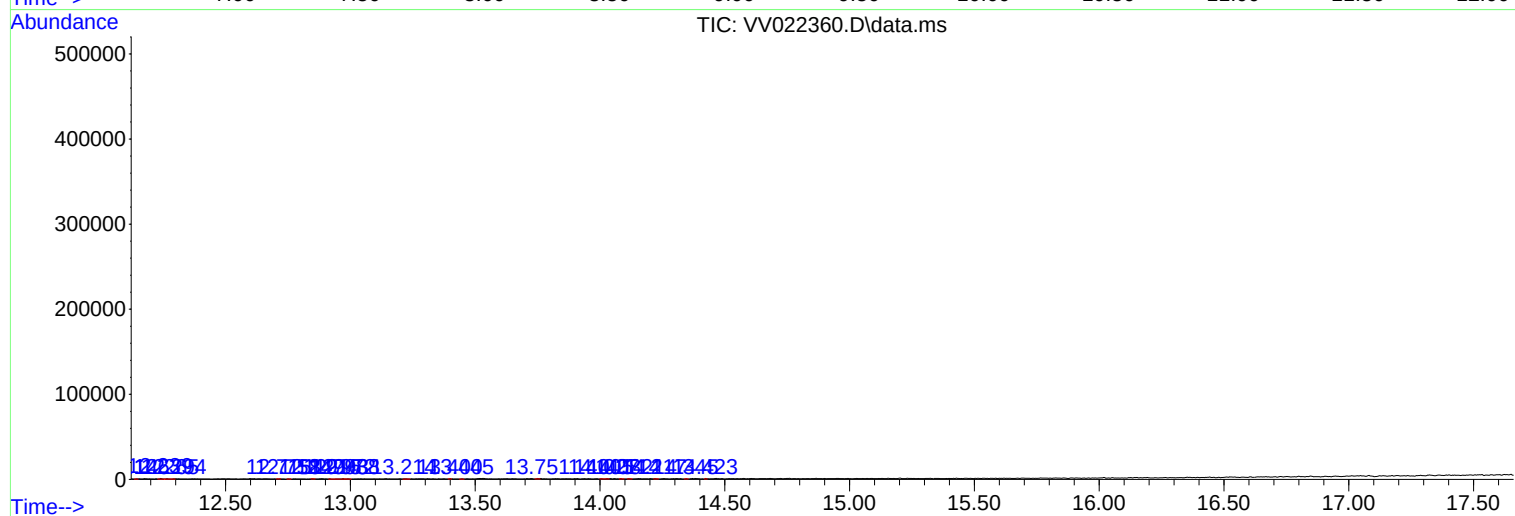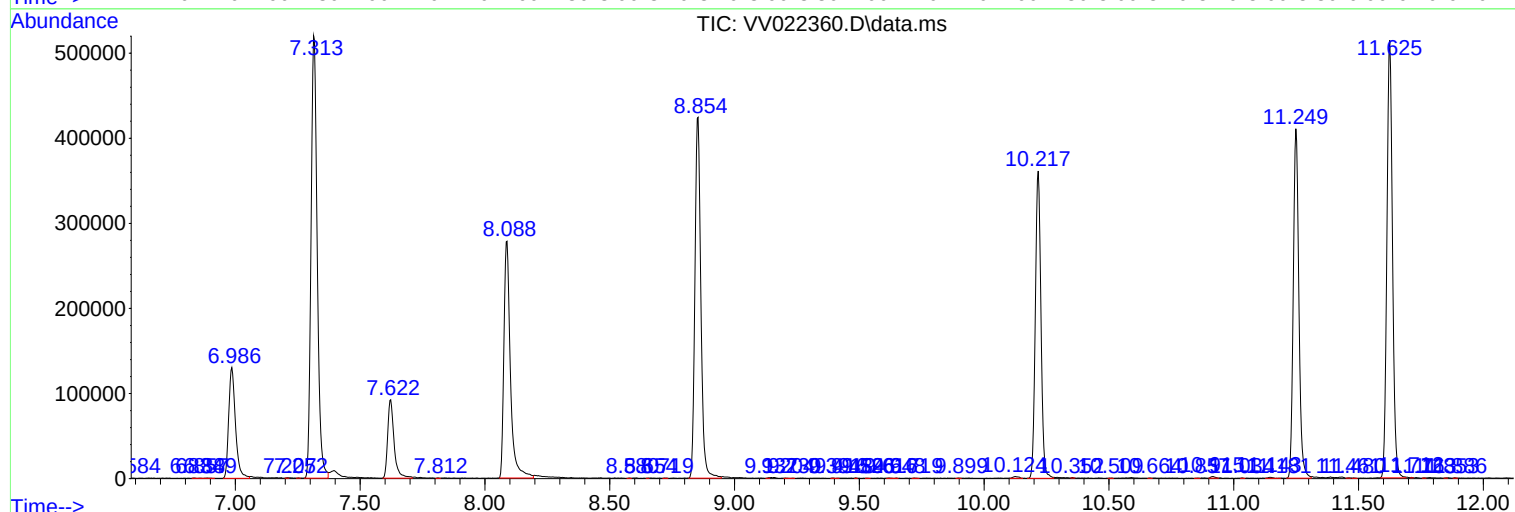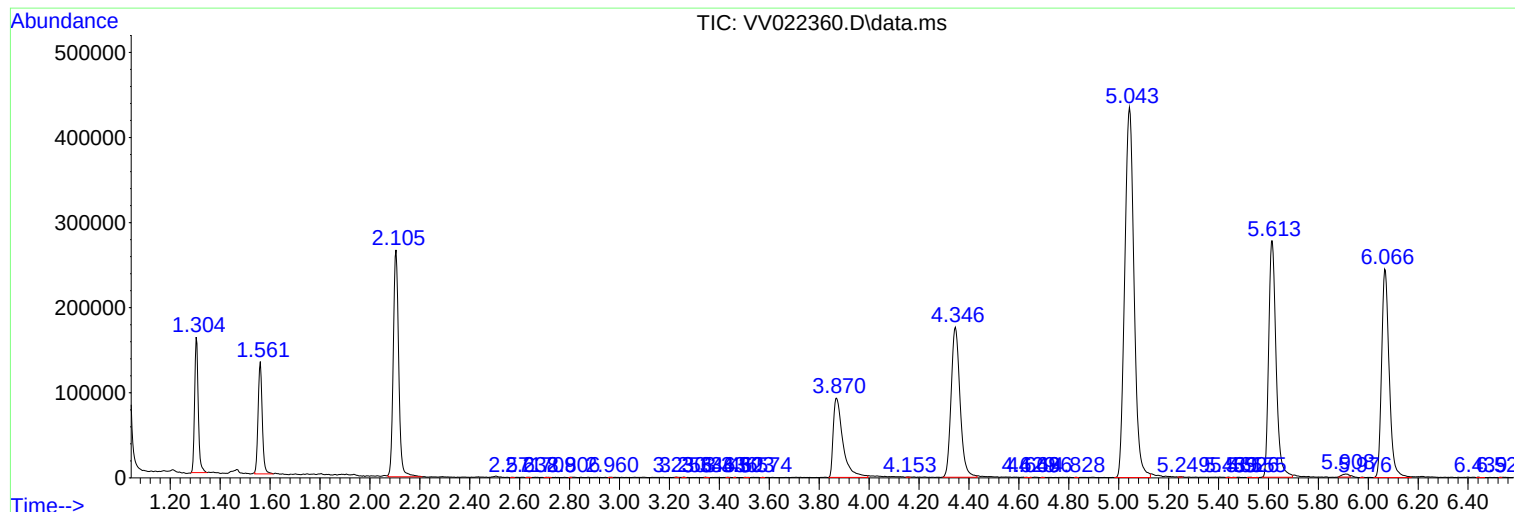

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022360.D
Acq On : 28 Sep 2021 11:03
Operator : SY/MD
Sample : VV0928WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022360.D
Acq On : 28 Sep 2021 11:03
Operator : SY/MD
Sample : VV0928WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
