

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100UL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	105	rVB	109898	164152	14.48%	1.977%
2	2.076	313	322	333	rBV	258438	368081	32.48%	4.433%
3	2.539	464	466	469	rVB3	500	232	0.02%	0.003%
4	2.574	476	477	481	rBV2	410	227	0.02%	0.003%
5	2.696	513	515	520	rVB4	316	178	0.02%	0.002%
6	2.770	535	538	541	rBV2	336	262	0.02%	0.003%
7	2.818	551	553	556	rBV2	279	153	0.01%	0.002%
8	2.896	573	577	579	rBV3	185	180	0.02%	0.002%
9	2.925	584	586	589	rVV	371	191	0.02%	0.002%
10	3.191	667	669	673	rVB3	343	235	0.02%	0.003%
11	3.246	682	686	688	rBV	185	150	0.01%	0.002%
12	3.310	702	706	710	rVB4	653	514	0.05%	0.006%
13	3.343	713	716	718	rBV	245	157	0.01%	0.002%
14	3.372	721	725	730	rBV2	367	295	0.03%	0.004%
15	3.597	793	795	797	rBV2	320	183	0.02%	0.002%
16	3.638	805	808	810	rBV	313	161	0.01%	0.002%
17	3.790	852	855	860	rVB2	232	173	0.02%	0.002%
18	3.886	875	885	924	rBV	58350	226567	19.99%	2.729%
19	4.339	1011	1026	1057	rBV	168502	436098	38.48%	5.252%
20	4.526	1082	1084	1086	rBV2	393	169	0.01%	0.002%
21	4.622	1112	1114	1116	rBV2	336	176	0.02%	0.002%
22	4.767	1156	1159	1163	rBV3	351	253	0.02%	0.003%
23	4.925	1205	1208	1209	rBV2	376	195	0.02%	0.002%
24	5.037	1226	1243	1275	rBV2	447359	1133393	100.00%	13.651%
25	5.330	1327	1334	1341	rBV8	3040	5747	0.51%	0.069%
26	5.506	1387	1389	1392	rBV2	340	246	0.02%	0.003%
27	5.539	1396	1399	1400	rBV2	342	187	0.02%	0.002%
28	5.609	1409	1421	1451	rBV	299617	633544	55.90%	7.631%
29	5.912	1505	1515	1526	rBV7	3104	6919	0.61%	0.083%
30	6.066	1550	1563	1589	rBV	233054	495315	43.70%	5.966%
31	6.314	1636	1640	1641	rBV2	431	266	0.02%	0.003%
32	6.323	1641	1643	1647	rVB2	463	285	0.03%	0.003%
33	6.349	1647	1651	1654	rBV2	364	301	0.03%	0.004%
34	6.394	1660	1665	1670	rBV3	499	628	0.06%	0.008%
35	6.445	1679	1681	1687	rBV3	243	206	0.02%	0.002%
36	6.490	1692	1695	1696	rBV	351	201	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.635	1736	1740	1741	rBV2	653	382	0.03%	0.005%
38	6.690	1754	1757	1758	rBV2	462	253	0.02%	0.003%
39	6.728	1766	1769	1770	rBV2	328	175	0.02%	0.002%
40	6.757	1774	1778	1781	rVB3	409	309	0.03%	0.004%
41	6.786	1783	1787	1791	rVB3	492	364	0.03%	0.004%
42	6.805	1791	1793	1795	rBV	477	316	0.03%	0.004%
43	6.982	1838	1848	1876	rBV	117882	237246	20.93%	2.857%
44	7.166	1902	1905	1909	rVB	567	352	0.03%	0.004%
45	7.259	1932	1934	1938	rVB2	448	342	0.03%	0.004%
46	7.313	1938	1951	1970	rBV	506856	906647	79.99%	10.920%
47	7.622	2037	2047	2076	rBV	81457	163741	14.45%	1.972%
48	7.850	2115	2118	2119	rBV2	447	250	0.02%	0.003%
49	8.053	2178	2181	2184	rBV2	343	204	0.02%	0.002%
50	8.101	2184	2196	2224	rBV2	209157	514491	45.39%	6.197%
51	8.410	2287	2292	2293	rBV2	443	333	0.03%	0.004%
52	8.545	2332	2334	2342	rVB3	396	355	0.03%	0.004%
53	8.748	2390	2397	2400	rBV3	554	650	0.06%	0.008%
54	8.802	2412	2414	2416	rBV	430	202	0.02%	0.002%
55	8.854	2418	2430	2448	rBV	455536	772991	68.20%	9.310%
56	9.204	2536	2539	2543	rBV3	350	295	0.03%	0.004%
57	9.243	2548	2551	2553	rBV	395	260	0.02%	0.003%
58	9.288	2563	2565	2568	rBV2	283	151	0.01%	0.002%
59	9.461	2615	2619	2622	rBV2	417	336	0.03%	0.004%
60	9.548	2643	2646	2647	rBV3	343	193	0.02%	0.002%
61	9.600	2661	2662	2665	rVV	340	152	0.01%	0.002%
62	9.661	2678	2681	2682	rBV	345	168	0.01%	0.002%
63	9.715	2690	2698	2713	rBV4	5427	10527	0.93%	0.127%
64	9.815	2727	2729	2732	rBV2	351	187	0.02%	0.002%
65	9.873	2743	2747	2749	rBV2	441	300	0.03%	0.004%
66	9.976	2775	2779	2781	rVB2	326	222	0.02%	0.003%
67	10.011	2789	2790	2793	rVV2	492	241	0.02%	0.003%
68	10.072	2805	2809	2811	rBV2	313	163	0.01%	0.002%
69	10.127	2817	2826	2835	rVB3	3750	5545	0.49%	0.067%
70	10.220	2843	2855	2873	rBV	353959	579086	51.09%	6.975%
71	10.455	2925	2928	2931	rBV2	227	180	0.02%	0.002%
72	10.574	2960	2965	2969	rBV5	1237	1334	0.12%	0.016%
73	10.821	3040	3042	3044	rBV	433	299	0.03%	0.004%
74	10.915	3065	3071	3081	rVB7	2818	4178	0.37%	0.050%
75	11.050	3111	3113	3117	rVB2	510	267	0.02%	0.003%
76	11.153	3136	3145	3148	rBV4	1859	2467	0.22%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022361.D
 Acq On : 28 Sep 2021 11:33
 Operator : SY/MD
 Sample : M3834-06ME
 Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW407ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.252	3164	3176	3194	rBV	476892	754692	66.59%	9.090%
78	11.628	3280	3293	3315	rBV	538761	860357	75.91%	10.362%
79	11.963	3393	3397	3398	rBV2	239	172	0.02%	0.002%
80	12.127	3446	3448	3452	rVB2	465	178	0.02%	0.002%
81	12.236	3480	3482	3483	rBV	536	290	0.03%	0.003%
82	12.320	3505	3508	3510	rBV2	314	200	0.02%	0.002%
83	12.333	3510	3512	3516	rVV	241	160	0.01%	0.002%
84	12.413	3535	3537	3539	rBV	424	231	0.02%	0.003%
85	12.435	3542	3544	3547	rVB4	553	306	0.03%	0.004%
86	12.776	3647	3650	3653	rBV	383	223	0.02%	0.003%
87	12.808	3658	3660	3664	rBV2	300	261	0.02%	0.003%
88	12.879	3679	3682	3684	rVB2	337	208	0.02%	0.003%
89	12.998	3714	3719	3724	rBV3	331	368	0.03%	0.004%
90	13.387	3834	3840	3844	rBV4	316	403	0.04%	0.005%
91	13.406	3844	3846	3850	rBV2	399	175	0.02%	0.002%
92	13.513	3875	3879	3880	rBV	428	231	0.02%	0.003%
93	13.706	3937	3939	3942	rVB	426	226	0.02%	0.003%
94	13.767	3956	3958	3961	rBV	317	177	0.02%	0.002%
95	13.831	3976	3978	3980	rBV2	350	161	0.01%	0.002%
96	13.898	3997	3999	4002	rBV2	545	299	0.03%	0.004%
97	13.947	4011	4014	4017	rBV3	338	265	0.02%	0.003%
98	14.477	4177	4179	4183	rBV3	649	357	0.03%	0.004%
99	14.603	4216	4218	4219	rBV	453	204	0.02%	0.002%
100	14.908	4311	4313	4315	rBV3	453	158	0.01%	0.002%




Sum of corrected areas: 8302676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022361.D
Acq On : 28 Sep 2021 11:33
Operator : SY/MD
Sample : M3834-06ME
Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW407ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

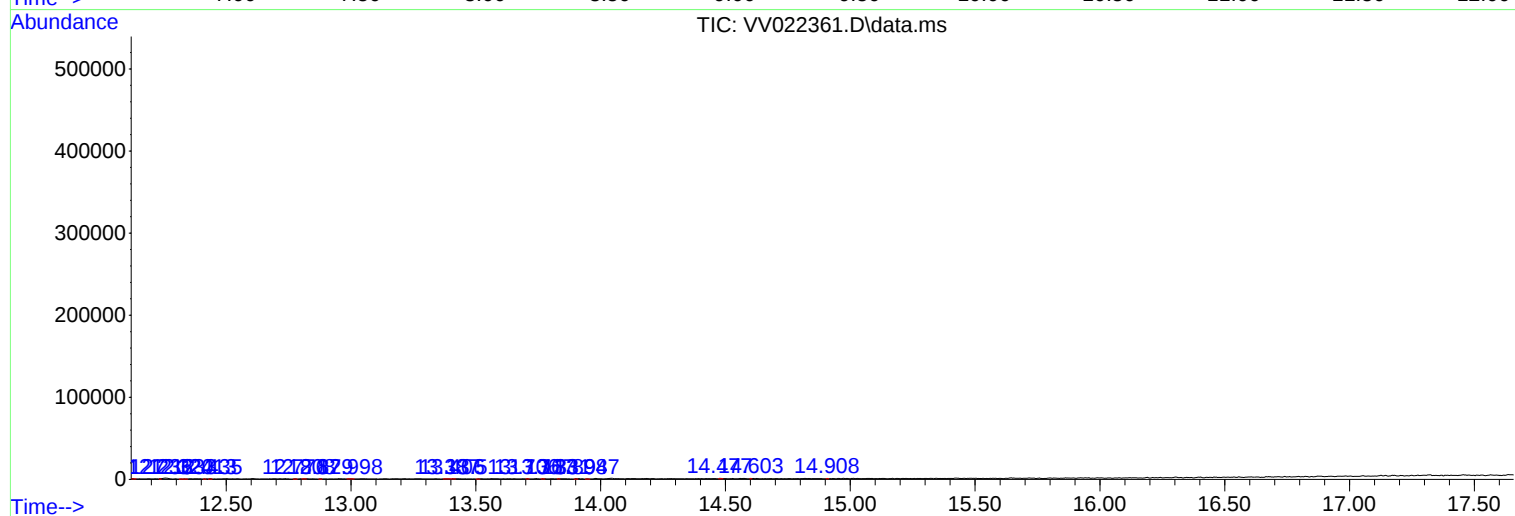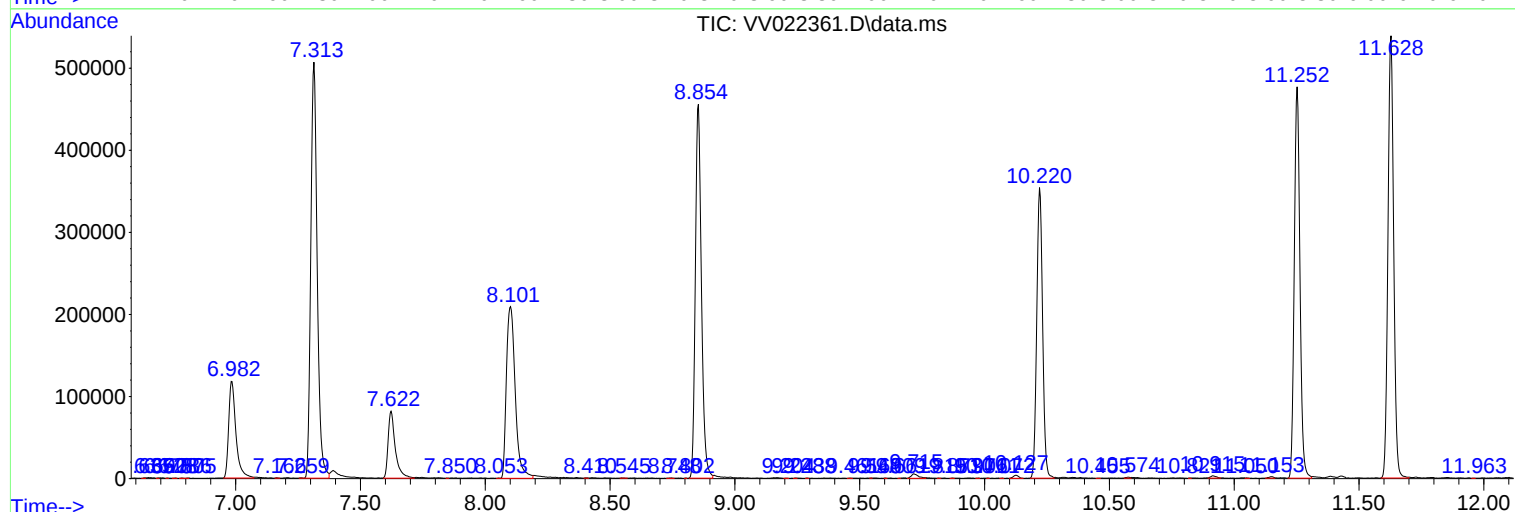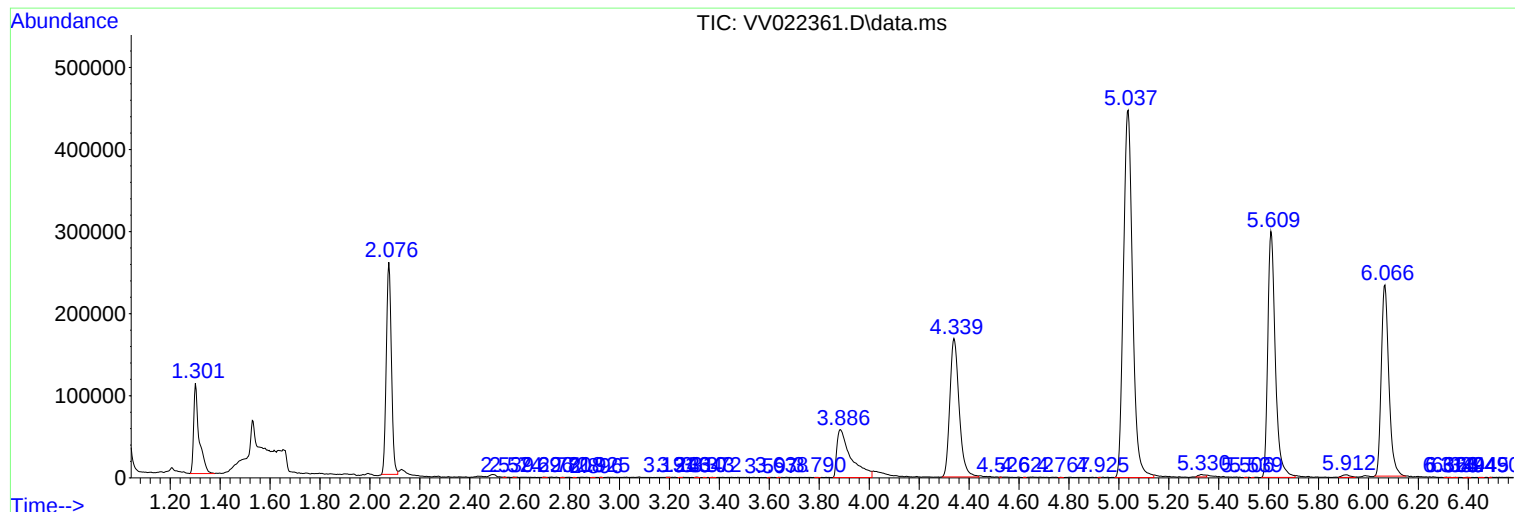

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022361.D
Acq On : 28 Sep 2021 11:33
Operator : SY/MD
Sample : M3834-06ME
Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW407ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022361.D
Acq On : 28 Sep 2021 11:33
Operator : SY/MD
Sample : M3834-06ME
Misc : 4.73g/5.0mL/100U1/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW407ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
