

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022363.D
 Acq On : 28 Sep 2021 13:18
 Operator : SY/MD
 Sample : M3873-11DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7X9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	97	rVB	171196	175666	14.70%	1.845%
2	1.561	156	162	179	rVB	139939	162085	13.57%	1.703%
3	2.105	321	331	351	rBV	279508	409951	34.32%	4.307%
4	2.410	424	426	428	rBV3	346	201	0.02%	0.002%
5	2.507	446	456	465	rBV5	2561	4195	0.35%	0.044%
6	2.561	470	473	474	rBV2	420	223	0.02%	0.002%
7	2.703	513	517	521	rBV4	368	363	0.03%	0.004%
8	2.764	525	536	548	rVB2	4952	9360	0.78%	0.098%
9	2.947	589	593	594	rBV2	223	167	0.01%	0.002%
10	2.998	607	609	613	rVB2	447	187	0.02%	0.002%
11	3.018	613	615	617	rBV	306	171	0.01%	0.002%
12	3.047	621	624	628	rBV3	345	256	0.02%	0.003%
13	3.117	642	646	649	rVB2	233	199	0.02%	0.002%
14	3.172	660	663	664	rBV	474	219	0.02%	0.002%
15	3.410	735	737	739	rBV2	377	197	0.02%	0.002%
16	3.767	844	848	851	rBV2	264	200	0.02%	0.002%
17	3.905	869	891	928	rBV2	327975	1030050	86.22%	10.821%
18	4.240	993	995	998	rVB3	645	240	0.02%	0.003%
19	4.342	1013	1027	1054	rBV2	184501	455223	38.11%	4.782%
20	4.622	1111	1114	1118	rBV2	704	436	0.04%	0.005%
21	4.760	1153	1157	1159	rBV	429	299	0.03%	0.003%
22	4.793	1164	1167	1170	rBV	281	204	0.02%	0.002%
23	4.895	1194	1199	1201	rBV	302	305	0.03%	0.003%
24	4.908	1201	1203	1207	rVB2	384	233	0.02%	0.002%
25	5.040	1228	1244	1282	rBV2	455016	1194633	100.00%	12.550%
26	5.339	1335	1337	1340	rBV2	558	269	0.02%	0.003%
27	5.452	1370	1372	1377	rBV	314	240	0.02%	0.003%
28	5.535	1395	1398	1399	rBV	357	191	0.02%	0.002%
29	5.564	1403	1407	1409	rBV2	293	211	0.02%	0.002%
30	5.613	1409	1422	1456	rBV	312374	640055	53.58%	6.724%
31	5.802	1479	1481	1488	rVB3	725	532	0.04%	0.006%
32	5.915	1503	1516	1533	rBV3	54119	117490	9.83%	1.234%
33	6.014	1545	1547	1549	rBV	410	174	0.01%	0.002%
34	6.066	1549	1563	1594	rBV	261129	541508	45.33%	5.689%
35	6.400	1662	1667	1670	rBV3	389	390	0.03%	0.004%
36	6.625	1734	1737	1742	rVB2	352	277	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022363.D
 Acq On : 28 Sep 2021 13:18
 Operator : SY/MD
 Sample : M3873-11DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7X9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.657	1742	1747	1749	rBV2	466	439	0.04%	0.005%
38	6.706	1759	1762	1764	rBV2	438	169	0.01%	0.002%
39	6.728	1764	1769	1770	rVV2	441	333	0.03%	0.003%
40	6.744	1770	1774	1776	rVB2	437	283	0.02%	0.003%
41	6.780	1783	1785	1788	rVB2	427	209	0.02%	0.002%
42	6.982	1837	1848	1876	rBV	134621	252565	21.14%	2.653%
43	7.265	1932	1936	1939	rBV3	214	166	0.01%	0.002%
44	7.313	1939	1951	1970	rBV	539385	942753	78.92%	9.904%
45	7.619	2035	2046	2062	rBV	92977	165190	13.83%	1.735%
46	7.911	2135	2137	2141	rBV3	391	214	0.02%	0.002%
47	8.085	2181	2191	2225	rBV	292662	516227	43.21%	5.423%
48	8.464	2306	2309	2311	rBV2	340	224	0.02%	0.002%
49	8.519	2323	2326	2328	rBV3	540	360	0.03%	0.004%
50	8.725	2386	2390	2393	rBV3	293	234	0.02%	0.002%
51	8.783	2404	2408	2412	rBV4	411	348	0.03%	0.004%
52	8.850	2417	2429	2458	rBV	461211	767561	64.25%	8.063%
53	9.034	2485	2486	2490	rVB2	639	221	0.02%	0.002%
54	9.091	2501	2504	2507	rBV3	283	257	0.02%	0.003%
55	9.146	2518	2521	2529	rVB4	878	1015	0.08%	0.011%
56	9.281	2559	2563	2566	rVB2	475	275	0.02%	0.003%
57	9.461	2615	2619	2620	rBV2	264	187	0.02%	0.002%
58	9.484	2624	2626	2629	rBV2	380	332	0.03%	0.003%
59	9.841	2734	2737	2739	rBV	310	203	0.02%	0.002%
60	9.931	2761	2765	2767	rVB2	429	267	0.02%	0.003%
61	10.124	2819	2825	2833	rVB4	2654	3432	0.29%	0.036%
62	10.217	2840	2854	2875	rBV	359468	573325	47.99%	6.023%
63	10.365	2898	2900	2905	rBV3	466	263	0.02%	0.003%
64	10.490	2935	2939	2941	rBV2	322	188	0.02%	0.002%
65	10.513	2944	2946	2950	rBV	224	186	0.02%	0.002%
66	10.686	2996	3000	3005	rBV2	274	234	0.02%	0.002%
67	10.712	3005	3008	3009	rBV2	255	168	0.01%	0.002%
68	10.789	3028	3032	3037	rBV4	447	399	0.03%	0.004%
69	10.828	3041	3044	3046	rBV	270	195	0.02%	0.002%
70	10.870	3055	3057	3060	rBV	401	234	0.02%	0.002%
71	10.915	3063	3071	3079	rBV6	2221	3055	0.26%	0.032%
72	10.969	3085	3088	3091	rBV2	272	193	0.02%	0.002%
73	11.030	3103	3107	3113	rBV3	491	509	0.04%	0.005%
74	11.143	3136	3142	3151	rVB6	1359	1959	0.16%	0.021%
75	11.249	3163	3175	3199	rBV	445067	698304	58.45%	7.336%
76	11.468	3239	3243	3246	rVB3	464	478	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022363.D
 Acq On : 28 Sep 2021 13:18
 Operator : SY/MD
 Sample : M3873-11DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7X9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.625	3279	3292	3311	rBV	524642	833500	69.77%	8.756%
78	11.847	3357	3361	3363	rBV3	566	376	0.03%	0.004%
79	11.960	3393	3396	3399	rBV2	247	213	0.02%	0.002%
80	12.201	3468	3471	3473	rBV2	545	247	0.02%	0.003%
81	12.214	3473	3475	3477	rVV	408	175	0.01%	0.002%
82	12.680	3617	3620	3624	rBV2	288	208	0.02%	0.002%
83	12.831	3666	3667	3672	rVB3	340	227	0.02%	0.002%
84	12.976	3708	3712	3713	rBV	328	243	0.02%	0.003%
85	13.017	3723	3725	3729	rBB	346	176	0.01%	0.002%
86	13.043	3729	3733	3735	rBV2	342	236	0.02%	0.002%
87	13.069	3738	3741	3743	rBV2	326	231	0.02%	0.002%
88	13.194	3778	3780	3784	rBV3	254	198	0.02%	0.002%
89	13.313	3815	3817	3821	rVB2	357	218	0.02%	0.002%
90	13.426	3850	3852	3854	rBV	379	246	0.02%	0.003%
91	13.435	3854	3855	3858	rVV	353	168	0.01%	0.002%
92	13.525	3880	3883	3885	rVB2	659	299	0.03%	0.003%
93	13.593	3902	3904	3909	rBV	303	218	0.02%	0.002%
94	13.670	3925	3928	3931	rBV2	372	264	0.02%	0.003%
95	13.718	3941	3943	3949	rVB2	511	342	0.03%	0.004%
96	13.940	4009	4012	4014	rBV2	304	175	0.01%	0.002%
97	13.988	4023	4027	4030	rBV3	481	370	0.03%	0.004%
98	14.049	4040	4046	4047	rBV3	444	398	0.03%	0.004%
99	14.448	4168	4170	4173	rBV2	437	272	0.02%	0.003%
100	14.940	4321	4323	4325	rBV	451	233	0.02%	0.002%




Sum of corrected areas: 9518987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022363.D
Acq On : 28 Sep 2021 13:18
Operator : SY/MD
Sample : M3873-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7X9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

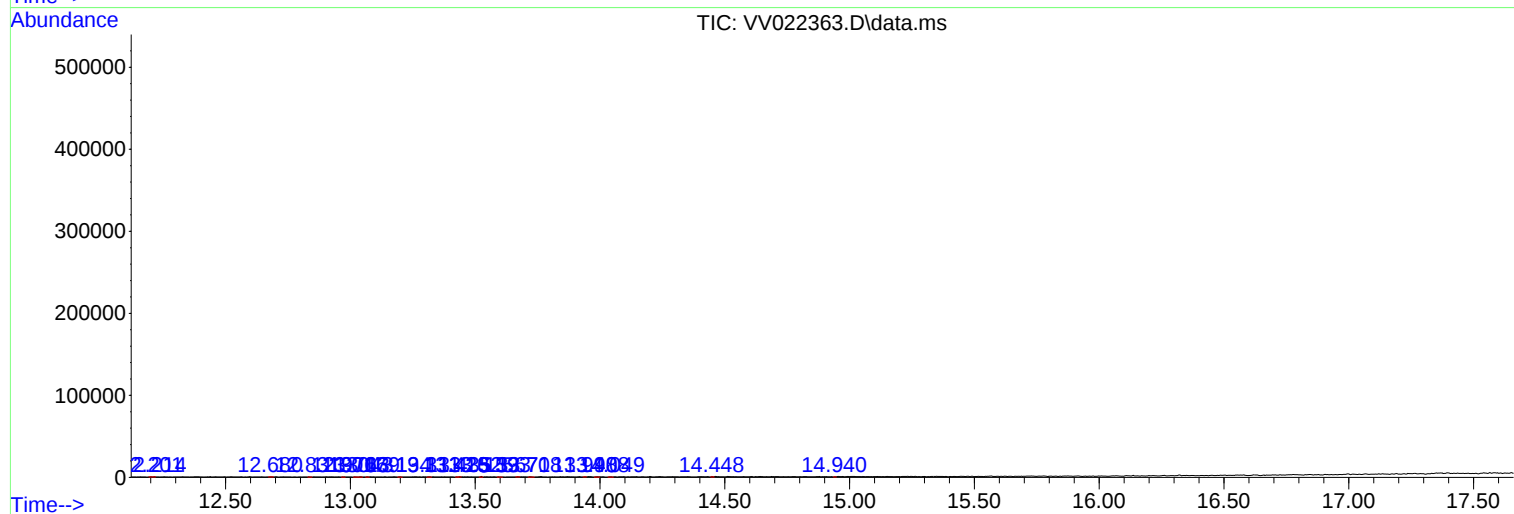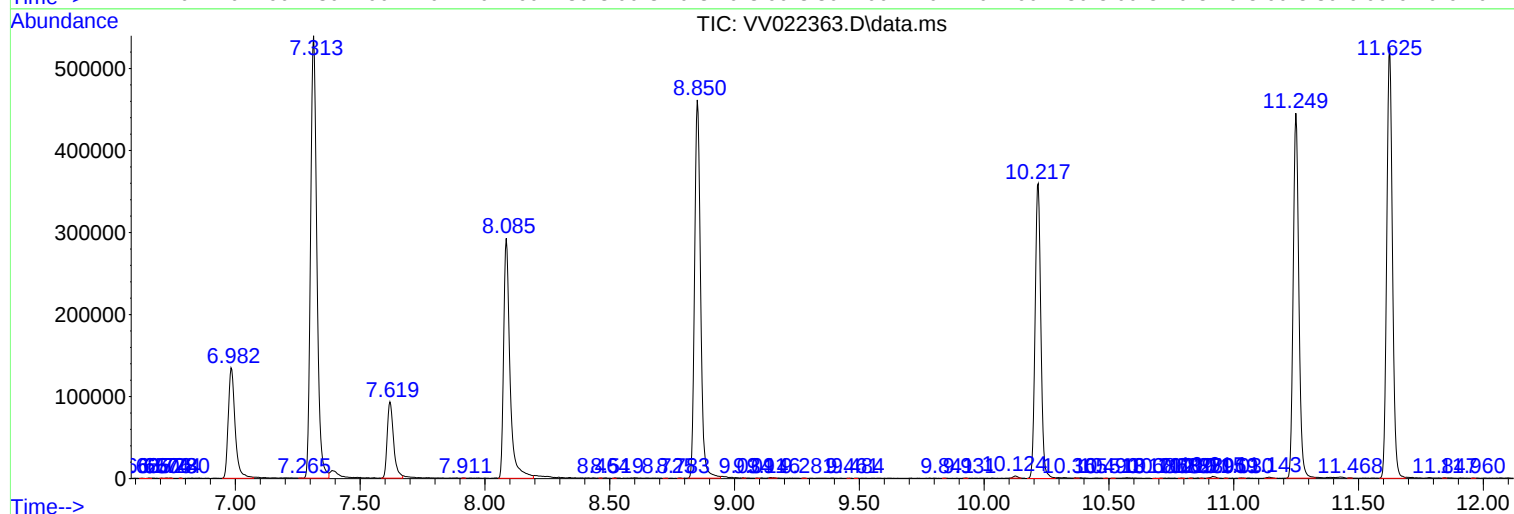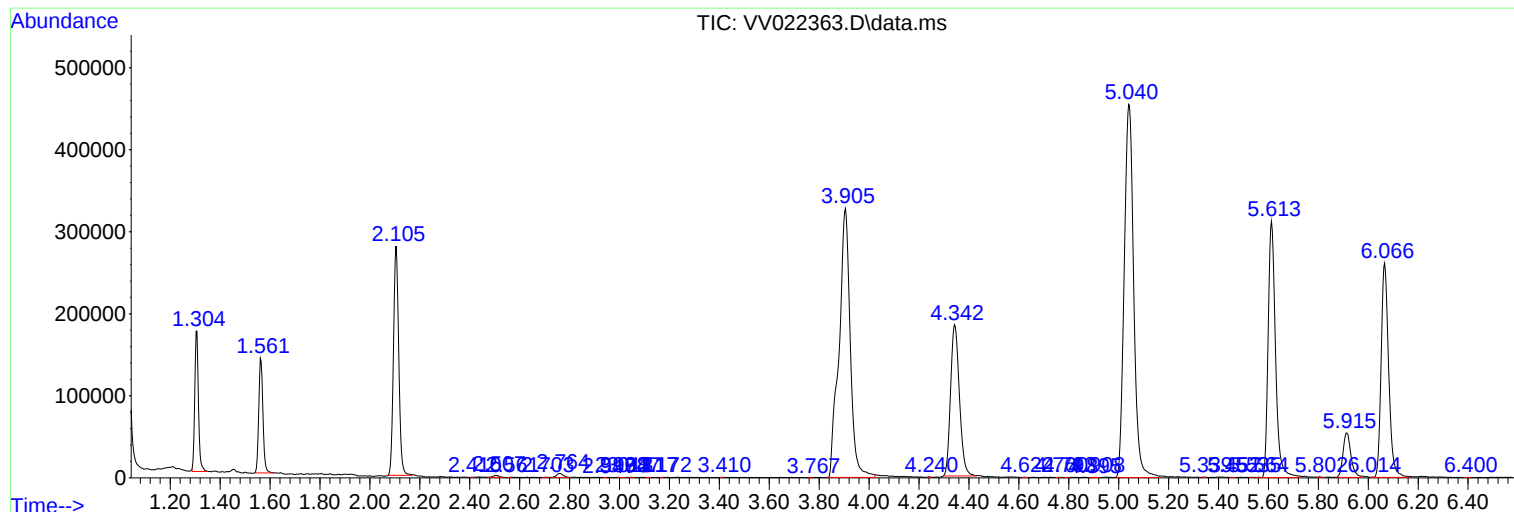

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022363.D
Acq On : 28 Sep 2021 13:18
Operator : SY/MD
Sample : M3873-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7X9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022363.D
Acq On : 28 Sep 2021 13:18
Operator : SY/MD
Sample : M3873-11DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7X9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
