

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022367.D
 Acq On : 28 Sep 2021 14:55
 Operator : SY/MD
 Sample : M3873-25
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	156135	160261	14.29%	1.953%
2	1.561	155	162	177	rVB	131569	153714	13.71%	1.873%
3	2.105	321	331	356	rVB	264334	392014	34.96%	4.776%
4	2.252	375	377	379	rBV	414	265	0.02%	0.003%
5	2.506	449	456	467	rVB5	3480	5944	0.53%	0.072%
6	2.764	534	536	538	rBV	229	107	0.01%	0.001%
7	2.828	553	556	559	rBV	241	198	0.02%	0.002%
8	2.934	587	589	593	rBV2	290	140	0.01%	0.002%
9	2.953	593	595	598	rVB2	290	123	0.01%	0.001%
10	2.969	598	600	603	rBV2	211	148	0.01%	0.002%
11	3.034	618	620	621	rBV2	338	166	0.01%	0.002%
12	3.072	627	632	633	rBV2	514	470	0.04%	0.006%
13	3.108	640	643	644	rBV	255	122	0.01%	0.001%
14	3.169	660	662	665	rBV2	277	217	0.02%	0.003%
15	3.577	786	789	793	rBV2	426	291	0.03%	0.004%
16	3.706	828	829	833	rVB	353	122	0.01%	0.001%
17	3.725	833	835	836	rBV	345	108	0.01%	0.001%
18	3.738	836	839	842	rVB2	461	281	0.03%	0.003%
19	3.838	867	870	872	rBV2	517	233	0.02%	0.003%
20	3.876	872	882	915	rBV2	94486	263035	23.46%	3.205%
21	4.349	1013	1029	1061	rBV2	166969	440345	39.28%	5.365%
22	4.538	1085	1088	1091	rBV4	701	554	0.05%	0.007%
23	4.616	1109	1112	1115	rVB3	509	351	0.03%	0.004%
24	4.696	1134	1137	1141	rVB3	721	525	0.05%	0.006%
25	4.860	1183	1188	1190	rBV3	297	298	0.03%	0.004%
26	4.899	1197	1200	1202	rBV2	429	244	0.02%	0.003%
27	5.047	1229	1246	1275	rBV2	435821	1121182	100.00%	13.660%
28	5.320	1329	1331	1332	rBV2	380	126	0.01%	0.002%
29	5.394	1351	1354	1355	rBV	226	117	0.01%	0.001%
30	5.429	1363	1365	1369	rVB3	772	550	0.05%	0.007%
31	5.513	1385	1391	1393	rBV2	304	254	0.02%	0.003%
32	5.551	1400	1403	1404	rBV2	405	181	0.02%	0.002%
33	5.616	1411	1423	1460	rBV	286882	588821	52.52%	7.174%
34	5.908	1503	1514	1516	rBV5	3489	4158	0.37%	0.051%
35	6.072	1549	1565	1595	rBV	248459	513506	45.80%	6.256%
36	6.278	1628	1629	1631	rBV	409	167	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022367.D
 Acq On : 28 Sep 2021 14:55
 Operator : SY/MD
 Sample : M3873-25
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.313	1638	1640	1642	rBV2	359	190	0.02%	0.002%
38	6.509	1699	1701	1704	rBV	392	209	0.02%	0.003%
39	6.529	1704	1707	1709	rBV2	417	184	0.02%	0.002%
40	6.641	1740	1742	1744	rBV	414	141	0.01%	0.002%
41	6.696	1757	1759	1760	rBV	281	128	0.01%	0.002%
42	6.760	1777	1779	1783	rVB4	293	158	0.01%	0.002%
43	6.799	1789	1791	1795	rBV2	228	163	0.01%	0.002%
44	6.821	1795	1798	1802	rVB2	250	158	0.01%	0.002%
45	6.989	1838	1850	1871	rBV	131334	238440	21.27%	2.905%
46	7.271	1936	1938	1940	rBV	464	244	0.02%	0.003%
47	7.317	1940	1952	1971	rBV	509328	891944	79.55%	10.867%
48	7.625	2038	2048	2068	rBV	89149	158291	14.12%	1.929%
49	7.882	2126	2128	2131	rBV2	261	117	0.01%	0.001%
50	8.001	2162	2165	2168	rBV2	265	233	0.02%	0.003%
51	8.050	2177	2180	2182	rVB	336	151	0.01%	0.002%
52	8.088	2182	2192	2225	rBV	298418	537946	47.98%	6.554%
53	8.471	2309	2311	2314	rBV2	481	260	0.02%	0.003%
54	8.538	2330	2332	2336	rBV2	385	250	0.02%	0.003%
55	8.632	2359	2361	2364	rVB3	697	336	0.03%	0.004%
56	8.741	2390	2395	2396	rBV	321	299	0.03%	0.004%
57	8.770	2402	2404	2410	rBV2	248	167	0.01%	0.002%
58	8.853	2419	2430	2455	rBV	433726	715180	63.79%	8.714%
59	9.078	2498	2500	2502	rVB	358	174	0.02%	0.002%
60	9.091	2502	2504	2506	rBV	433	252	0.02%	0.003%
61	9.156	2519	2524	2528	rBV2	635	551	0.05%	0.007%
62	9.201	2537	2538	2541	rVB	330	150	0.01%	0.002%
63	9.252	2552	2554	2555	rBV	266	134	0.01%	0.002%
64	9.265	2555	2558	2561	rVB2	653	407	0.04%	0.005%
65	9.532	2639	2641	2644	rVB2	285	141	0.01%	0.002%
66	9.673	2683	2685	2686	rBV2	251	127	0.01%	0.002%
67	9.699	2690	2693	2696	rVB	335	159	0.01%	0.002%
68	9.873	2744	2747	2750	rBV	238	158	0.01%	0.002%
69	9.931	2763	2765	2767	rBV	257	111	0.01%	0.001%
70	9.959	2772	2774	2776	rVB	434	164	0.01%	0.002%
71	9.976	2776	2779	2781	rBV	184	135	0.01%	0.002%
72	10.127	2821	2826	2837	rVB5	2078	3153	0.28%	0.038%
73	10.172	2837	2840	2842	rBV2	412	280	0.02%	0.003%
74	10.217	2842	2854	2877	rBV	360878	580023	51.73%	7.067%
75	10.570	2958	2964	2969	rBV3	680	974	0.09%	0.012%
76	10.670	2993	2995	2996	rBV3	346	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022367.D
 Acq On : 28 Sep 2021 14:55
 Operator : SY/MD
 Sample : M3873-25
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.828	3042	3044	3047	rBV	309	108	0.01%	0.001%
78	10.850	3049	3051	3052	rBV	421	142	0.01%	0.002%
79	10.918	3067	3072	3082	rVB4	1729	2423	0.22%	0.030%
80	11.024	3102	3105	3107	rBV2	377	215	0.02%	0.003%
81	11.037	3107	3109	3113	rVB	658	421	0.04%	0.005%
82	11.252	3164	3176	3202	rBV	399525	632228	56.39%	7.703%
83	11.387	3216	3218	3220	rBV	729	387	0.03%	0.005%
84	11.467	3241	3243	3245	rBV2	331	141	0.01%	0.002%
85	11.519	3256	3259	3262	rBV	198	166	0.01%	0.002%
86	11.557	3266	3271	3274	rBV2	579	453	0.04%	0.006%
87	11.625	3280	3292	3312	rBV	497920	786162	70.12%	9.578%
88	11.882	3370	3372	3373	rBV	267	134	0.01%	0.002%
89	12.291	3498	3499	3502	rBV	224	134	0.01%	0.002%
90	12.438	3542	3545	3548	rVB3	325	244	0.02%	0.003%
91	12.532	3573	3574	3580	rBV2	303	346	0.03%	0.004%
92	12.654	3609	3612	3613	rBV	331	121	0.01%	0.001%
93	12.734	3636	3637	3641	rVB	323	128	0.01%	0.002%
94	12.831	3665	3667	3670	rBV	294	189	0.02%	0.002%
95	12.947	3700	3703	3709	rBV2	485	348	0.03%	0.004%
96	13.262	3799	3801	3805	rBV2	274	163	0.01%	0.002%
97	13.898	3995	3999	4001	rBV3	448	364	0.03%	0.004%
98	14.268	4111	4114	4115	rBV2	417	222	0.02%	0.003%
99	14.532	4193	4196	4198	rBV	598	316	0.03%	0.004%
100	14.622	4221	4224	4228	rBV	480	364	0.03%	0.004%




Sum of corrected areas: 8207653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022367.D
Acq On : 28 Sep 2021 14:55
Operator : SY/MD
Sample : M3873-25
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

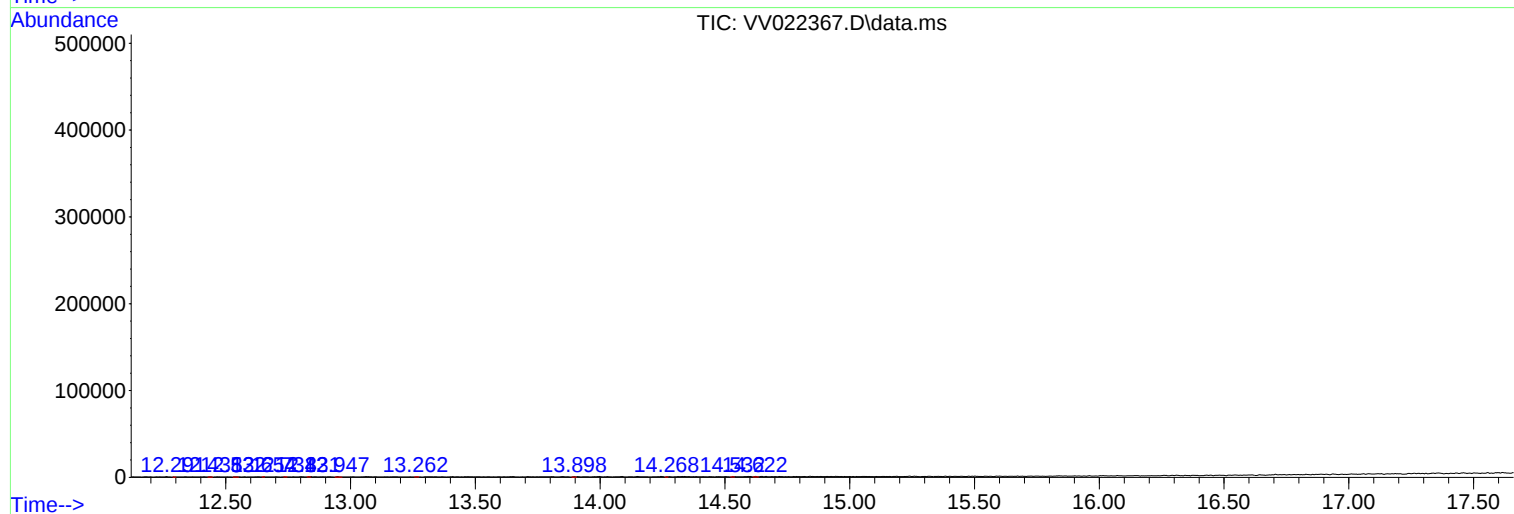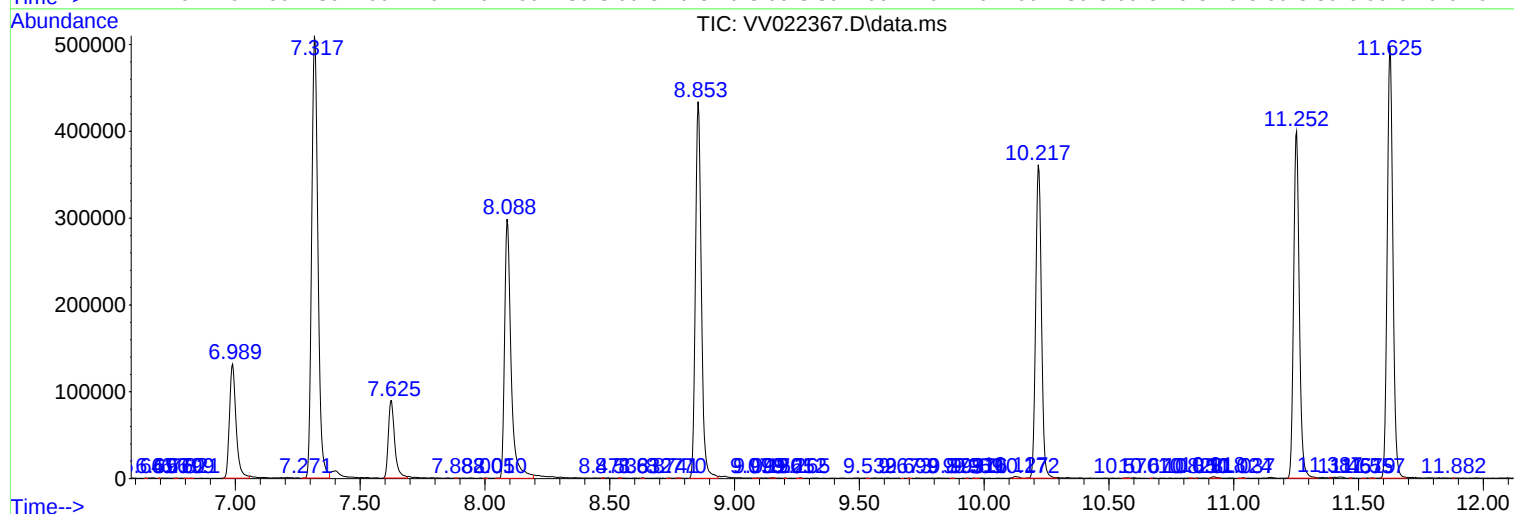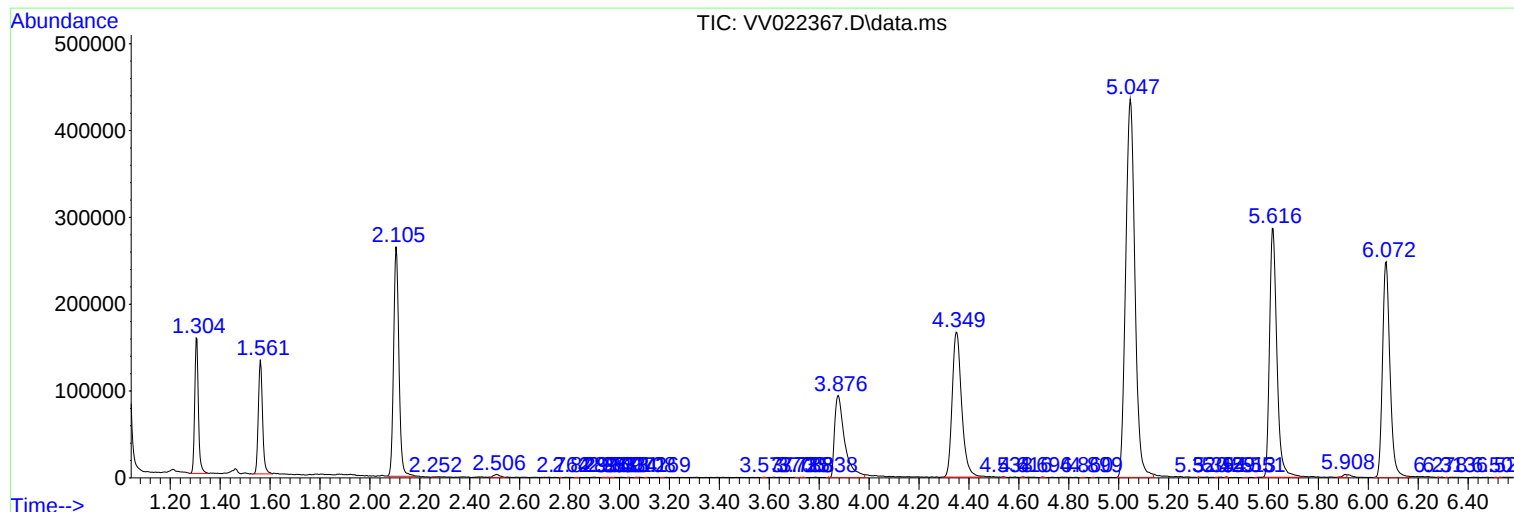

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022367.D
Acq On : 28 Sep 2021 14:55
Operator : SY/MD
Sample : M3873-25
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022367.D
Acq On : 28 Sep 2021 14:55
Operator : SY/MD
Sample : M3873-25
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
