

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022368.D
 Acq On : 28 Sep 2021 15:19
 Operator : SY/MD
 Sample : M3876-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	150017	150119	13.62%	1.876%
2	1.561	155	162	176	rVB	125449	146860	13.32%	1.835%
3	2.105	321	331	346	rBV	252490	366616	33.25%	4.581%
4	2.510	445	457	466	rBV7	3603	6451	0.59%	0.081%
5	2.812	548	551	554	rBV3	257	233	0.02%	0.003%
6	2.841	557	560	561	rBV2	483	226	0.02%	0.003%
7	3.005	606	611	614	rBV2	335	265	0.02%	0.003%
8	3.111	642	644	647	rVB	340	166	0.02%	0.002%
9	3.233	679	682	684	rVB2	344	193	0.02%	0.002%
10	3.282	695	697	702	rVB2	683	356	0.03%	0.004%
11	3.310	702	706	707	rBV	411	204	0.02%	0.003%
12	3.420	737	740	745	rVV3	347	161	0.01%	0.002%
13	3.632	802	806	813	rVB2	307	343	0.03%	0.004%
14	3.661	813	815	818	rVB2	395	190	0.02%	0.002%
15	3.709	828	830	833	rVB3	483	230	0.02%	0.003%
16	3.873	867	881	915	rBV2	95479	256735	23.29%	3.208%
17	4.349	1013	1029	1058	rBV	173148	431740	39.16%	5.395%
18	4.661	1124	1126	1129	rBV2	245	193	0.02%	0.002%
19	4.770	1158	1160	1162	rBV2	471	228	0.02%	0.003%
20	4.799	1166	1169	1171	rBV	344	268	0.02%	0.003%
21	5.047	1227	1246	1278	rBV2	428333	1102548	100.00%	13.778%
22	5.458	1371	1374	1377	rVB2	486	286	0.03%	0.004%
23	5.552	1400	1403	1406	rBV3	486	250	0.02%	0.003%
24	5.619	1412	1424	1453	rBV	277008	570812	51.77%	7.133%
25	5.870	1499	1502	1506	rVB5	550	346	0.03%	0.004%
26	5.912	1506	1515	1530	rVB4	3349	7216	0.65%	0.090%
27	5.973	1530	1534	1538	rBV4	540	459	0.04%	0.006%
28	6.072	1551	1565	1589	rBV	238092	498559	45.22%	6.230%
29	6.400	1664	1667	1670	rBV3	347	229	0.02%	0.003%
30	6.523	1700	1705	1709	rBV4	445	412	0.04%	0.005%
31	6.587	1722	1725	1728	rBV	304	212	0.02%	0.003%
32	6.629	1736	1738	1741	rBV2	342	172	0.02%	0.002%
33	6.796	1787	1790	1792	rVV	360	172	0.02%	0.002%
34	6.989	1838	1850	1876	rBV	125617	233521	21.18%	2.918%
35	7.317	1937	1952	1971	rBV	487769	861696	78.15%	10.768%
36	7.622	2037	2047	2072	rBV	86336	158138	14.34%	1.976%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022368.D
 Acq On : 28 Sep 2021 15:19
 Operator : SY/MD
 Sample : M3876-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	8.088	2182	2192	2221	rBV	300582	526470	47.75%	6.579%
38	8.407	2288	2291	2292	rBV2	355	166	0.02%	0.002%
39	8.584	2340	2346	2347	rBV2	313	289	0.03%	0.004%
40	8.619	2355	2357	2360	rBV2	297	173	0.02%	0.002%
41	8.635	2360	2362	2365	rVB3	473	256	0.02%	0.003%
42	8.674	2372	2374	2376	rBV3	368	227	0.02%	0.003%
43	8.815	2416	2418	2419	rBV2	382	172	0.02%	0.002%
44	8.854	2419	2430	2463	rVV	431203	698191	63.33%	8.725%
45	9.104	2506	2508	2510	rBV	434	249	0.02%	0.003%
46	9.137	2515	2518	2519	rVV	480	208	0.02%	0.003%
47	9.146	2519	2521	2524	rVV3	730	433	0.04%	0.005%
48	9.172	2527	2529	2534	rVB3	369	279	0.03%	0.003%
49	9.268	2557	2559	2563	rBV3	257	166	0.02%	0.002%
50	9.378	2591	2593	2599	rVB2	498	407	0.04%	0.005%
51	9.474	2620	2623	2627	rBV2	197	176	0.02%	0.002%
52	9.519	2634	2637	2641	rVB3	314	272	0.02%	0.003%
53	9.558	2645	2649	2652	rVV3	377	264	0.02%	0.003%
54	9.603	2660	2663	2666	rVB2	250	152	0.01%	0.002%
55	9.703	2689	2694	2697	rBV2	337	284	0.03%	0.004%
56	9.902	2752	2756	2761	rBV3	270	239	0.02%	0.003%
57	9.940	2765	2768	2771	rBB2	359	181	0.02%	0.002%
58	9.969	2773	2777	2780	rBV2	341	207	0.02%	0.003%
59	10.069	2806	2808	2810	rBV	308	174	0.02%	0.002%
60	10.092	2814	2815	2818	rVB2	303	157	0.01%	0.002%
61	10.133	2818	2828	2835	rBV3	1901	3163	0.29%	0.040%
62	10.217	2841	2854	2877	rBV	360630	567094	51.43%	7.087%
63	10.362	2896	2899	2901	rBV	398	301	0.03%	0.004%
64	10.375	2901	2903	2906	rBV2	572	297	0.03%	0.004%
65	10.445	2921	2925	2928	rVB2	291	246	0.02%	0.003%
66	10.465	2928	2931	2937	rBV3	433	336	0.03%	0.004%
67	10.567	2959	2963	2964	rBV	373	241	0.02%	0.003%
68	10.632	2981	2983	2985	rBV	260	162	0.01%	0.002%
69	10.690	2998	3001	3005	rVB2	319	246	0.02%	0.003%
70	10.744	3016	3018	3023	rVB2	364	205	0.02%	0.003%
71	10.828	3042	3044	3045	rVV	350	181	0.02%	0.002%
72	10.841	3046	3048	3050	rVB	589	245	0.02%	0.003%
73	10.857	3050	3053	3056	rBV2	211	154	0.01%	0.002%
74	10.918	3065	3072	3080	rBV5	1614	2668	0.24%	0.033%
75	10.953	3080	3083	3086	rBV3	394	239	0.02%	0.003%
76	11.149	3138	3144	3149	rVB3	975	1178	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022368.D
 Acq On : 28 Sep 2021 15:19
 Operator : SY/MD
 Sample : M3876-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.194	3156	3158	3162	rBV2	251	158	0.01%	0.002%
78	11.252	3164	3176	3199	rBV	388137	621139	56.34%	7.762%
79	11.529	3260	3262	3265	rBV	295	199	0.02%	0.002%
80	11.625	3280	3292	3315	rBV	485748	772000	70.02%	9.647%
81	11.860	3363	3365	3368	rVB2	637	351	0.03%	0.004%
82	11.940	3388	3390	3395	rBV3	422	291	0.03%	0.004%
83	12.056	3424	3426	3431	rVB2	489	382	0.03%	0.005%
84	12.095	3434	3438	3440	rVB3	423	304	0.03%	0.004%
85	12.217	3474	3476	3478	rBV	292	170	0.02%	0.002%
86	12.259	3487	3489	3492	rBV2	404	189	0.02%	0.002%
87	12.387	3525	3529	3530	rVV2	243	162	0.01%	0.002%
88	12.416	3535	3538	3539	rBV2	323	196	0.02%	0.002%
89	12.448	3545	3548	3550	rBV	255	197	0.02%	0.002%
90	12.500	3561	3564	3572	rVB3	346	388	0.04%	0.005%
91	12.619	3599	3601	3603	rBV2	249	162	0.01%	0.002%
92	12.960	3703	3707	3712	rBV3	249	315	0.03%	0.004%
93	13.146	3762	3765	3768	rBV2	488	371	0.03%	0.005%
94	13.172	3771	3773	3776	rBV2	315	251	0.02%	0.003%
95	13.214	3784	3786	3789	rBV	433	248	0.02%	0.003%
96	13.255	3794	3799	3801	rBV	313	269	0.02%	0.003%
97	13.612	3908	3910	3913	rBV	238	153	0.01%	0.002%
98	13.677	3928	3930	3934	rVV	259	189	0.02%	0.002%
99	13.927	4006	4008	4014	rBV3	502	446	0.04%	0.006%
100	14.017	4034	4036	4039	rBV2	485	293	0.03%	0.004%


Sum of corrected areas: 8002376

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022368.D
Acq On : 28 Sep 2021 15:19
Operator : SY/MD
Sample : M3876-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

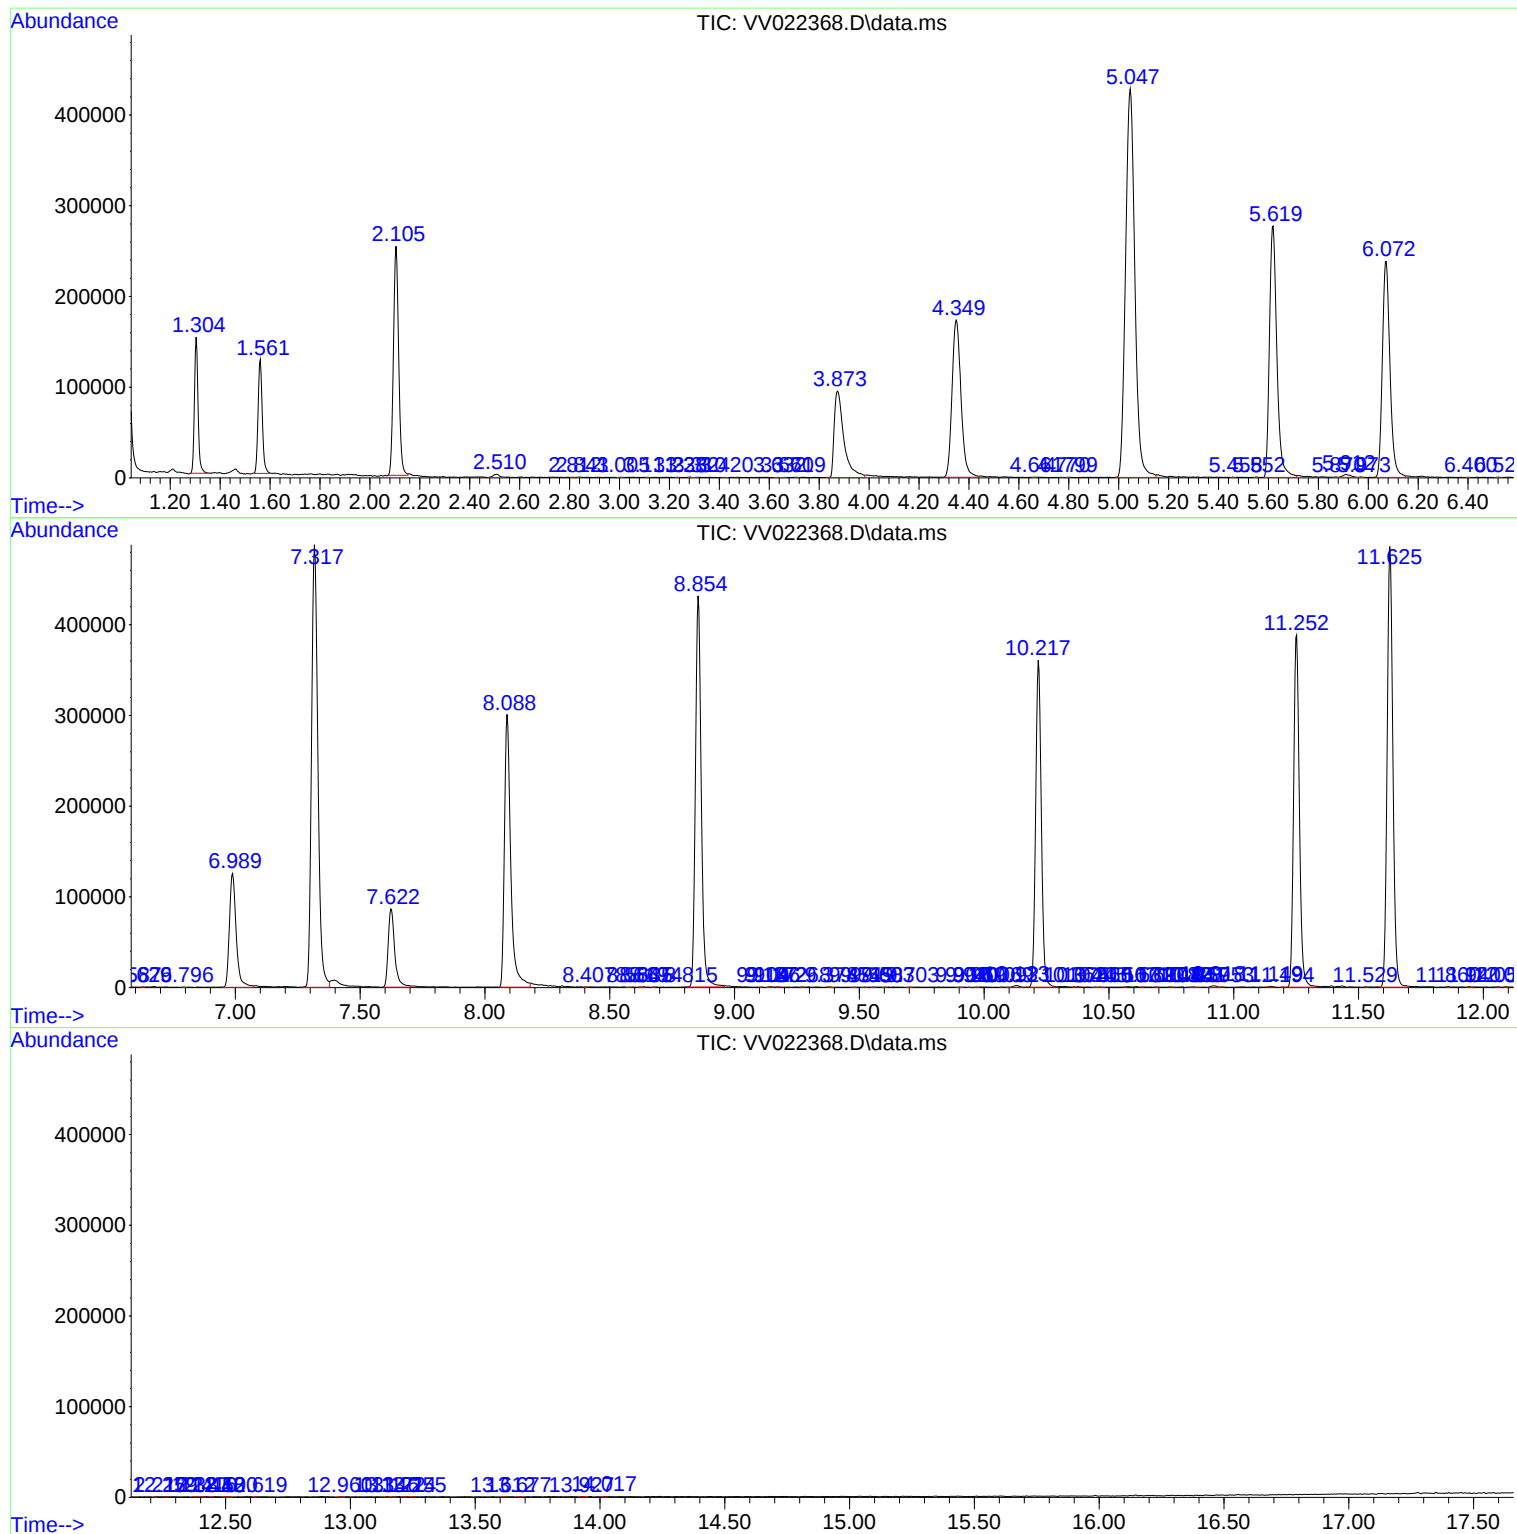

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022368.D
Acq On : 28 Sep 2021 15:19
Operator : SY/MD
Sample : M3876-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
Data File : VV022368.D
Acq On : 28 Sep 2021 15:19
Operator : SY/MD
Sample : M3876-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
