


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022334.D
 Acq On : 27 Sep 2021 15:27
 Operator : SY/MD
 Sample : BFB235
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB235

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 01 04:27:45 2021

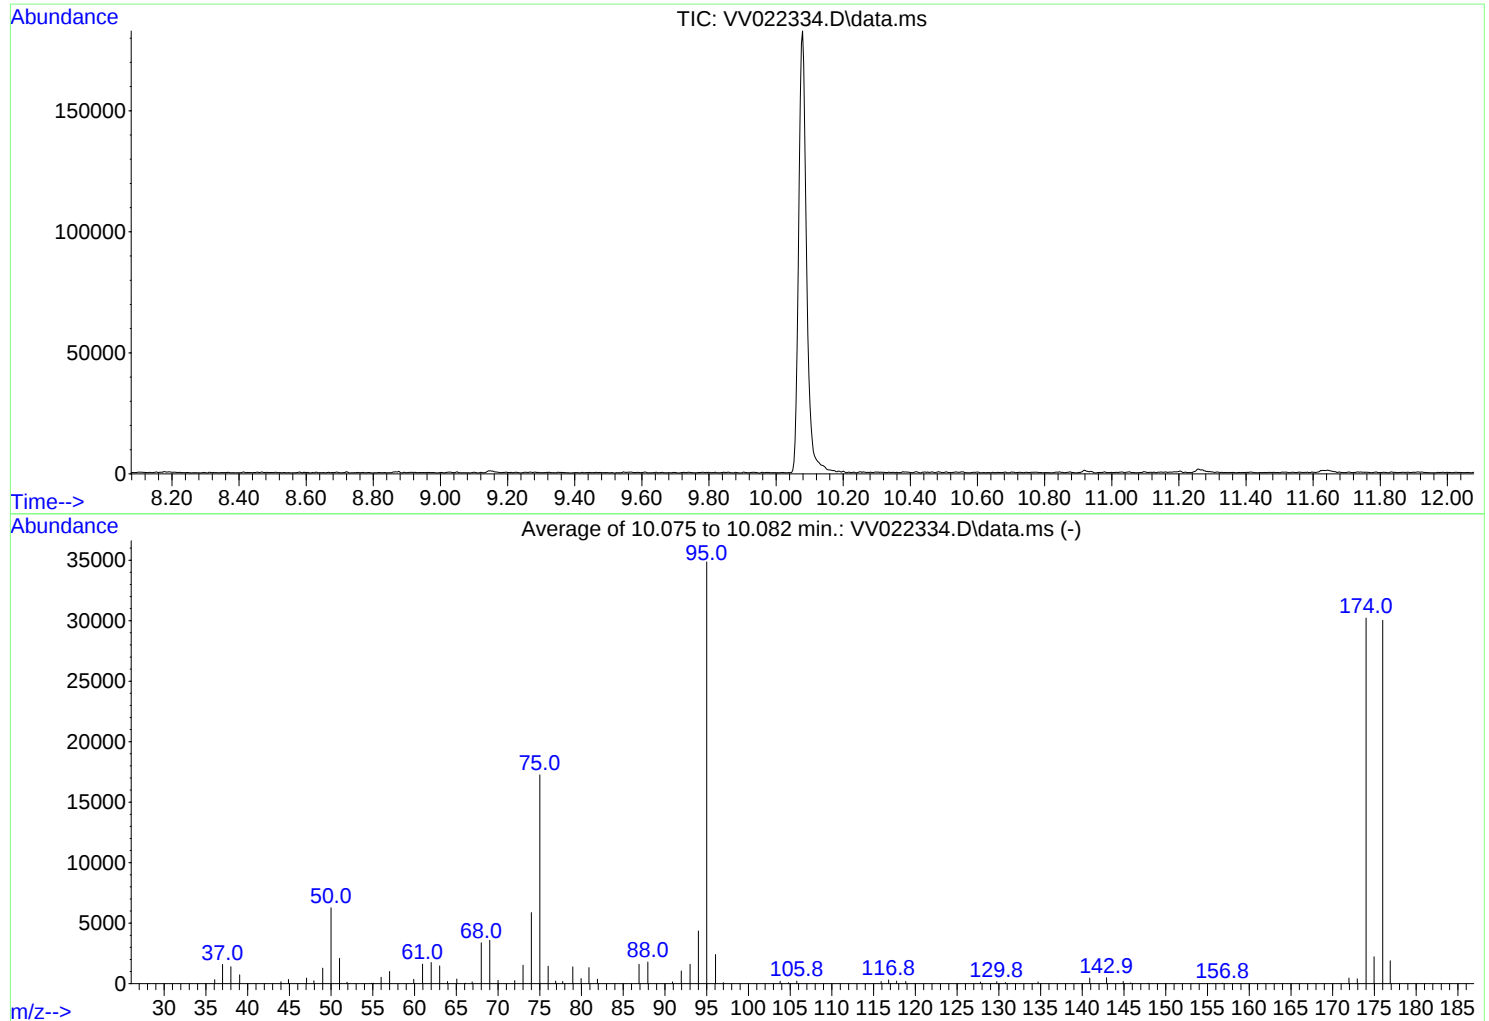

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6275	PASS
75	95	30	80	49.5	17256	PASS
95	95	100	100	100.0	34867	PASS
96	95	5	9	6.9	2403	PASS
173	174	0.00	2	1.3	396	PASS
174	95	50	120	86.7	30216	PASS
175	174	5	9	7.4	2226	PASS
176	174	95	105	99.4	30035	PASS
177	176	5	10	6.3	1889	PASS

m/z	Abundance
36.00	343.0
37.00	1617.0
38.00	1444.0
39.00	764.0
40.00	195.0
44.00	435.0
44.90	338.0
47.00	474.0
47.90	248.0
49.00	1283.0
50.00	6533.0
51.00	2180.0
51.90	128.0
55.10	102.0
56.00	552.0
57.00	1043.0
59.90	377.0
61.00	1667.0
62.00	1811.0
63.00	1508.0
64.00	185.0
65.00	376.0
66.10	102.0
66.90	153.0
68.00	3536.0
69.00	3753.0
70.00	281.0
72.00	254.0
73.00	1581.0
74.00	6039.0
75.00	17856.0
76.00	1464.0
76.90	210.0
77.70	188.0
79.00	1464.0
80.00	436.0
80.90	1350.0
81.90	387.0
86.90	1625.0
88.00	1831.0
90.90	140.0
91.90	1049.0
93.00	1650.0
94.00	4443.0
95.00	36008.0
96.00	2518.0
97.00	115.0
103.80	204.0
104.80	105.0
105.80	217.0
115.90	174.0
116.80	297.0
117.80	208.0
118.80	185.0
127.80	119.0
129.80	182.0
130.80	132.0
134.70	143.0
140.90	501.0
142.90	519.0
144.90	190.0
145.80	102.0
156.80	105.0
172.00	467.0
173.00	420.0
174.00	31336.0
175.00	2276.0
176.00	31080.0
176.90	1948.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.10	280.0
37.00	1502.0
38.00	1273.0
39.10	601.0
39.90	229.0
44.00	472.0
44.90	369.0
47.10	410.0
47.90	262.0
49.00	1082.0
50.00	5819.0
51.00	1885.0
51.90	129.0
54.80	116.0
56.00	513.0
57.00	940.0
59.90	335.0
60.90	1564.0
62.00	1655.0
63.00	1468.0
63.90	169.0
65.10	377.0
66.90	104.0
68.00	3245.0
69.00	3314.0
70.00	294.0
72.00	203.0
73.00	1442.0
74.00	5741.0
75.00	16640.0
76.00	1352.0
76.90	180.0
77.80	159.0
79.00	1344.0
80.00	405.0
80.90	1238.0
81.90	352.0
86.90	1577.0
87.90	1762.0
90.90	129.0
92.00	1113.0
93.00	1472.0
94.00	4114.0
95.00	33528.0
96.10	2191.0
103.80	195.0
105.80	159.0
115.90	155.0
116.80	290.0
117.70	188.0
118.90	196.0
127.80	143.0
129.70	166.0
134.60	142.0
140.90	453.0
142.90	524.0
144.90	161.0
145.80	110.0
171.90	490.0
173.00	398.0
174.00	29128.0
174.90	2077.0
176.00	29424.0
176.90	1793.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
39.90	227.0
44.00	284.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	364.0
37.00	1642.0
38.00	1476.0
39.00	814.0
40.00	175.0
44.00	415.0
44.90	312.0
47.00	502.0
48.00	214.0
49.00	1480.0
50.00	6473.0
51.00	2197.0
51.90	112.0
56.00	545.0
57.00	1051.0
59.90	360.0
61.00	1617.0
62.00	1789.0
63.00	1423.0
64.00	173.0
65.00	408.0
66.90	197.0
68.00	3356.0
69.00	3707.0
70.00	256.0
72.00	303.0
73.00	1529.0
74.00	5824.0
75.00	17272.0
76.00	1495.0
76.90	245.0
77.70	198.0
78.90	1349.0
79.90	421.0
80.90	1365.0
81.90	379.0
86.90	1590.0
88.00	1768.0
90.90	152.0
91.90	978.0
93.00	1671.0
94.00	4517.0
95.00	35064.0
96.00	2499.0
97.00	126.0
103.80	197.0
104.80	118.0
105.80	248.0
115.90	173.0
116.80	316.0
117.80	235.0
118.80	185.0
127.80	123.0
129.80	163.0
130.80	132.0
134.80	144.0
140.90	425.0
142.90	436.0
144.90	205.0
147.90	113.0
172.00	425.0
172.90	369.0
174.00	30184.0
175.00	2324.0
176.00	29600.0
176.90	1927.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235