


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092821\
 Data File : VV022357.D
 Acq On : 28 Sep 2021 09:25
 Operator : SY/MD
 Sample : BFB236
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB236

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 01 04:27:45 2021

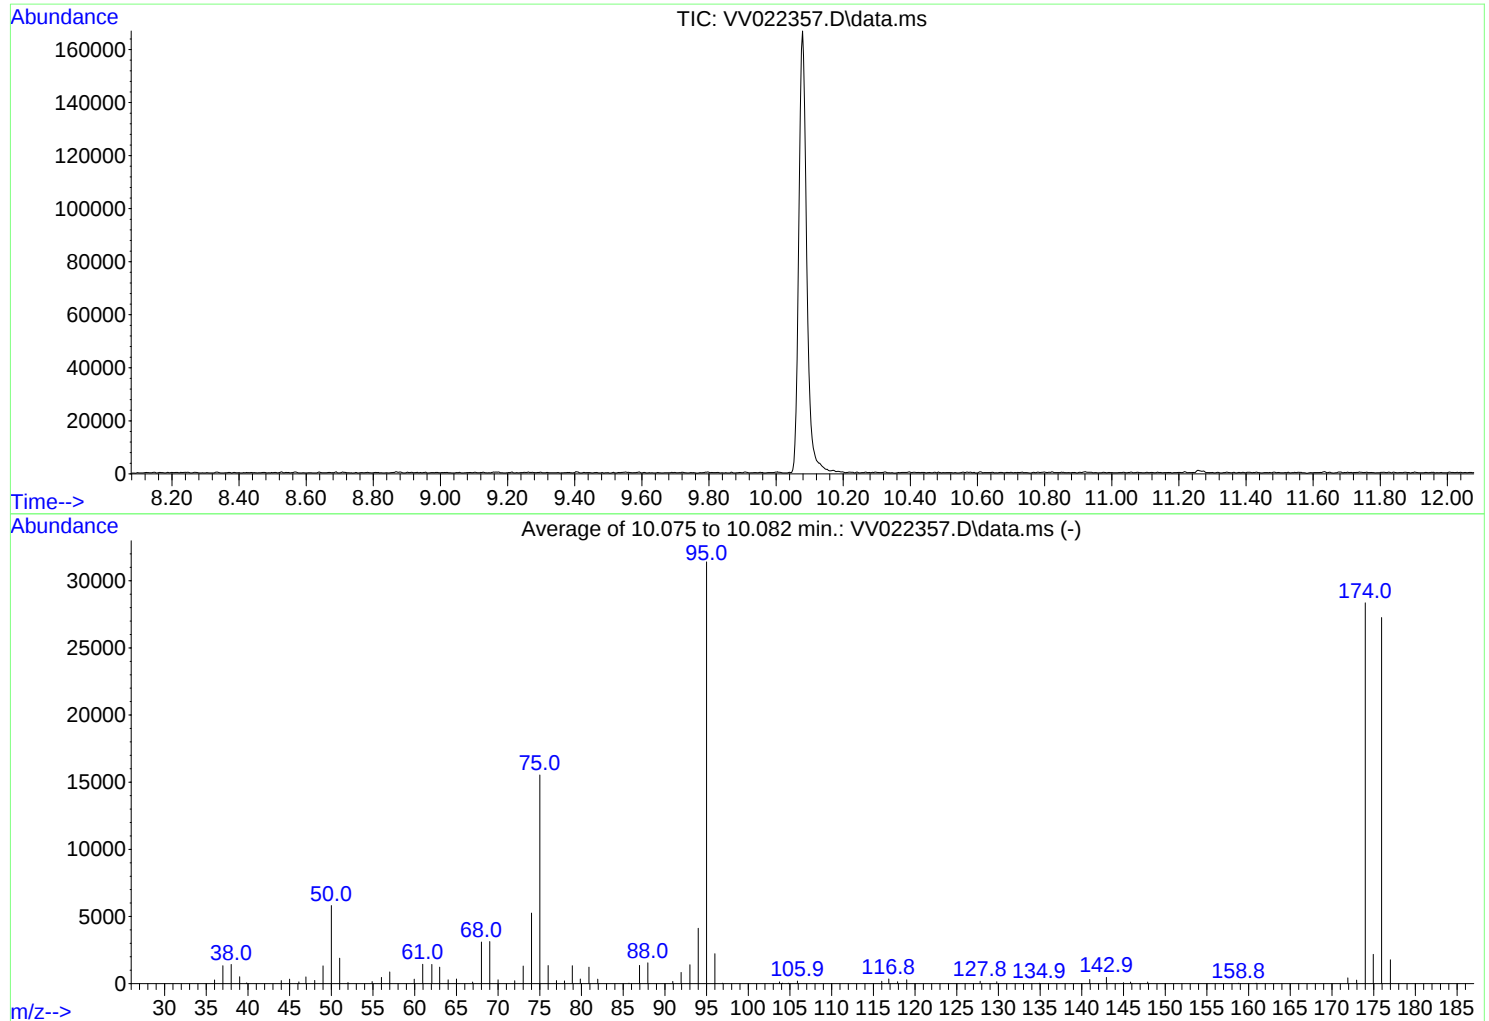

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5813	PASS
75	95	30	80	49.5	15535	PASS
95	95	100	100	100.0	31408	PASS
96	95	5	9	7.1	2229	PASS
173	174	0.00	2	0.9	259	PASS
174	95	50	120	90.3	28360	PASS
175	174	5	9	7.7	2180	PASS
176	174	95	105	96.1	27261	PASS
177	176	5	10	6.5	1772	PASS

m/z	Abundance
36.00	281.0
37.00	1357.0
38.00	1476.0
39.00	648.0
39.90	202.0
44.00	446.0
45.00	365.0
46.10	144.0
47.00	498.0
48.00	243.0
49.00	1402.0
50.00	5987.0
51.00	1967.0
52.00	115.0
54.90	159.0
56.00	461.0
57.00	880.0
59.90	338.0
61.00	1487.0
62.10	1492.0
63.00	1255.0
64.00	307.0
65.00	358.0
66.90	120.0
68.00	3209.0
69.00	3236.0
69.90	303.0
72.00	217.0
73.00	1320.0
74.00	5439.0
75.00	16158.0
76.00	1376.0
77.00	240.0
77.90	220.0
78.90	1374.0
79.90	351.0
80.90	1230.0
81.90	335.0
86.90	1393.0
87.90	1582.0
90.90	168.0
92.00	854.0
93.00	1430.0
94.00	4271.0
95.00	32336.0
96.00	2291.0
103.70	122.0
104.10	108.0
105.90	190.0
116.00	180.0
116.80	355.0
117.90	142.0
119.00	300.0
127.80	190.0
129.80	134.0
134.90	104.0
140.90	325.0
142.90	482.0
145.00	112.0
145.90	130.0
147.90	117.0
160.90	104.0
171.90	458.0
173.00	402.0
174.00	29320.0
175.00	2256.0
176.00	28288.0
177.00	1849.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	220.0
37.00	1212.0
38.00	1332.0
39.00	693.0
39.90	190.0
43.90	479.0
45.00	299.0
46.10	104.0
47.00	533.0
48.00	232.0
49.00	1236.0
50.00	5616.0
51.00	1740.0
54.90	157.0
56.00	494.0
57.00	876.0
59.90	347.0
61.00	1473.0
62.00	1368.0
63.00	1206.0
64.00	265.0
65.00	329.0
67.00	126.0
68.00	2933.0
69.00	2957.0
70.00	297.0
72.00	185.0
73.00	1199.0
74.00	5159.0
75.00	15144.0
76.00	1272.0
77.00	230.0
78.00	166.0
78.90	1278.0
79.80	376.0
80.90	1198.0
82.00	312.0
86.90	1319.0
88.00	1447.0
90.90	182.0
91.90	824.0
93.00	1313.0
94.00	4052.0
95.00	30568.0
96.00	2209.0
103.70	114.0
105.90	201.0
116.00	189.0
116.90	327.0
117.80	165.0
119.00	257.0
127.80	185.0
129.80	144.0
140.90	277.0
142.90	456.0
145.00	118.0
145.80	113.0
147.90	119.0
171.90	466.0
174.00	27936.0
175.00	2109.0
176.00	27536.0
177.00	1722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

Scan 2800 (10.043 min): VV022357.D\data.ms
BFB236

m/z	Abundance
39.10	112.0
39.80	151.0
44.10	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	321.0
37.00	1420.0
38.00	1475.0
39.00	546.0
39.90	223.0
44.00	446.0
45.00	352.0
46.10	150.0
46.90	479.0
48.00	242.0
49.00	1347.0
50.00	5836.0
51.00	1976.0
52.00	134.0
54.90	135.0
56.00	449.0
57.00	858.0
60.00	306.0
60.90	1376.0
62.00	1437.0
63.00	1214.0
64.00	278.0
65.00	337.0
66.90	103.0
68.00	3160.0
69.00	3201.0
70.10	265.0
72.00	227.0
73.00	1423.0
74.00	5151.0
75.00	15304.0
76.00	1381.0
77.00	222.0
77.90	219.0
78.90	1356.0
79.90	316.0
80.90	1246.0
81.90	361.0
85.70	118.0
87.00	1381.0
87.90	1625.0
91.00	156.0
92.00	828.0
93.00	1474.0
94.00	4048.0
95.00	31320.0
96.00	2187.0
96.90	124.0
103.80	141.0
104.80	108.0
105.90	174.0
116.00	157.0
116.80	351.0
118.10	108.0
119.00	308.0
127.80	169.0
129.80	151.0
141.00	331.0
143.00	466.0
145.90	110.0
147.90	110.0
158.80	107.0
171.90	347.0
172.90	374.0
174.00	27824.0
174.90	2174.0
175.90	25960.0
177.00	1745.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236