

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092920\
 Data File : VV018539.D
 Acq On : 30 Sep 2020 00:35
 Operator : SY/MD
 Sample : L4141-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FG7

Quant Time: Sep 30 05:33:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 30 04:50:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	387792	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	373830	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	191021	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	103688	45.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.18%
7) Chloroethane-d5	1.58	69	96186	51.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.30%
11) 1,1-Dichloroethene-d2	2.12	63	166068	35.84	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.68%
21) 2-Butanone-d5	3.92	46	174986	103.15	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.15%
24) Chloroform-d	4.38	84	228800	46.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.04%
26) 1,2-Dichloroethane-d4	5.06	65	154802	49.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.16%
32) Benzene-d6	5.08	84	473295	49.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.96%
36) 1,2-Dichloropropane-d6	6.09	67	146460	51.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.38%
41) Toluene-d8	7.34	98	427548	47.99	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.98%
43) trans-1,3-Dichloropropene-	7.64	79	70057	45.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.66%
47) 2-Hexanone-d5	8.11	63	95456	87.84	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.84%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	168925	44.53	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.06%
64) 1,2-Dichlorobenzene-d4	11.65	152	189932	51.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	8631	5.889 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092920\
Data File : VV018539.D
Acq On : 30 Sep 2020 00:35
Operator : SY/MD
Sample : L4141-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FG7

Quant Time: Sep 30 05:33:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 30 04:50:47 2020
Response via : Initial Calibration

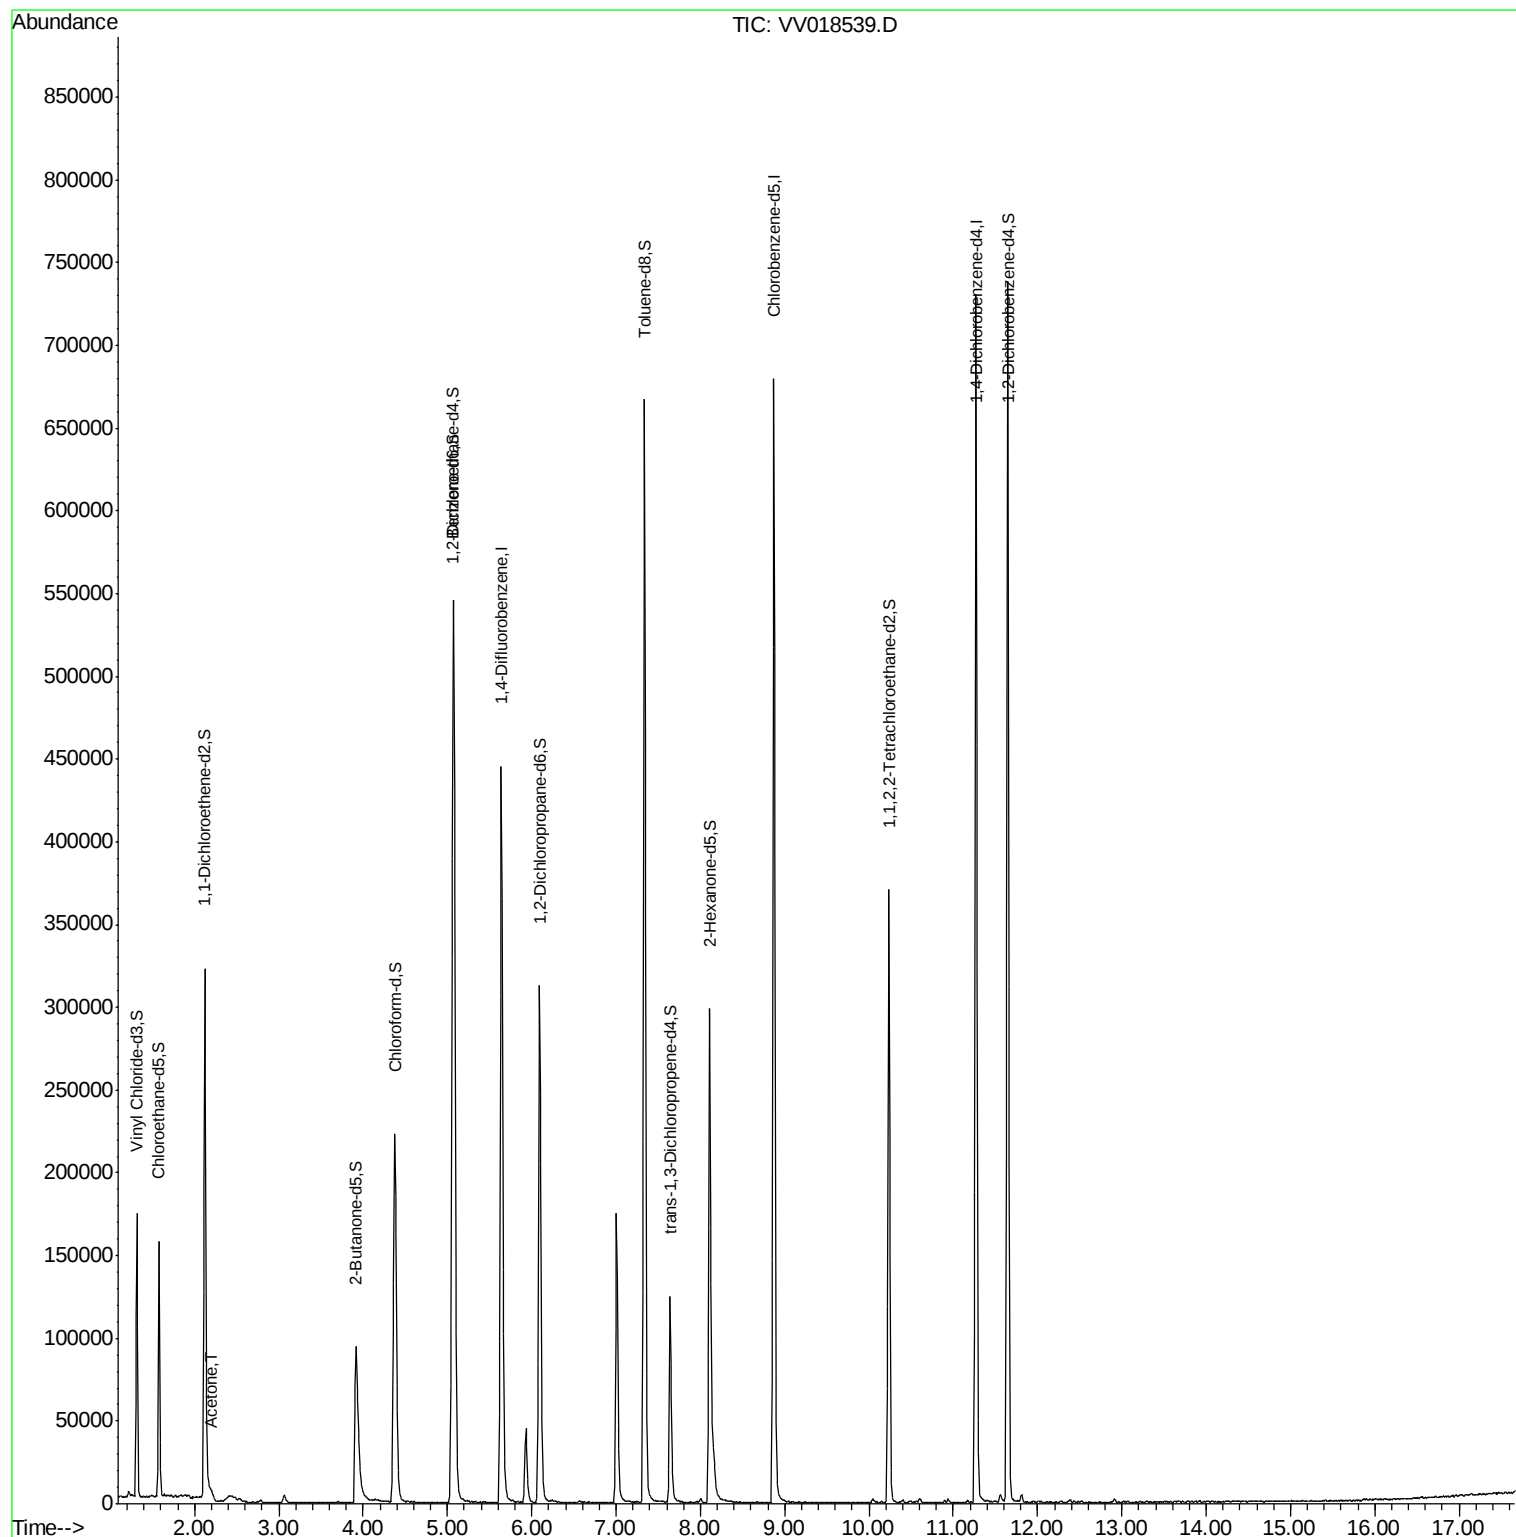

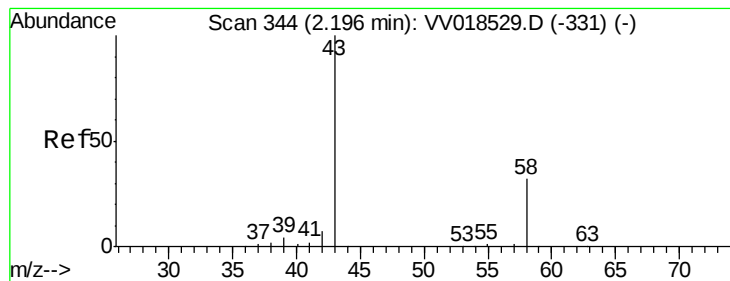

#13
 Acetone
 Concen: 5.889 ug/L
 RT: 2.20 min Scan# 346
 Delta R.T. 0.01 min
 Lab File: VV018539.D
 Acq: 30 Sep 2020 00:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FG7

Tot Ion: 43 Resp: 8631
 Ion Ratio Lower Upper
 43 100
 58 18.4 0.0 64.0

