


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092920\
 Data File : VV018507.D
 Acq On : 29 Sep 2020 09:48
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 30 04:50:47 2020

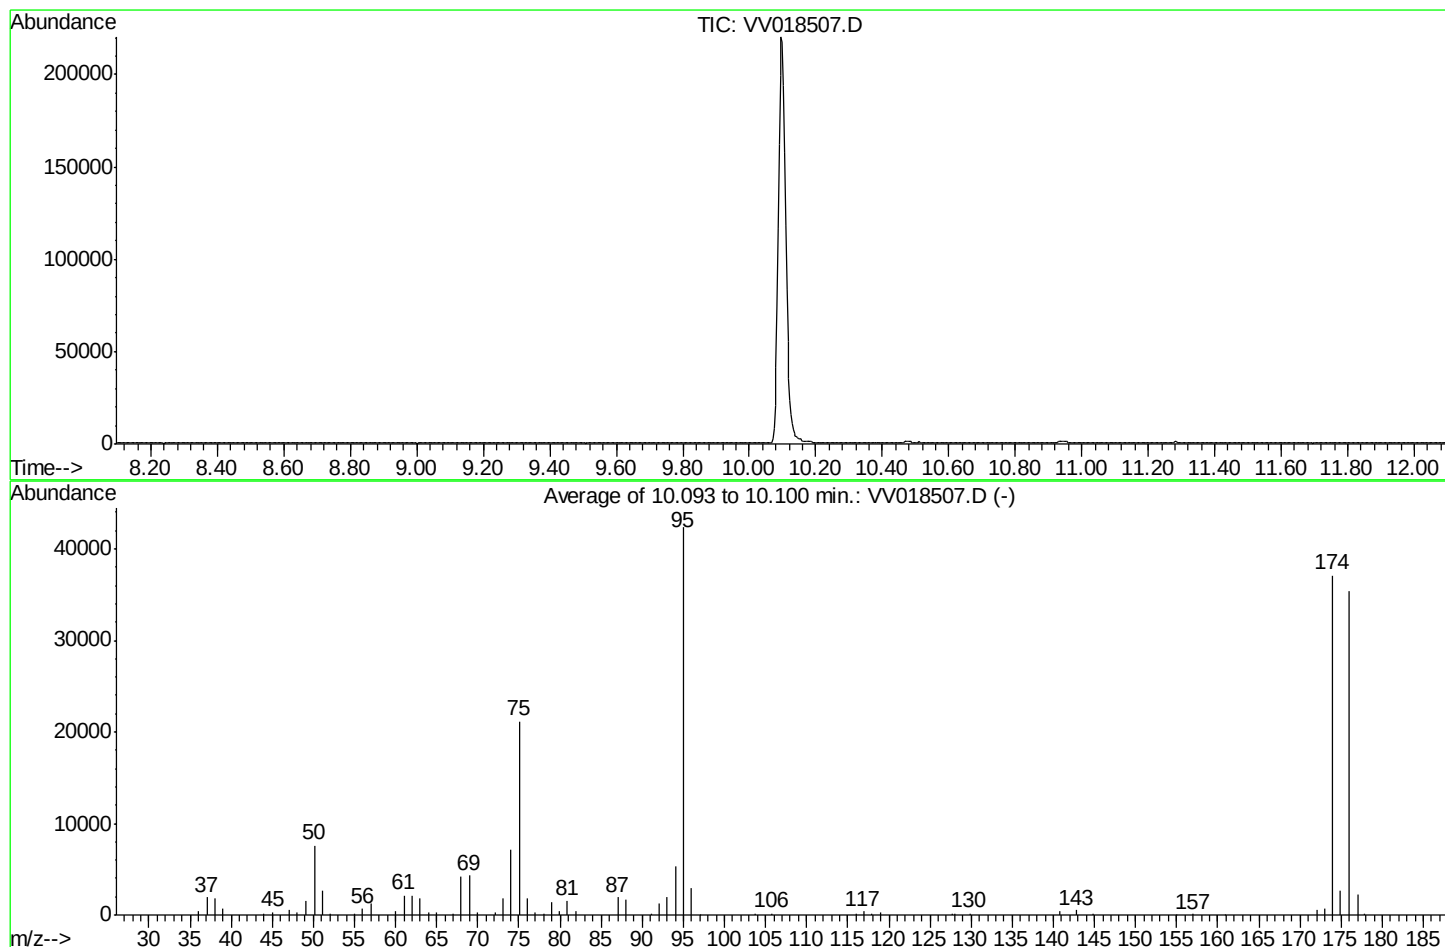

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	7616	PASS
75	95	30	80	49.9	21157	PASS
95	95	100	100	100.0	42357	PASS
96	95	5	9	7.0	2974	PASS
173	174	0.00	2	1.9	693	PASS
174	95	50	120	87.7	37130	PASS
175	174	5	9	7.2	2656	PASS
176	174	95	101	95.5	35445	PASS
177	176	5	9	6.5	2302	PASS

m/z	Abundance
36.00	360.0
37.00	1802.0
38.10	1730.0
39.00	754.0
40.00	136.0
44.00	439.0
45.00	300.0
47.00	555.0
48.00	258.0
49.00	1447.0
50.10	7441.0
51.10	2522.0
55.10	153.0
56.00	636.0
57.00	1168.0
60.10	385.0
61.00	2048.0
62.00	1926.0
63.00	1815.0
64.00	250.0
64.90	313.0
67.00	119.0
68.00	3947.0
69.00	4239.0
70.00	324.0
72.10	324.0
73.10	1801.0
74.00	6762.0
75.10	19808.0
76.00	1850.0
76.90	301.0
78.00	162.0
78.90	1290.0
79.90	467.0
80.90	1475.0
81.90	305.0
87.00	1729.0
88.00	1564.0
91.10	192.0
92.00	1297.0
93.00	1832.0
94.00	5076.0
95.00	40288.0
96.00	2879.0
103.80	178.0
105.80	213.0
116.00	161.0
116.90	334.0
117.90	136.0
119.00	256.0
127.80	129.0
129.90	175.0
140.90	467.0
142.90	536.0
144.90	156.0
155.00	120.0
157.00	104.0
172.00	523.0
173.00	659.0
174.00	34256.0
174.90	2383.0
176.00	32424.0
177.00	2180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	371.0
37.00	1974.0
38.00	1858.0
39.00	800.0
39.90	149.0
44.00	444.0
45.10	302.0
47.00	610.0
48.00	284.0
49.10	1531.0
50.10	7885.0
51.10	2727.0
52.00	133.0
55.00	142.0
56.00	668.0
57.00	1292.0
60.10	482.0
61.00	2216.0
62.00	2125.0
63.00	1886.0
64.00	254.0
65.00	313.0
67.00	124.0
68.00	4408.0
69.00	4412.0
70.00	329.0
72.10	352.0
73.00	1892.0
74.00	7332.0
75.00	21864.0
76.10	1932.0
77.00	346.0
78.00	193.0
78.90	1440.0
79.90	518.0
80.90	1670.0
81.90	379.0
87.00	1983.0
88.00	1686.0
91.10	228.0
92.00	1319.0
93.00	2010.0
94.00	5481.0
95.00	43848.0
96.00	3101.0
103.80	213.0
105.80	223.0
116.00	189.0
116.90	377.0
117.90	141.0
119.00	263.0
127.70	120.0
128.10	145.0
129.90	187.0
140.80	498.0
142.80	571.0
144.90	188.0
155.00	102.0
157.00	151.0
160.90	104.0
172.00	574.0
173.00	746.0
174.00	38400.0
175.00	2735.0
176.00	36672.0
177.00	2373.0
177.80	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.10	355.0
37.10	1950.0
38.00	1754.0
39.00	755.0
40.00	167.0
44.00	428.0
45.10	316.0
47.00	550.0
48.10	317.0
49.00	1498.0
50.10	7522.0
51.00	2605.0
52.00	133.0
55.00	120.0
56.00	644.0
57.00	1160.0
60.00	514.0
61.00	2185.0
62.00	2051.0
63.00	1719.0
64.00	258.0
65.00	342.0
67.00	126.0
68.00	4375.0
69.00	4186.0
70.00	324.0
72.00	293.0
73.00	1807.0
74.00	7157.0
75.00	21800.0
76.00	1639.0
77.00	334.0
78.00	189.0
79.00	1419.0
79.90	483.0
80.90	1617.0
81.90	407.0
87.00	2011.0
87.90	1627.0
91.10	220.0
92.00	1238.0
93.00	1980.0
94.00	5219.0
95.00	42936.0
96.00	2943.0
97.00	103.0
103.80	230.0
105.80	199.0
116.00	203.0
116.90	391.0
117.90	132.0
119.00	237.0
128.00	155.0
129.80	190.0
140.80	485.0
142.80	568.0
144.90	185.0
157.00	159.0
172.00	582.0
173.00	676.0
174.00	38736.0
175.00	2850.0
176.00	37240.0
177.00	2354.0
177.80	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Scan 2790 (10.061 min): VV018507.D
BFB62

m/z	Abundance
39.90	155.0
44.00	357.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62