

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022372.D
 Acq On : 29 Sep 2021 12:56
 Operator : SY/MD
 Sample : VV0929MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Quant Time: Sep 30 05:27:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 30 05:14:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	256244	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	242953	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	108435	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	94030	43.240	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.480%		
7) Chloroethane-d5	1.561	69	80228	46.644	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.280%		
11) 1,1-Dichloroethene-d2	2.105	63	127428	33.703	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.400%		
21) 2-Butanone-d5	3.873	46	148497	96.759	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.760%		
24) Chloroform-d	4.346	84	181317	46.175	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.340%		
26) 1,2-Dichloroethane-d4	5.030	65	111033	46.109	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.220%		
32) Benzene-d6	5.050	84	364950	47.749	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.500%		
36) 1,2-Dichloropropane-d6	6.069	67	118919	48.634	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.260%		
41) Toluene-d8	7.317	98	322706	46.129	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.260%		
43) trans-1,3-Dichloroprop...	7.622	79	49233	44.094	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.180%		
47) 2-Hexanone-d5	8.088	63	96657	97.284	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.280%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	162667	45.829	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.660%		
66) 1,2-Dichlorobenzene-d4	11.625	152	126179	52.331	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.660%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.622	75	2466	0.922	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022372.D
Acq On : 29 Sep 2021 12:56
Operator : SY/MD
Sample : VV0929MBL01
Misc : 5.00g/5.0ml/100ul/5.0ml/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Time: Sep 30 05:27:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 30 05:14:53 2021
Response via : Initial Calibration

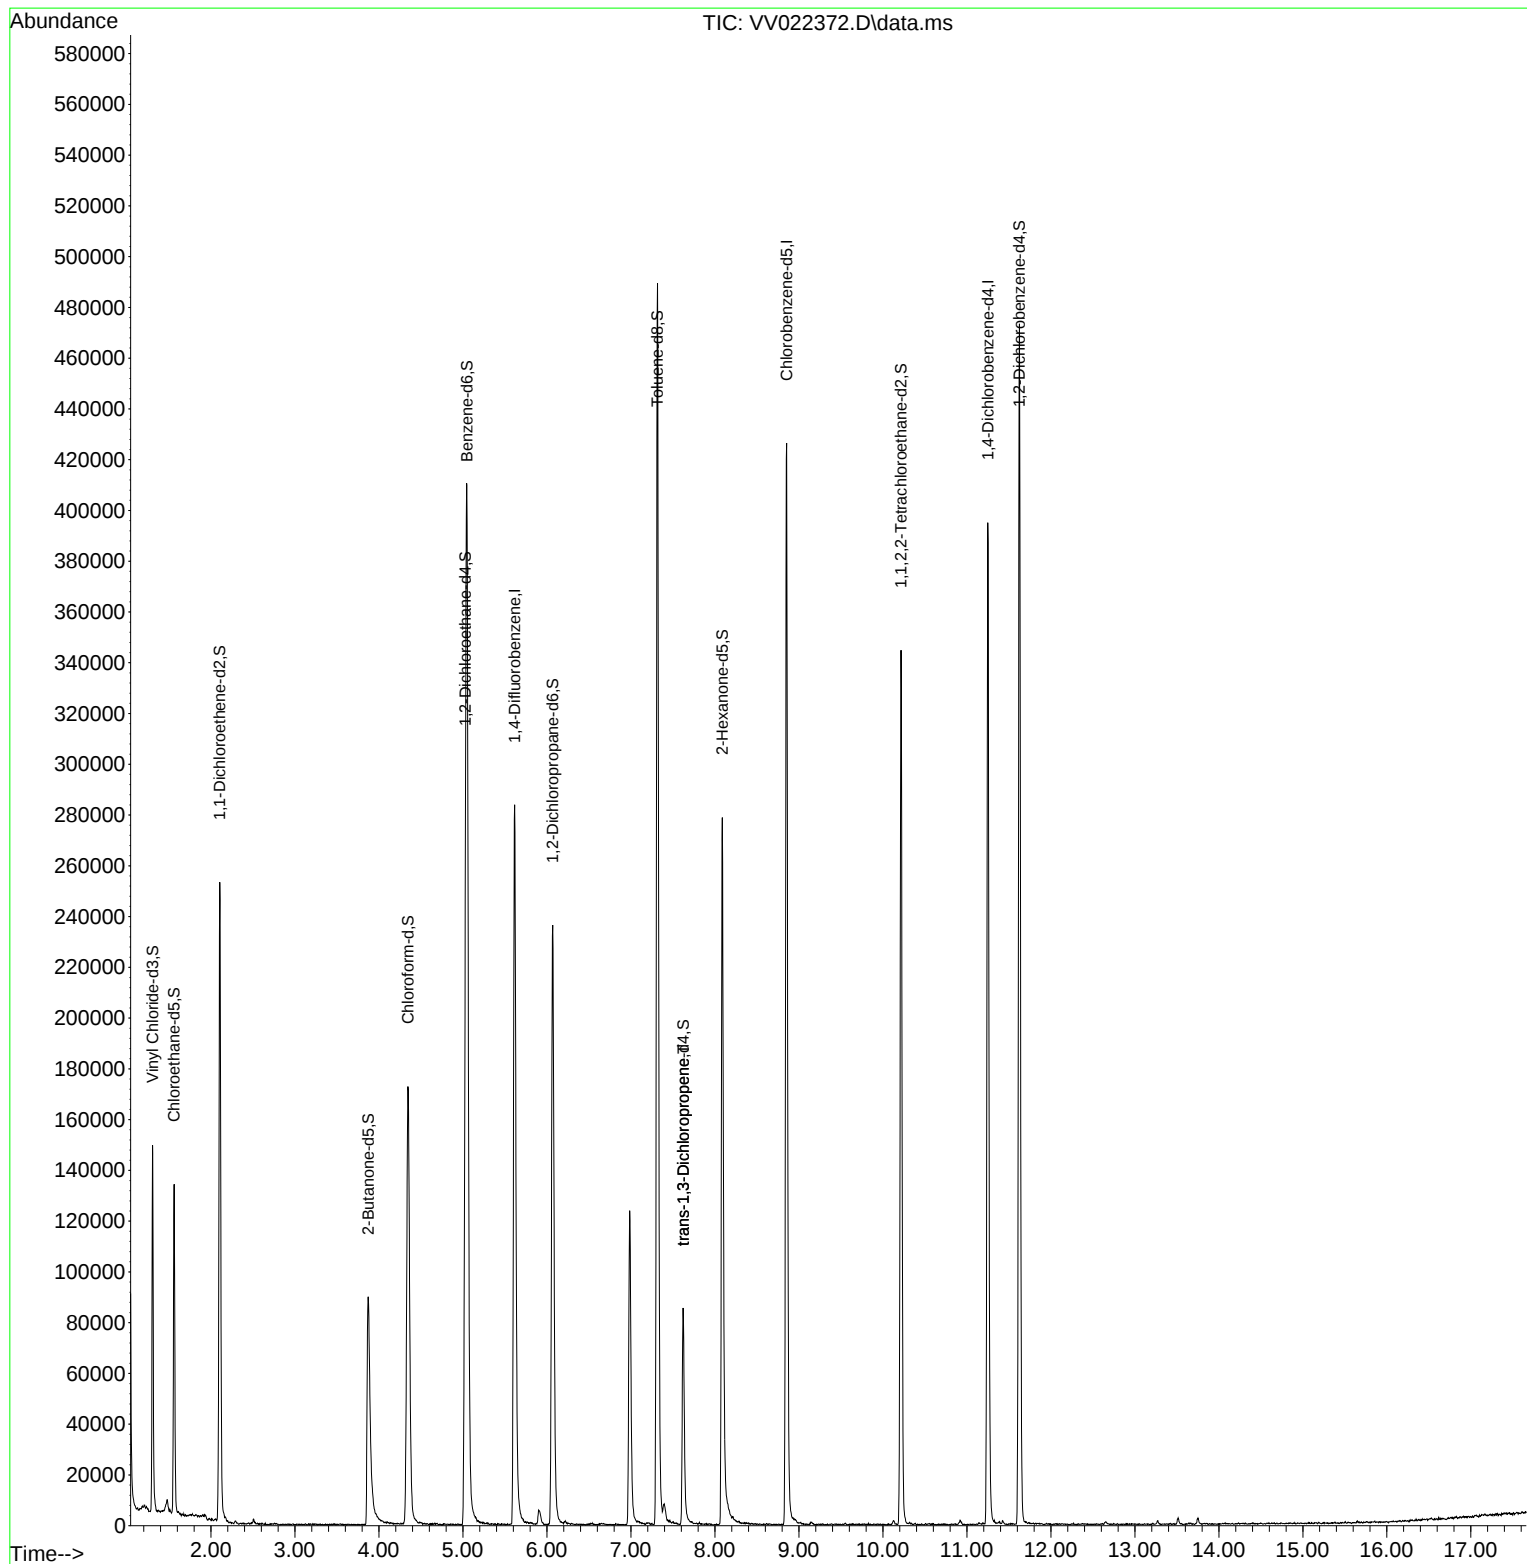

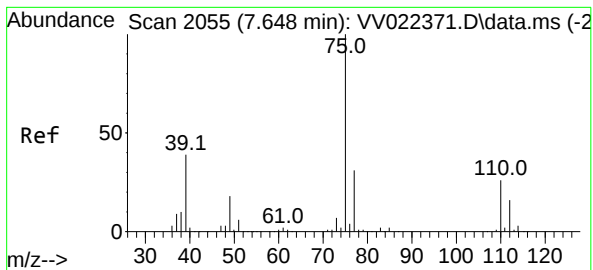

#44
 trans-1,3-Dichloropropene
 Concen: 0.922 ug/L
 RT: 7.622 min Scan# 2047
 Delta R.T. -0.026 min
 Lab File: VV022372.D
 Acq: 29 Sep 2021 12:56

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Tgt Ion: 75 Resp: 2466
 Ion Ratio Lower Upper
 75 100
 77 33.2 22.3 41.3

