

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022396.D
 Acq On : 29 Sep 2021 22:56
 Operator : SY/MD
 Sample : VV0929WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 30 06:56:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 30 06:55:59 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	250984	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	234607	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	102831	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	91232	42.832	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.660%
7) Chloroethane-d5	1.564	69	78287	46.469	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.940%
11) 1,1-Dichloroethene-d2	2.105	63	128503	34.700	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.400%
21) 2-Butanone-d5	3.905	46	160232	106.593	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.590%
24) Chloroform-d	4.349	84	180997	47.059	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.120%
26) 1,2-Dichloroethane-d4	5.034	65	115556	48.993	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.980%
32) Benzene-d6	5.050	84	374966	50.805	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.072	67	121982	51.662	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.320%
41) Toluene-d8	7.317	98	325970	48.254	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.500%
43) trans-1,3-Dichloroprop...	7.622	79	47288	43.859	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.720%
47) 2-Hexanone-d5	8.092	63	105303	109.756	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.760%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	164300	47.936	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.880%
66) 1,2-Dichlorobenzene-d4	11.625	152	128538	56.214	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.420%
Target Compounds						
35) Methylcyclohexane	6.072	83	28090	9.903	ug/L #	20
37) 1,2-Dichloropropane	6.069	63	12924	7.034	ug/L #	86
48) 2-Hexanone	8.092	43	11655	5.936	ug/L #	68
61) 1,2,3-Trichloropropane	11.249	75	11983	6.246	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022396.D
Acq On : 29 Sep 2021 22:56
Operator : SY/MD
Sample : VV0929WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 30 06:56:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 30 06:55:59 2021
Response via : Initial Calibration

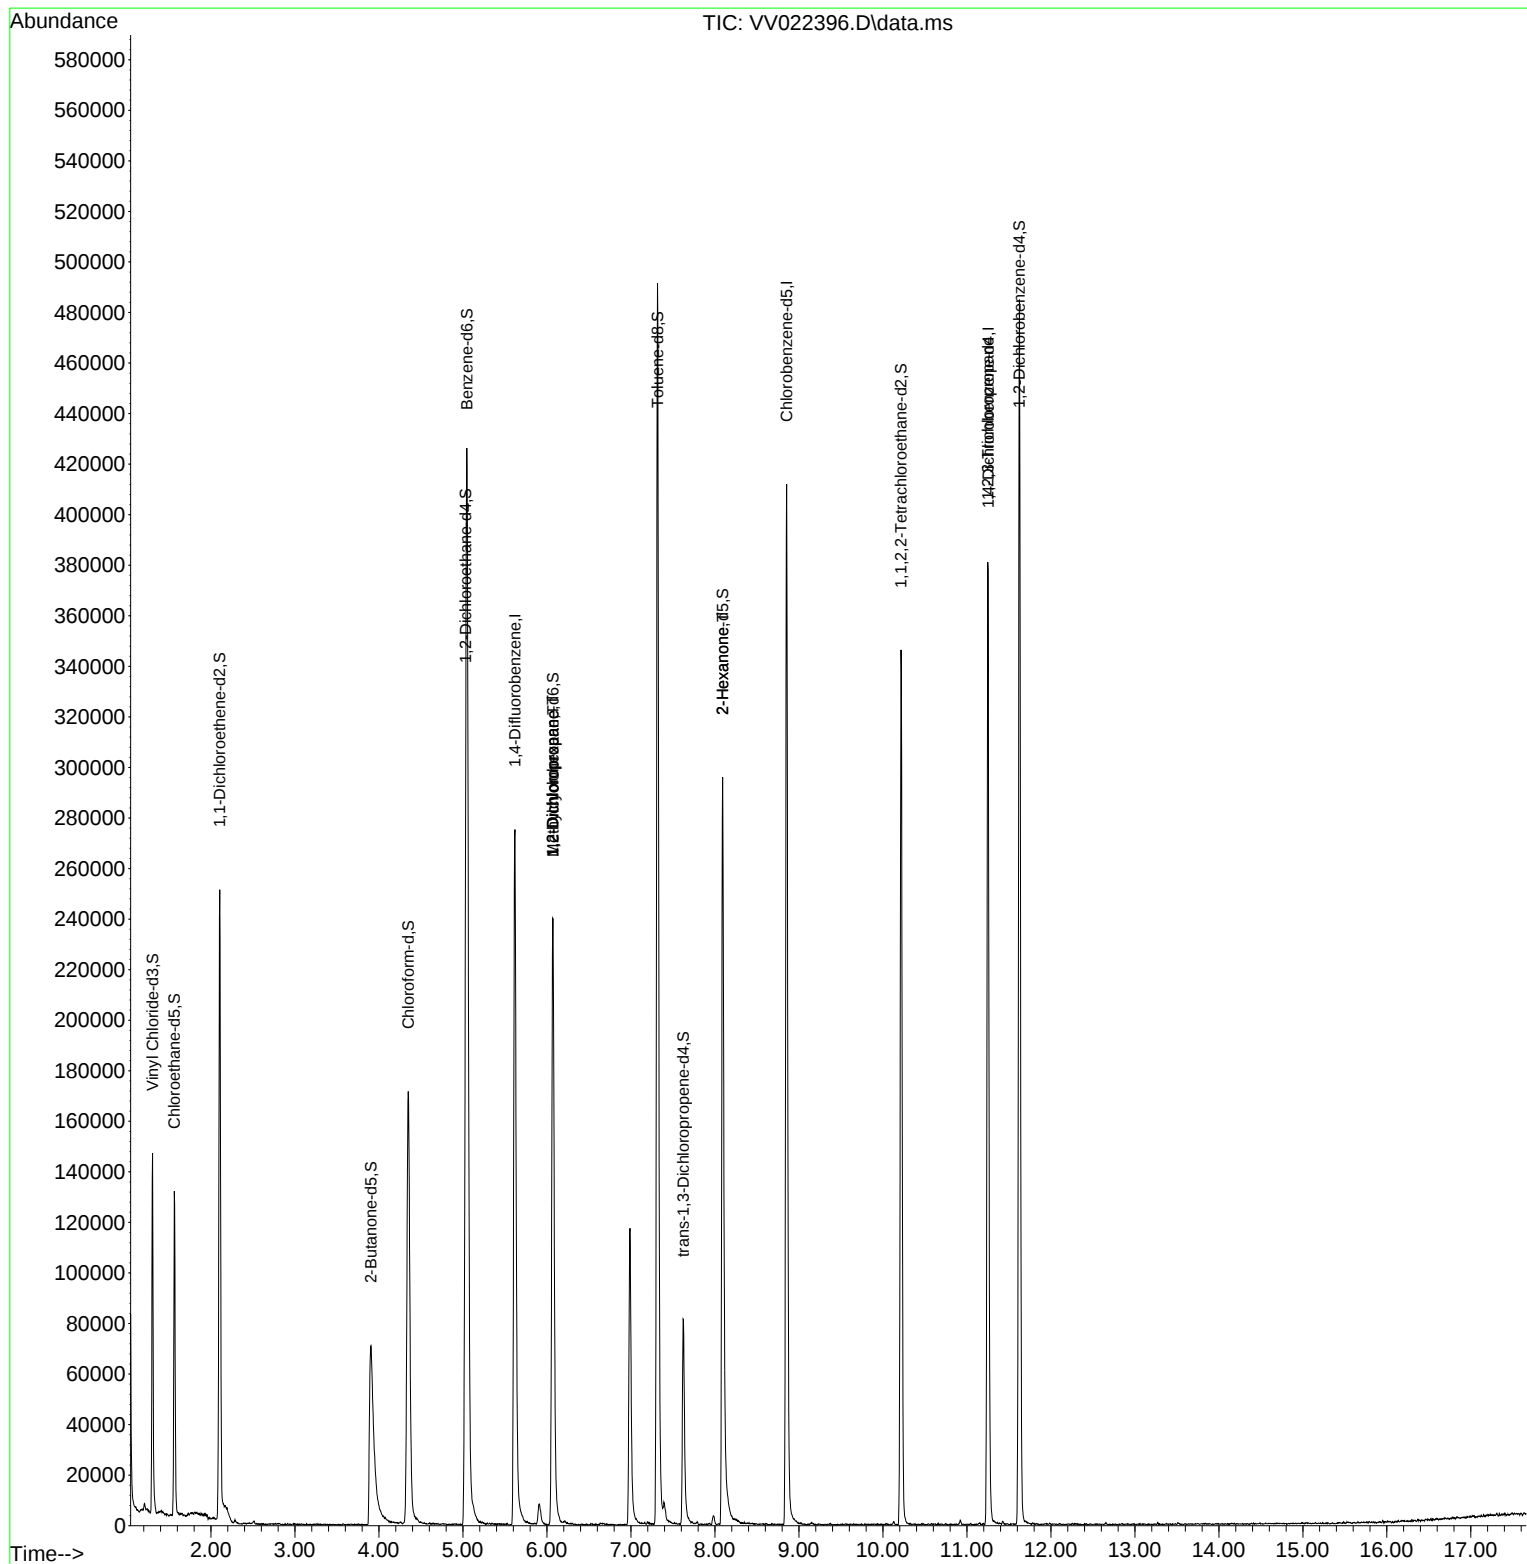

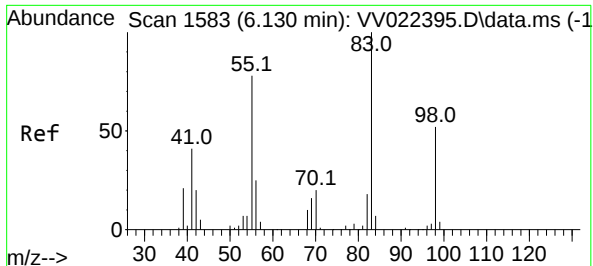

#35

Methylcyclohexane

Concen: 9.903 ug/L

RT: 6.072 min Scan# 1565





Delta R.T. -0.058 min

Lab File: VV022396.D

Acq: 29 Sep 2021 22:56

Tgt Ion:	83	Resp:	28090
Ion Ratio	Lower	Upper	
83	100		
55	0.3	58.6	87.8#
98	1.9	39.2	58.8#

Instrument :
MSVOA_V
ClientSampled :

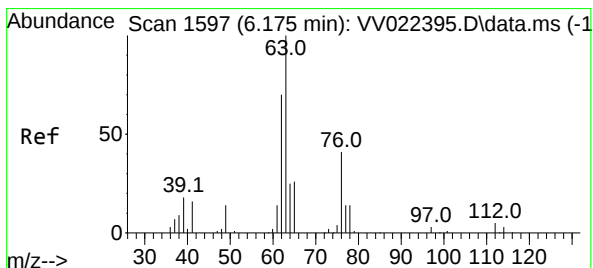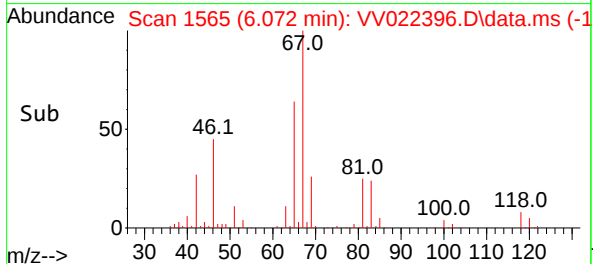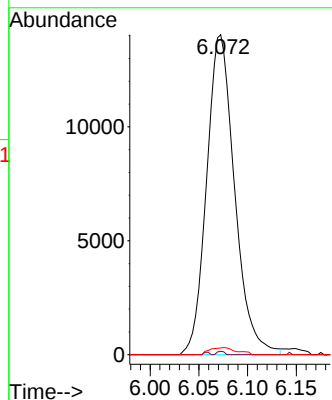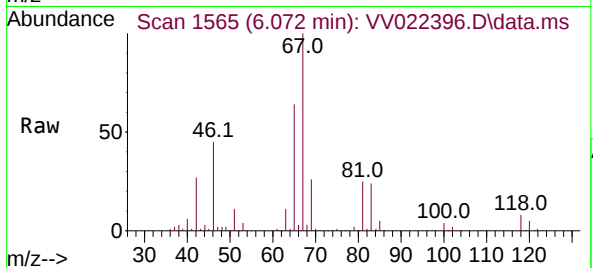

#37

1,2-Dichloropropane

Concen: 7.034 ug/L




RT: 6.069 min Scan# 1564


Delta R.T. -0.106 min

Lab File: VV022396.D

Acq: 29 Sep 2021 22:56

Tgt Ion:	63	Resp:	12924
Ion Ratio	Lower	Upper	
63	100		
112	0.3	3.9	5.9#


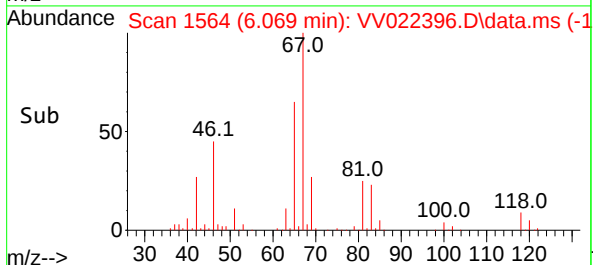
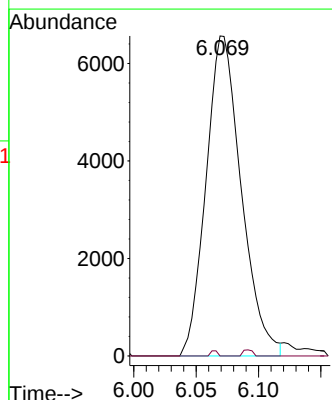
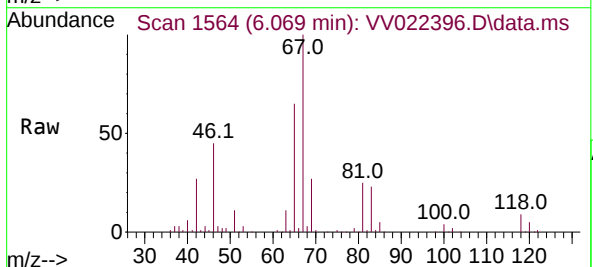


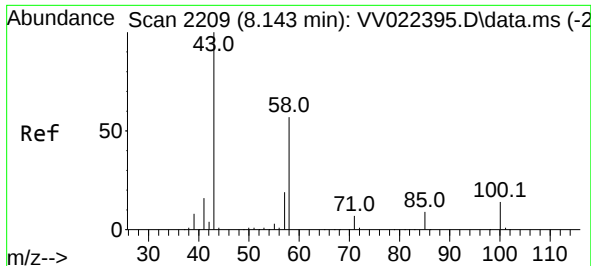

#48
2-Hexanone
Concen: 5.936 ug/L
RT: 8.092 min Scan# 2193
Delta R.T. -0.051 min
Lab File: VV022396.D
Acq: 29 Sep 2021 22:56

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
43	100		
58	31.6	45.4	68.2#
57	31.9	15.0	22.4#
100	1.9	10.7	16.1#

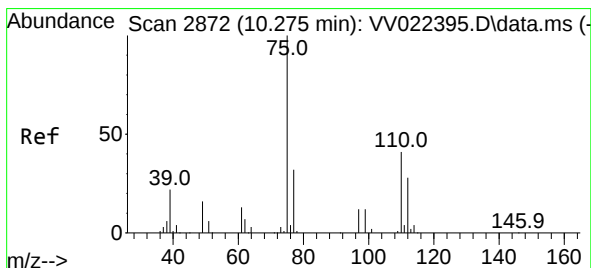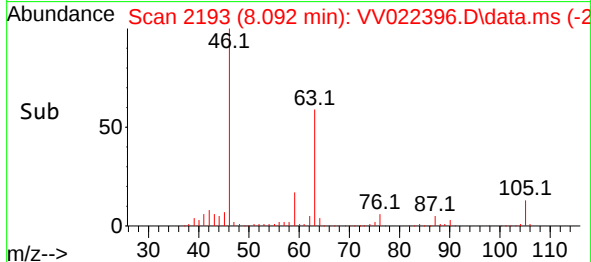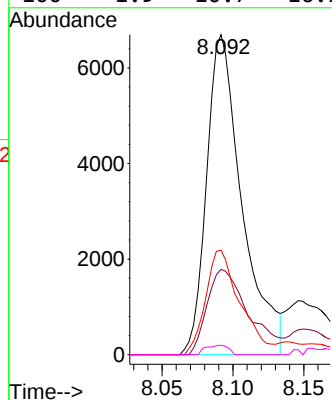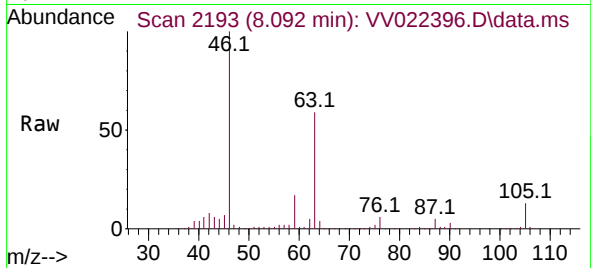

#61
1,2,3-Trichloropropane
Concen: 6.246 ug/L
RT: 11.249 min Scan# 3175
Delta R.T. 0.974 min
Lab File: VV022396.D
Acq: 29 Sep 2021 22:56

Tgt Ion	Ratio	Lower	Upper
75	100		
77	32.9	25.4	38.0
110	1.9	32.6	48.8#

