


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022407.D
Acq On : 30 Sep 2021 03:20
Operator : SY/MD
Sample : M3979-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A08

Manual Integrations
APPROVED

MMDadoda
9/30/2021 1:55:11 PM

Quant Time: Sep 30 07:09:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 30 06:55:59 2021
Response via : Initial Calibration

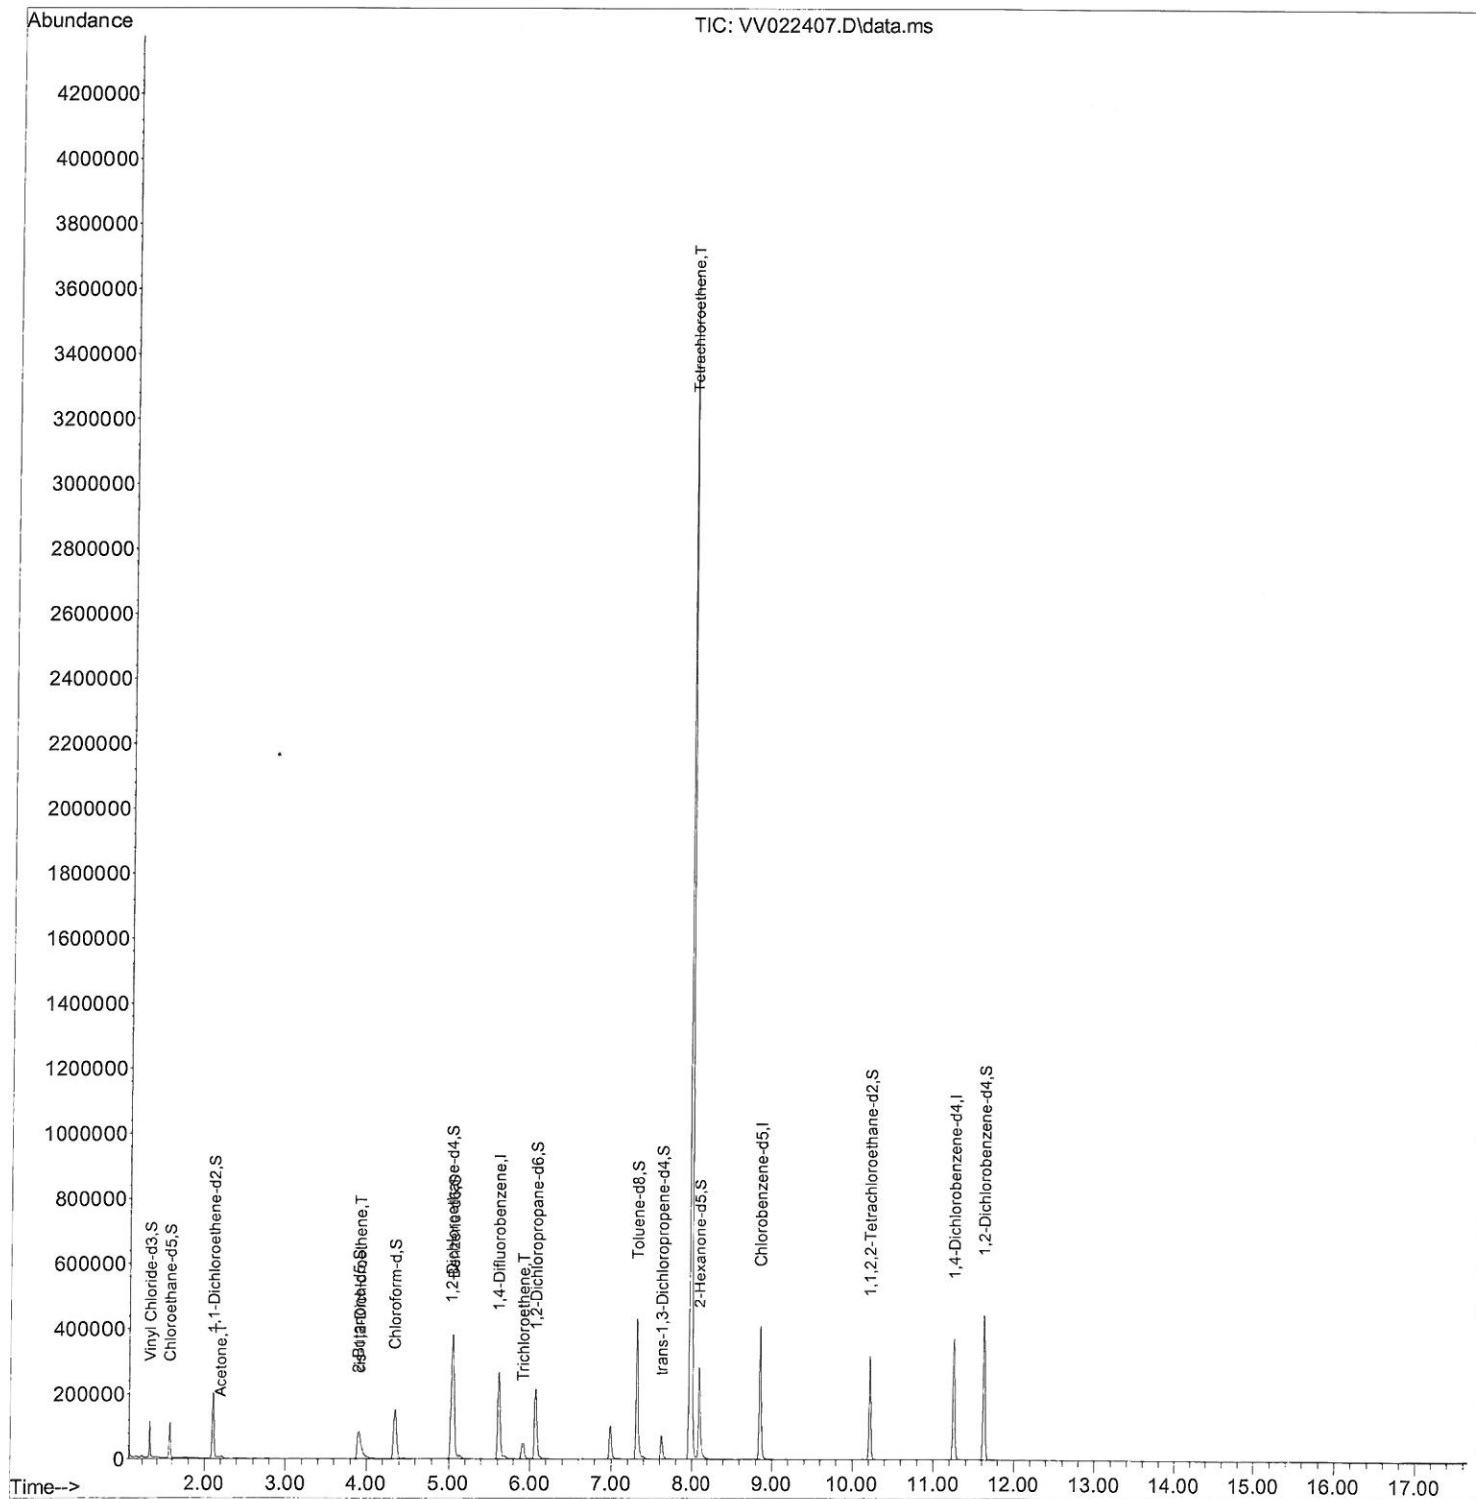

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022407.D
 Acq On : 30 Sep 2021 03:20
 Operator : SY/MD
 Sample : M3979-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A08

Manual Integrations
 APPROVED

MMDadoda
 9/30/2021 1:55:11 PM

Quant Time: Sep 30 07:09:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 30 06:55:59 2021
 Response via : Initial Calibration

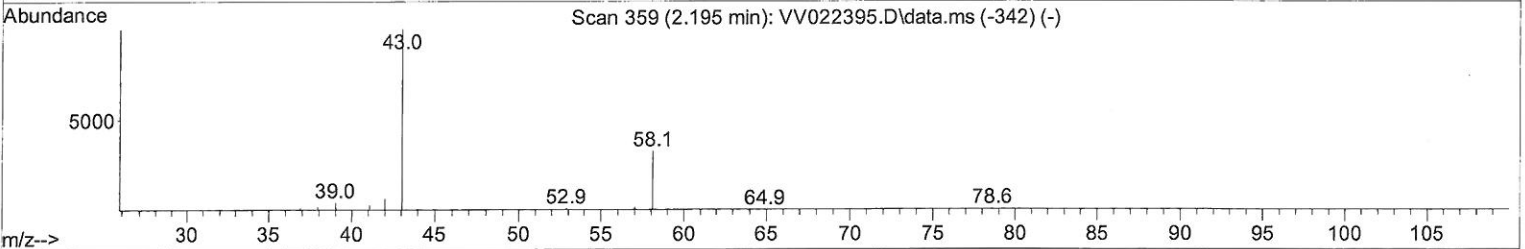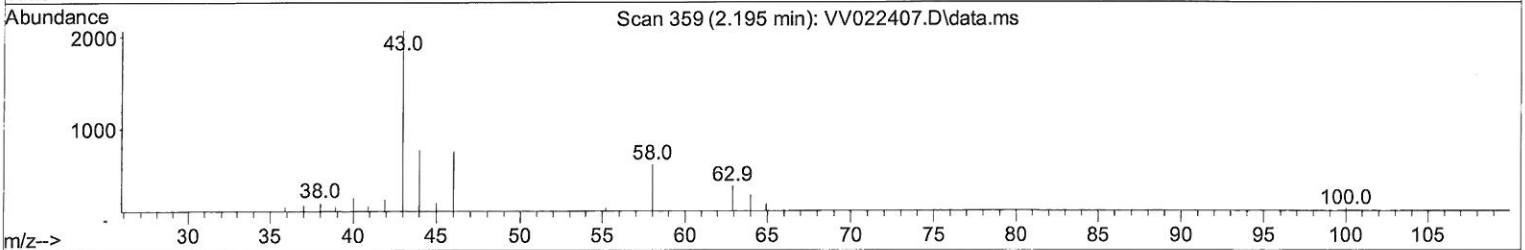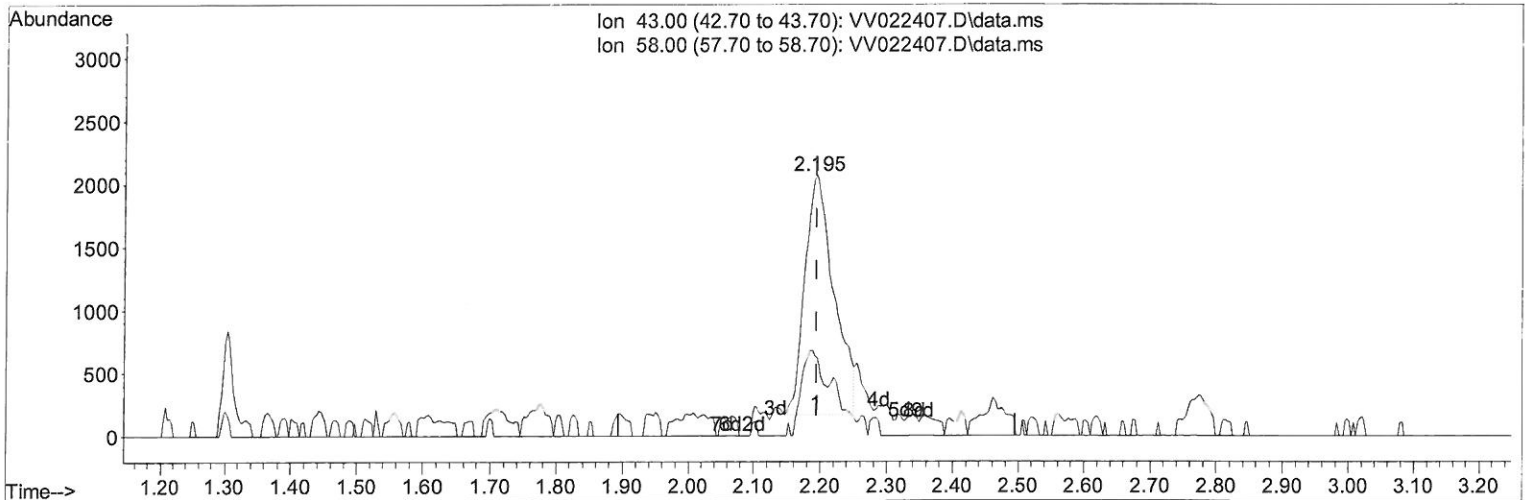

TIC: VV022407.D\data.ms

(13) Acetone (T)

2.195min (+ 0.000) 5.12 ug/L

response 5750

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	25.62
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022407.D
Acq On : 30 Sep 2021 03:20
Operator : SY/MD
Sample : M3979-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A08

Manual Integrations
APPROVED

MMDadoda
9/30/2021 1:55:11 PM

Quant Time: Sep 30 07:09:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 30 06:55:59 2021
Response via : Initial Calibration

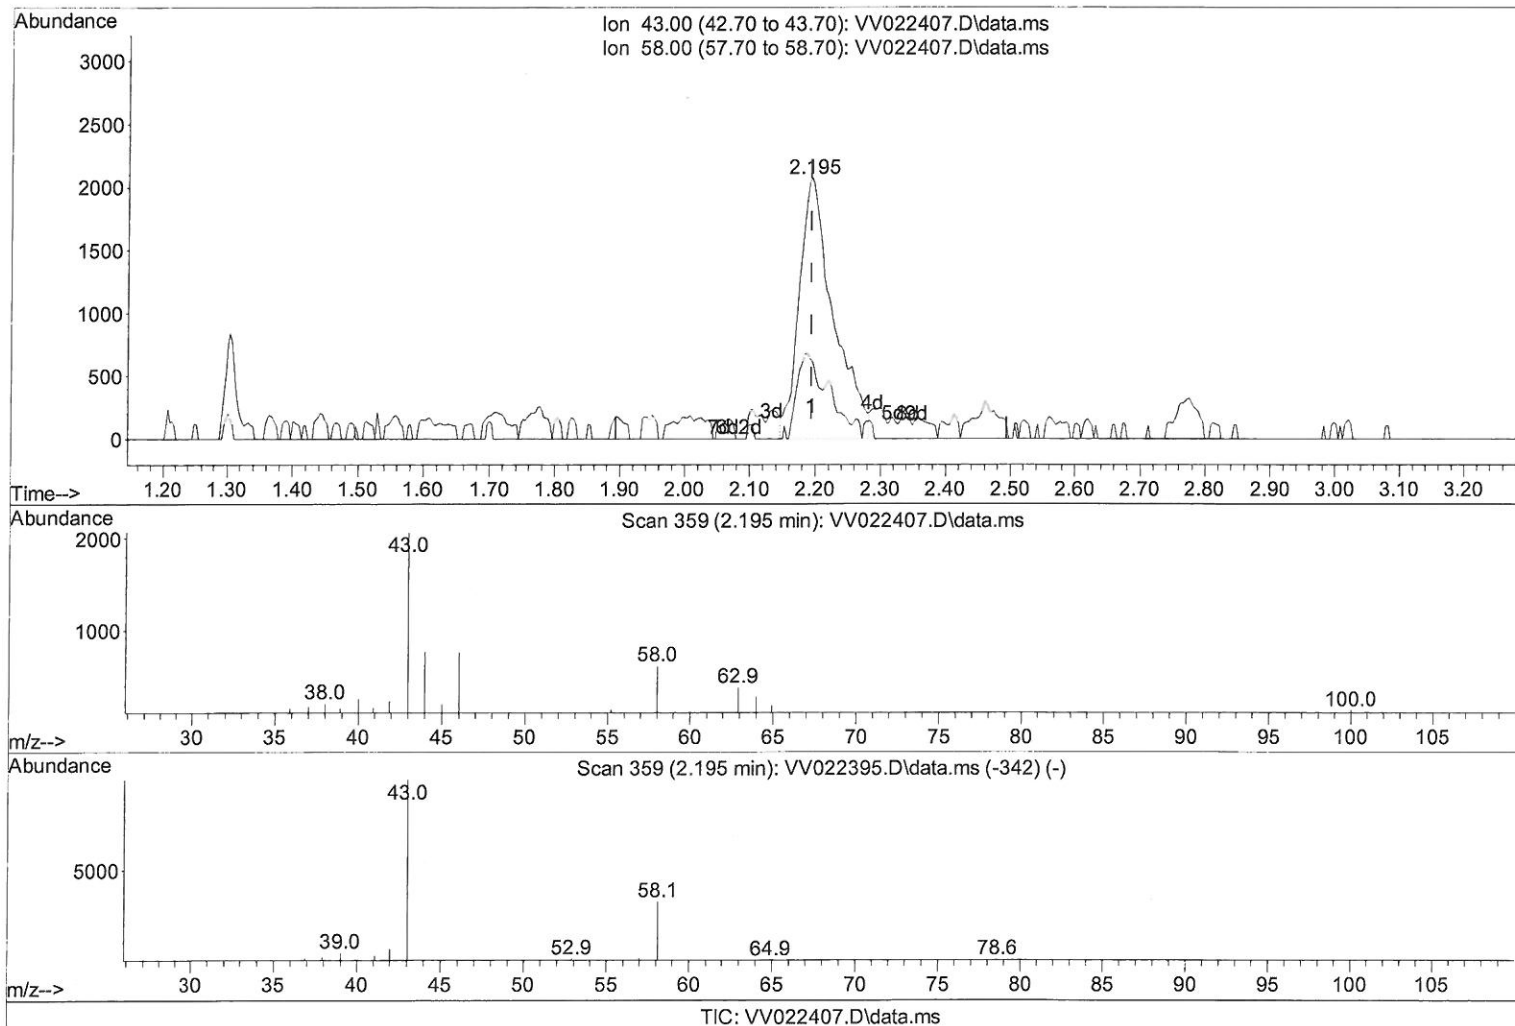

(13) Acetone (T)

2.195min (+ 0.000) 6.67 ug/L m

response 7490

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	19.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022407.D
 Acq On : 30 Sep 2021 03:20
 Operator : SY/MD
 Sample : M3979-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A08

Manual Integrations
 APPROVED

MMDadoda
 9/30/2021 1:55:11 PM

Quant Time: Sep 30 07:09:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 30 06:55:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	238941	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	239342	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	102089	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	70310	34.673	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	69.340%	
7) Chloroethane-d5	1.564	69	65673	40.947	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	81.900%	
11) 1,1-Dichloroethene-d2	2.101	63	104312	29.587	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	59.180%#	
21) 2-Butanone-d5	3.899	46	153409	107.198	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	107.200%	
24) Chloroform-d	4.349	84	161555	44.122	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.240%	
26) 1,2-Dichloroethane-d4	5.034	65	102810	45.786	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.580%	
32) Benzene-d6	5.050	84	330068	43.837	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.680%	
36) 1,2-Dichloropropane-d6	6.072	67	112166	46.565	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	93.120%	
41) Toluene-d8	7.317	98	297329	43.143	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.280%	
43) trans-1,3-Dichloroprop...	7.625	79	43695	39.724	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.440%	
47) 2-Hexanone-d5	8.092	63	103755	106.003	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	106.000%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	154270	44.119	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.240%	
66) 1,2-Dichlorobenzene-d4	11.625	152	115973	51.088	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.180%	
Target Compounds						
13) Acetone	2.195	43	7490m	6.668	ug/L	Qvalue
20) cis-1,2-Dichloroethene	3.912	96	7632	3.954	ug/L	92
34) Trichloroethene	5.918	95	18225	9.703	ug/L	97
46) Tetrachloroethene	7.976	164	838169	541.937	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed