

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022375.D
 Acq On : 29 Sep 2021 14:08
 Operator : SY/MD
 Sample : M3978-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A64

Quant Time: Sep 30 05:28:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 30 05:14:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	251073	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	237060	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	106621	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	89524	42.015	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.040%		
7) Chloroethane-d5	1.561	69	76425	45.348	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.700%		
11) 1,1-Dichloroethene-d2	2.105	63	124786	33.684	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.360%		
21) 2-Butanone-d5	3.873	46	144371	96.008	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.010%		
24) Chloroform-d	4.349	84	174530	45.362	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.720%		
26) 1,2-Dichloroethane-d4	5.034	65	109978	46.612	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.220%		
32) Benzene-d6	5.050	84	358582	48.082	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.160%		
36) 1,2-Dichloropropane-d6	6.069	67	116369	48.774	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.540%		
41) Toluene-d8	7.317	98	313249	45.891	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.780%		
43) trans-1,3-Dichloroprop...	7.622	79	48545	44.559	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.120%		
47) 2-Hexanone-d5	8.088	63	89715	92.541	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.540%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	159551	46.069	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.140%		
66) 1,2-Dichlorobenzene-d4	11.625	152	124315	52.435	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.860%		
Target Compounds					Qvalue	
13) Acetone	2.159	43	26497	22.451	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022375.D
Acq On : 29 Sep 2021 14:08
Operator : SY/MD
Sample : M3978-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A64

Quant Time: Sep 30 05:28:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 30 05:14:53 2021
Response via : Initial Calibration

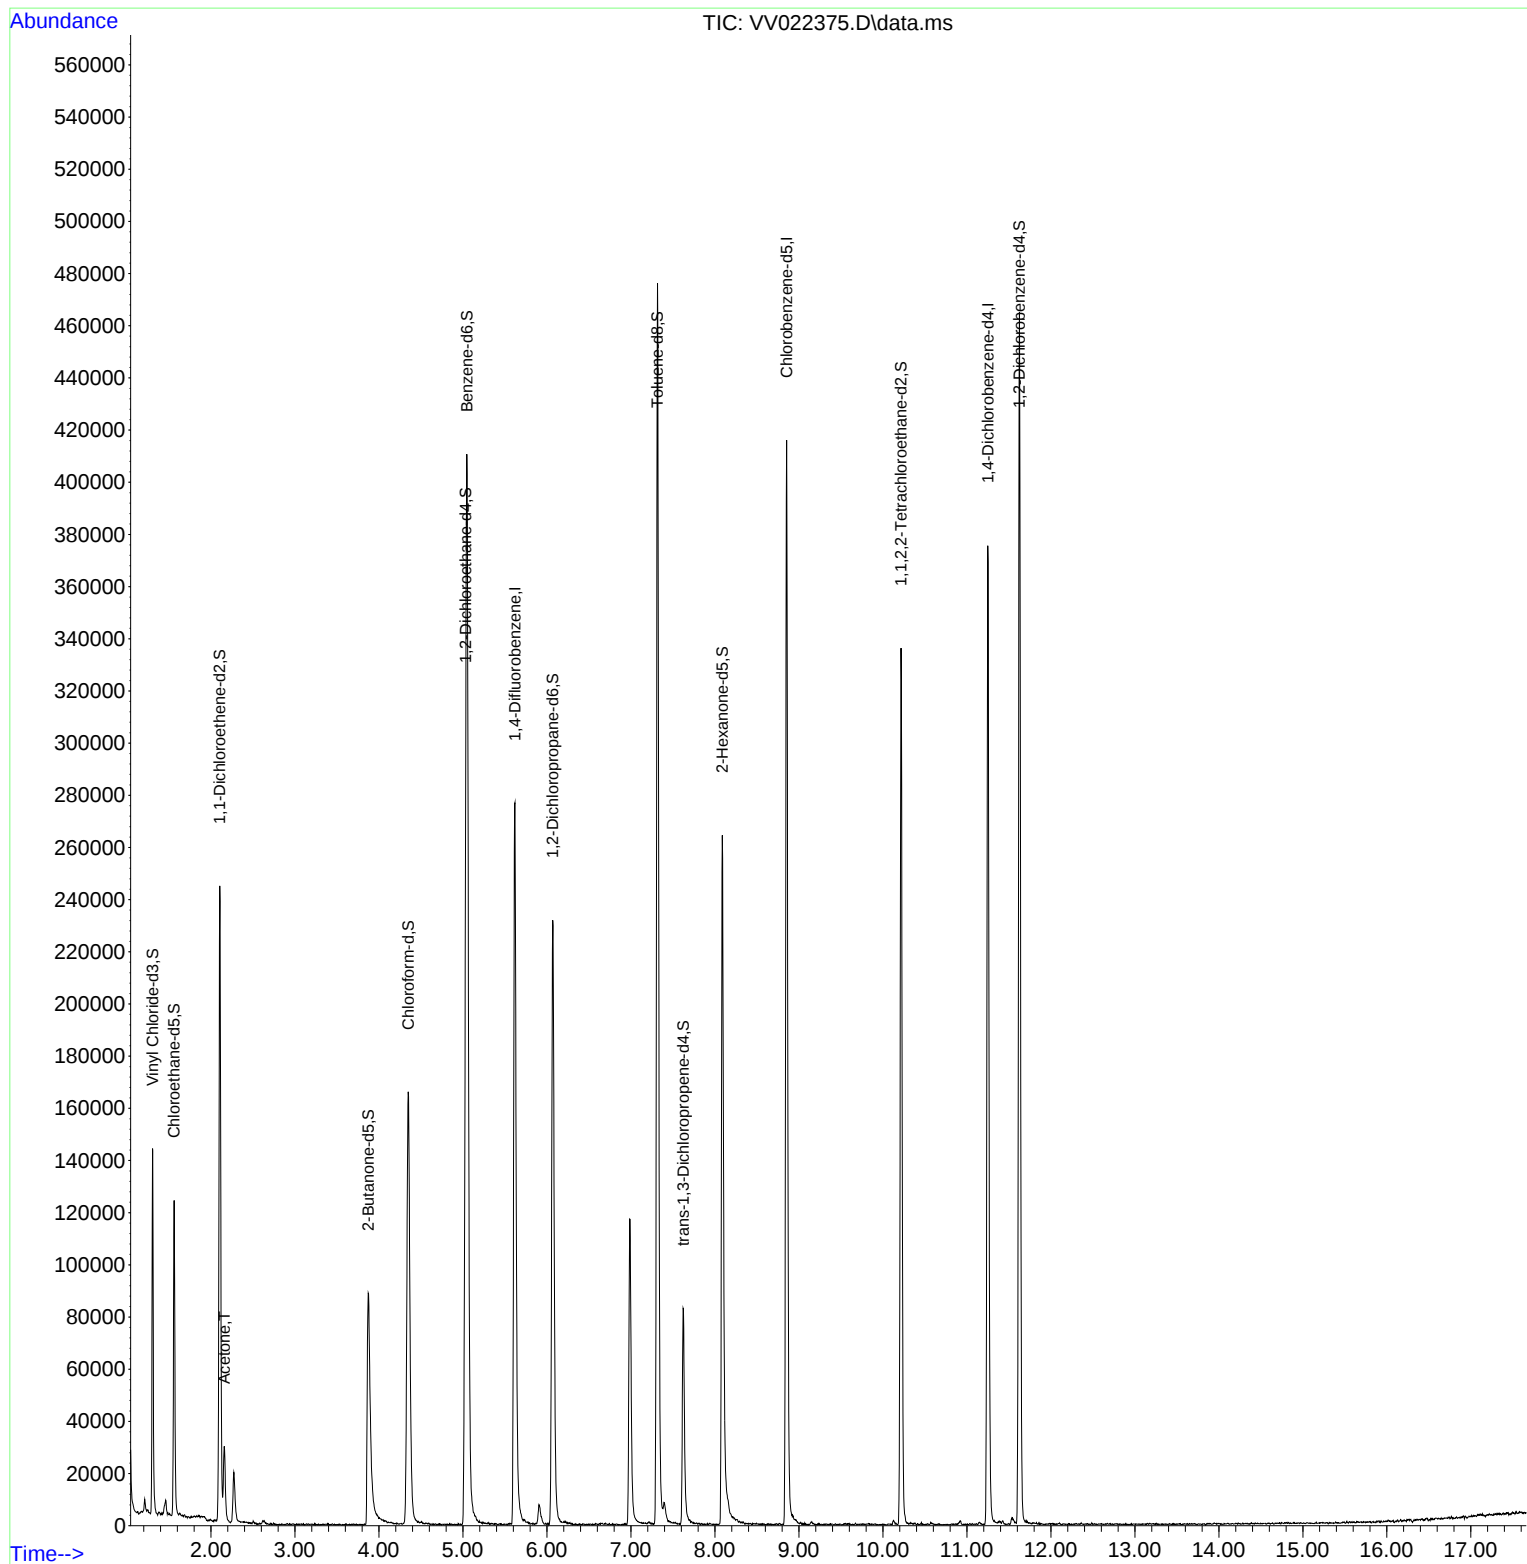

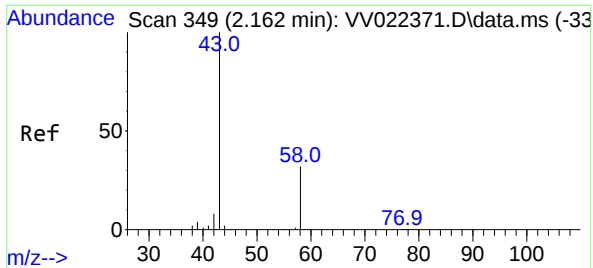

#13
 Acetone
 Concen: 22.451 ug/L
 RT: 2.159 min Scan# 348
 Delta R.T. -0.003 min
 Lab File: VV022375.D
 Acq: 29 Sep 2021 14:08

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A64

Tgt Ion:	43	Resp:	26497
Ion Ratio	Lower	Upper	
43	100		
58	31.8	0.0	67.2

