

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022373.D
 Acq On : 29 Sep 2021 13:20
 Operator : SY/MD
 Sample : VV0929WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	138364	143030	13.63%	1.851%
2	1.561	155	162	174	rVB	120841	140531	13.39%	1.818%
3	2.108	321	332	349	rBV	243731	360686	34.38%	4.667%
4	2.503	449	455	457	rBV5	1353	1462	0.14%	0.019%
5	2.664	503	505	509	rVB3	360	255	0.02%	0.003%
6	2.828	553	556	560	rVB2	204	183	0.02%	0.002%
7	2.908	577	581	583	rBV3	397	273	0.03%	0.004%
8	2.979	601	603	606	rVB	526	196	0.02%	0.003%
9	3.185	665	667	672	rVB	369	221	0.02%	0.003%
10	3.214	673	676	682	rVB3	308	324	0.03%	0.004%
11	3.391	727	731	734	rBV2	316	223	0.02%	0.003%
12	3.410	734	737	739	rBV2	264	169	0.02%	0.002%
13	3.522	767	772	774	rBV2	240	172	0.02%	0.002%
14	3.535	774	776	780	rVB2	401	194	0.02%	0.003%
15	3.564	781	785	787	rVB2	332	174	0.02%	0.002%
16	3.873	871	881	909	rBV	94277	247065	23.55%	3.197%
17	4.349	1014	1029	1056	rBV	165278	412307	39.30%	5.335%
18	4.632	1115	1117	1123	rVB4	446	315	0.03%	0.004%
19	4.670	1127	1129	1132	rBV2	346	227	0.02%	0.003%
20	4.725	1141	1146	1148	rBV2	500	327	0.03%	0.004%
21	4.744	1150	1152	1155	rVB	597	264	0.03%	0.003%
22	4.783	1155	1164	1167	rVB2	205	232	0.02%	0.003%
23	4.805	1167	1171	1174	rBV2	348	318	0.03%	0.004%
24	4.873	1189	1192	1196	rBV2	246	270	0.03%	0.003%
25	4.915	1201	1205	1209	rVB	343	267	0.03%	0.003%
26	4.956	1216	1218	1223	rVB3	283	171	0.02%	0.002%
27	5.046	1229	1246	1281	rBV2	407882	1049227	100.00%	13.576%
28	5.275	1315	1317	1321	rBV2	504	255	0.02%	0.003%
29	5.448	1367	1371	1372	rBV2	331	199	0.02%	0.003%
30	5.619	1412	1424	1454	rBV	275800	566450	53.99%	7.330%
31	5.911	1505	1515	1529	rBV6	6239	12732	1.21%	0.165%
32	6.069	1551	1564	1593	rBV	231580	480830	45.83%	6.222%
33	6.323	1641	1643	1649	rVB4	436	411	0.04%	0.005%
34	6.532	1705	1708	1711	rBV3	378	304	0.03%	0.004%
35	6.606	1728	1731	1735	rVB2	342	187	0.02%	0.002%
36	6.641	1739	1742	1743	rBV2	447	231	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022373.D
 Acq On : 29 Sep 2021 13:20
 Operator : SY/MD
 Sample : VV0929WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.693	1755	1758	1764	rBV4	511	406	0.04%	0.005%
38	6.741	1767	1773	1775	rVB3	268	216	0.02%	0.003%
39	6.847	1804	1806	1811	rBV2	299	226	0.02%	0.003%
40	6.889	1817	1819	1824	rVB2	396	218	0.02%	0.003%
41	6.931	1829	1832	1835	rBV2	272	168	0.02%	0.002%
42	6.989	1839	1850	1871	rBV	118873	218883	20.86%	2.832%
43	7.316	1940	1952	1970	rBV	470563	821523	78.30%	10.630%
44	7.622	2037	2047	2065	rBV2	82984	148030	14.11%	1.915%
45	7.873	2122	2125	2127	rVB3	295	182	0.02%	0.002%
46	7.943	2145	2147	2149	rBV	337	193	0.02%	0.002%
47	7.979	2155	2158	2167	rVB2	435	469	0.04%	0.006%
48	8.021	2167	2171	2173	rBV3	488	360	0.03%	0.005%
49	8.088	2181	2192	2224	rBV	285862	508943	48.51%	6.585%
50	8.371	2276	2280	2282	rBV3	489	393	0.04%	0.005%
51	8.442	2297	2302	2303	rBV3	409	316	0.03%	0.004%
52	8.461	2306	2308	2313	rVB2	510	369	0.04%	0.005%
53	8.500	2316	2320	2323	rVB2	524	274	0.03%	0.004%
54	8.538	2328	2332	2333	rBV2	339	226	0.02%	0.003%
55	8.564	2336	2340	2342	rBV	276	199	0.02%	0.003%
56	8.593	2346	2349	2350	rBV2	396	191	0.02%	0.002%
57	8.638	2360	2363	2365	rBV	518	251	0.02%	0.003%
58	8.693	2378	2380	2384	rVB3	535	368	0.04%	0.005%
59	8.802	2412	2414	2418	rVB3	395	239	0.02%	0.003%
60	8.853	2418	2430	2455	rBV	421723	690063	65.77%	8.929%
61	9.104	2506	2508	2510	rVB	609	254	0.02%	0.003%
62	9.120	2510	2513	2516	rBV2	404	302	0.03%	0.004%
63	9.140	2516	2519	2520	rBV2	354	199	0.02%	0.003%
64	9.201	2536	2538	2541	rVB	324	192	0.02%	0.002%
65	9.213	2541	2542	2547	rBV	334	223	0.02%	0.003%
66	9.365	2583	2589	2591	rBV2	263	311	0.03%	0.004%
67	9.455	2612	2617	2622	rVB3	250	291	0.03%	0.004%
68	9.548	2642	2646	2647	rBV	256	175	0.02%	0.002%
69	9.750	2706	2709	2711	rBV	366	178	0.02%	0.002%
70	9.940	2766	2768	2775	rVB2	347	226	0.02%	0.003%
71	9.976	2776	2779	2783	rVB	355	219	0.02%	0.003%
72	10.062	2802	2806	2807	rBV	272	177	0.02%	0.002%
73	10.130	2819	2827	2834	rBV4	1876	2639	0.25%	0.034%
74	10.217	2843	2854	2877	rVB	346820	540421	51.51%	6.993%
75	10.603	2973	2974	2978	rBV2	404	246	0.02%	0.003%
76	10.635	2982	2984	2987	rVB3	389	195	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022373.D
 Acq On : 29 Sep 2021 13:20
 Operator : SY/MD
 Sample : VV0929WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	10.651	2987	2989	2993	rBV3	387	355	0.03%	0.005%
78	10.693	3000	3002	3006	rVB2	306	172	0.02%	0.002%
79	10.747	3016	3019	3023	rBV2	254	207	0.02%	0.003%
80	10.892	3061	3064	3065	rVV2	463	233	0.02%	0.003%
81	10.918	3066	3072	3083	rVB7	1486	2695	0.26%	0.035%
82	11.101	3126	3129	3132	rVV	246	188	0.02%	0.002%
83	11.143	3138	3142	3146	rBV3	708	650	0.06%	0.008%
84	11.252	3164	3176	3201	rBV	389812	610452	58.18%	7.899%
85	11.625	3280	3292	3309	rBV	476515	750063	71.49%	9.705%
86	11.818	3348	3352	3354	rVB3	319	194	0.02%	0.003%
87	11.898	3375	3377	3380	rBV2	335	215	0.02%	0.003%
88	12.020	3413	3415	3419	rVB2	407	212	0.02%	0.003%
89	12.101	3437	3440	3446	rVB3	665	524	0.05%	0.007%
90	12.139	3450	3452	3456	rVB2	413	172	0.02%	0.002%
91	12.197	3468	3470	3473	rVB3	376	170	0.02%	0.002%
92	12.358	3518	3520	3523	rBV3	306	209	0.02%	0.003%
93	12.532	3571	3574	3578	rBV3	468	319	0.03%	0.004%
94	12.943	3700	3702	3706	rVB	395	191	0.02%	0.002%
95	13.149	3763	3766	3772	rBV2	313	251	0.02%	0.003%
96	13.236	3791	3793	3796	rBV	415	227	0.02%	0.003%
97	13.834	3977	3979	3980	rBV	386	173	0.02%	0.002%
98	14.149	4073	4077	4078	rBV	327	239	0.02%	0.003%
99	14.426	4161	4163	4167	rBV2	415	261	0.02%	0.003%
100	15.175	4394	4396	4399	rBV2	633	340	0.03%	0.004%


Sum of corrected areas: 7728348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022373.D
Acq On : 29 Sep 2021 13:20
Operator : SY/MD
Sample : VV0929WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

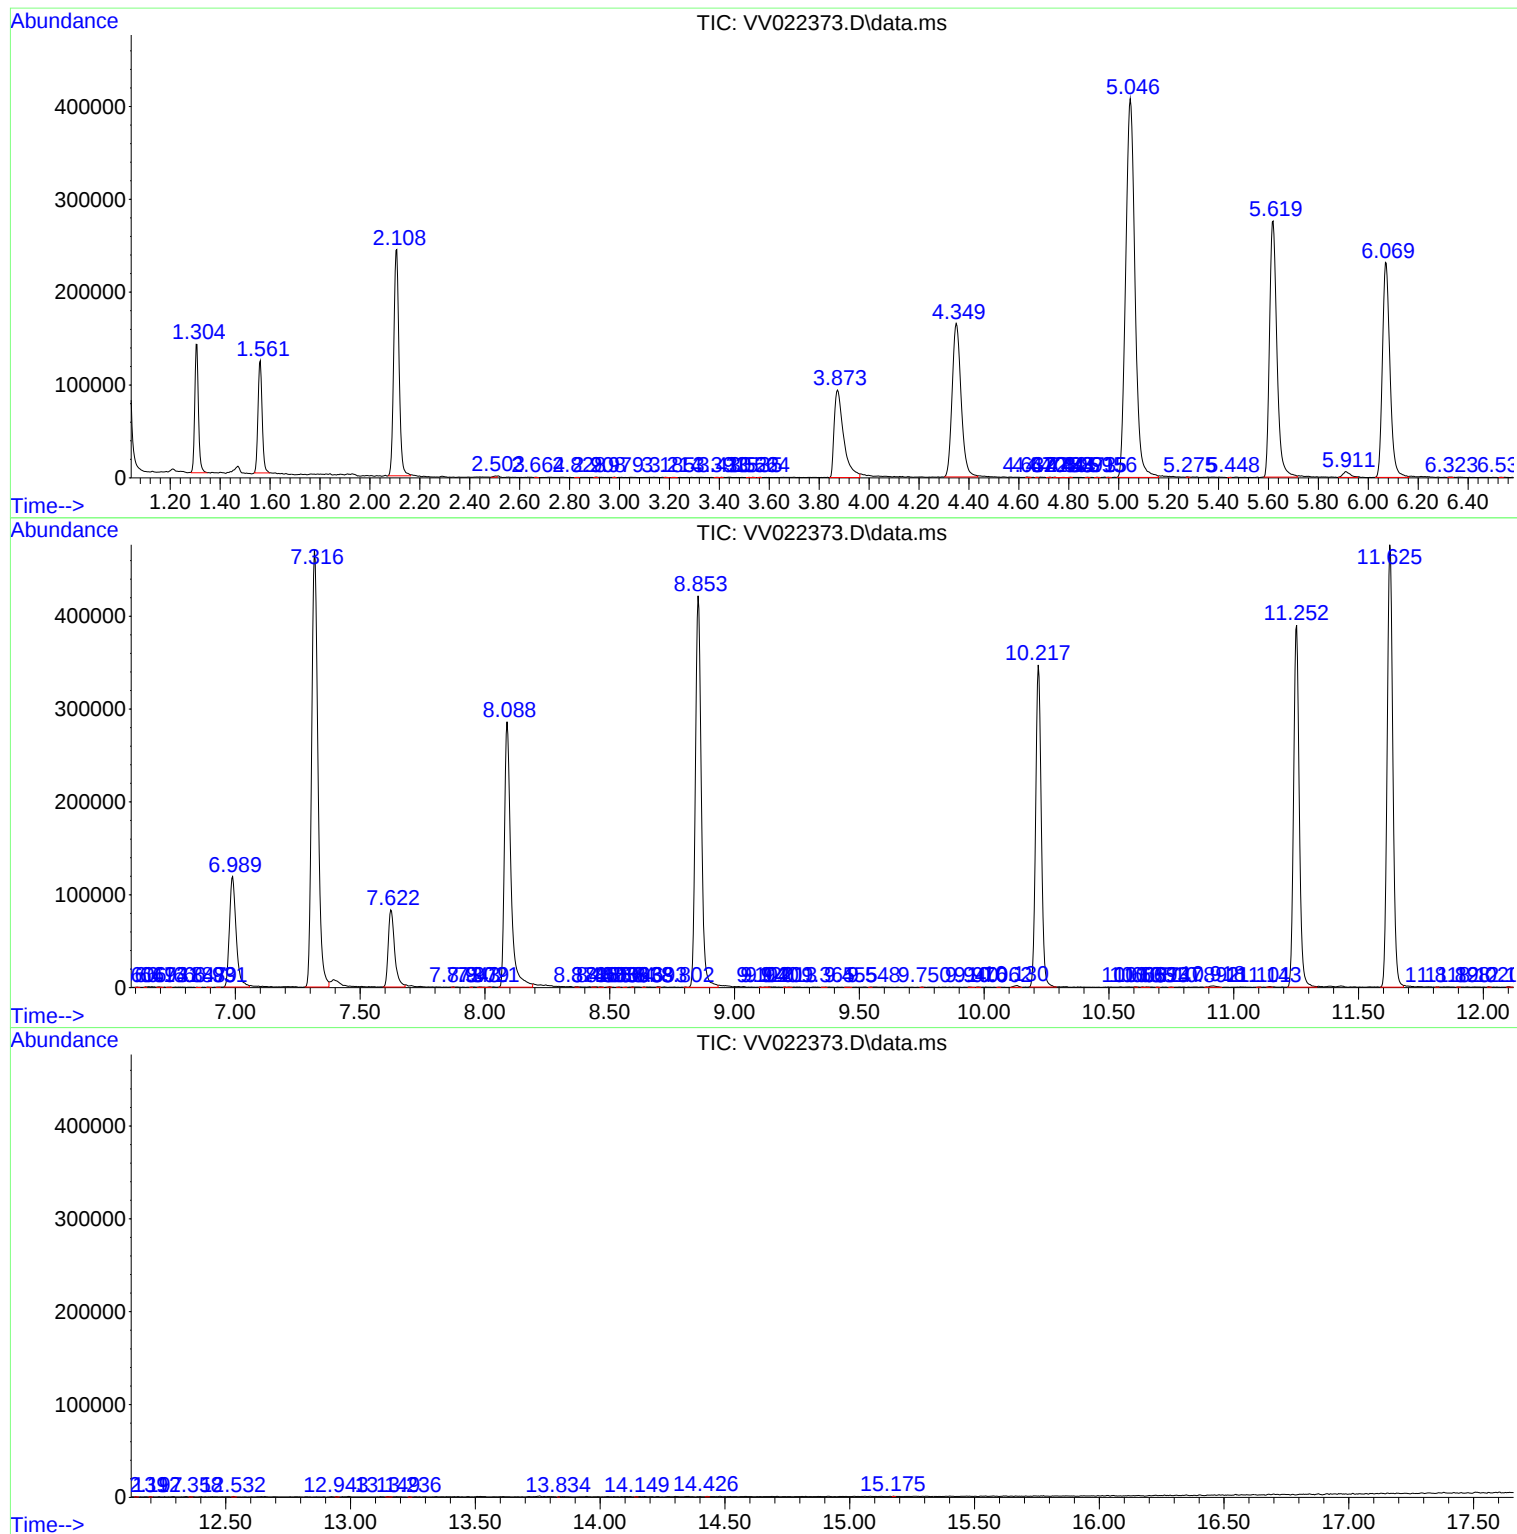

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022373.D
Acq On : 29 Sep 2021 13:20
Operator : SY/MD
Sample : VV0929WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022373.D
Acq On : 29 Sep 2021 13:20
Operator : SY/MD
Sample : VV0929WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
