

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022374.D
 Acq On : 29 Sep 2021 13:44
 Operator : SY/MD
 Sample : M3978-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	144627	141609	13.54%	1.842%
2	1.561	155	162	182	rVB	120776	141895	13.57%	1.846%
3	2.105	321	331	348	rBV	238135	353246	33.77%	4.595%
4	2.500	451	454	455	rBV3	1119	678	0.06%	0.009%
5	2.561	470	473	475	rBV2	332	174	0.02%	0.002%
6	2.577	476	478	480	rBV2	254	117	0.01%	0.002%
7	2.687	509	512	513	rBV	349	202	0.02%	0.003%
8	2.841	559	560	564	rBV2	271	162	0.02%	0.002%
9	2.950	592	594	597	rBV	284	141	0.01%	0.002%
10	3.011	611	613	615	rBV	313	150	0.01%	0.002%
11	3.066	628	630	632	rVB	502	138	0.01%	0.002%
12	3.085	632	636	640	rBV4	403	361	0.03%	0.005%
13	3.108	641	643	646	rVV2	305	151	0.01%	0.002%
14	3.391	726	731	737	rVB	336	319	0.03%	0.004%
15	3.413	737	738	740	rBV	239	104	0.01%	0.001%
16	3.423	740	741	745	rVV2	238	101	0.01%	0.001%
17	3.458	750	752	758	rVB3	307	241	0.02%	0.003%
18	3.484	758	760	762	rBV2	176	117	0.01%	0.002%
19	3.500	762	765	768	rVV2	370	291	0.03%	0.004%
20	3.513	768	769	771	rVB2	401	108	0.01%	0.001%
21	3.593	790	794	795	rBV2	535	256	0.02%	0.003%
22	3.622	800	803	806	rVV2	167	114	0.01%	0.001%
23	3.831	866	868	871	rBV	173	127	0.01%	0.002%
24	3.873	871	881	913	rBV	93362	260726	24.93%	3.392%
25	4.349	1015	1029	1061	rVB	166434	421221	40.27%	5.480%
26	4.558	1091	1094	1095	rBV2	485	244	0.02%	0.003%
27	4.609	1108	1110	1111	rBV2	526	190	0.02%	0.002%
28	4.680	1130	1132	1135	rBV2	387	201	0.02%	0.003%
29	4.709	1139	1141	1144	rBV	318	140	0.01%	0.002%
30	4.728	1145	1147	1150	rBV	316	224	0.02%	0.003%
31	4.863	1186	1189	1192	rBV	311	127	0.01%	0.002%
32	5.047	1230	1246	1273	rBV2	406670	1045955	100.00%	13.607%
33	5.487	1380	1383	1384	rBV2	199	118	0.01%	0.002%
34	5.503	1386	1388	1391	rBV3	313	140	0.01%	0.002%
35	5.519	1391	1393	1395	rBV	235	139	0.01%	0.002%
36	5.619	1411	1424	1456	rBV	280883	577917	55.25%	7.518%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022374.D
 Acq On : 29 Sep 2021 13:44
 Operator : SY/MD
 Sample : M3978-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.069	1551	1564	1595	rBV	231579	480391	45.93%	6.250%
38	6.410	1668	1670	1673	rVB	457	171	0.02%	0.002%
39	6.439	1676	1679	1681	rBV	379	159	0.02%	0.002%
40	6.574	1718	1721	1722	rBV2	312	204	0.02%	0.003%
41	6.645	1739	1743	1745	rBV3	623	420	0.04%	0.005%
42	6.735	1767	1771	1773	rBV2	277	208	0.02%	0.003%
43	6.760	1776	1779	1781	rBV	444	209	0.02%	0.003%
44	6.989	1838	1850	1875	rBV	118534	221257	21.15%	2.878%
45	7.214	1918	1920	1922	rVB	328	99	0.01%	0.001%
46	7.317	1940	1952	1971	rBV	470365	820886	78.48%	10.679%
47	7.622	2037	2047	2064	rBV	84064	145500	13.91%	1.893%
48	7.866	2121	2123	2126	rBV2	309	152	0.01%	0.002%
49	7.927	2139	2142	2143	rBV2	714	356	0.03%	0.005%
50	7.976	2154	2157	2167	rVB4	1488	2028	0.19%	0.026%
51	8.088	2182	2192	2228	rBV	263585	485129	46.38%	6.311%
52	8.471	2309	2311	2314	rVB2	390	184	0.02%	0.002%
53	8.522	2320	2327	2329	rBV2	524	491	0.05%	0.006%
54	8.554	2335	2337	2341	rBV	364	303	0.03%	0.004%
55	8.641	2362	2364	2369	rBV2	396	288	0.03%	0.004%
56	8.763	2399	2402	2405	rBV2	237	209	0.02%	0.003%
57	8.792	2409	2411	2414	rVB3	234	122	0.01%	0.002%
58	8.853	2419	2430	2456	rBV	425638	693011	66.26%	9.016%
59	9.143	2516	2520	2521	rBV	420	304	0.03%	0.004%
60	9.265	2556	2558	2561	rBV2	217	136	0.01%	0.002%
61	9.329	2574	2578	2580	rBV2	227	175	0.02%	0.002%
62	9.358	2586	2587	2591	rBV	238	136	0.01%	0.002%
63	9.410	2601	2603	2605	rBV2	480	188	0.02%	0.002%
64	9.474	2620	2623	2626	rBV2	599	500	0.05%	0.007%
65	9.490	2626	2628	2630	rVB2	311	123	0.01%	0.002%
66	9.763	2711	2713	2715	rBV	465	132	0.01%	0.002%
67	9.844	2736	2738	2739	rBV	288	143	0.01%	0.002%
68	9.866	2742	2745	2747	rVV	410	208	0.02%	0.003%
69	9.966	2773	2776	2780	rBB2	338	195	0.02%	0.003%
70	9.985	2780	2782	2785	rVB2	301	134	0.01%	0.002%
71	9.998	2785	2786	2787	rBV2	269	96	0.01%	0.001%
72	10.027	2792	2795	2800	rVB2	539	354	0.03%	0.005%
73	10.217	2843	2854	2876	rBV	339314	537141	51.35%	6.988%
74	10.381	2902	2905	2909	rVB2	495	354	0.03%	0.005%
75	10.406	2909	2913	2914	rBV2	355	247	0.02%	0.003%
76	10.451	2924	2927	2929	rBV	260	172	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022374.D
 Acq On : 29 Sep 2021 13:44
 Operator : SY/MD
 Sample : M3978-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >




Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.484	2933	2937	2940	rBV2	325	249	0.02%	0.003%
78	10.545	2955	2956	2958	rVB2	309	100	0.01%	0.001%
79	10.599	2972	2973	2976	rBV2	430	260	0.02%	0.003%
80	10.738	3013	3016	3018	rBV	254	141	0.01%	0.002%
81	10.805	3033	3037	3040	rVB2	340	240	0.02%	0.003%
82	10.828	3040	3044	3046	rBV2	350	267	0.03%	0.003%
83	10.879	3057	3060	3062	rBV2	399	230	0.02%	0.003%
84	10.921	3068	3073	3082	rVB7	1202	1640	0.16%	0.021%
85	11.033	3106	3108	3112	rVB3	592	353	0.03%	0.005%
86	11.072	3116	3120	3123	rBV2	322	179	0.02%	0.002%
87	11.117	3131	3134	3137	rBV2	232	222	0.02%	0.003%
88	11.252	3164	3176	3198	rBV	385136	608829	58.21%	7.920%
89	11.532	3259	3263	3266	rBV2	496	382	0.04%	0.005%
90	11.625	3280	3292	3312	rBV	453166	730726	69.86%	9.506%
91	12.091	3436	3437	3440	rBV2	332	222	0.02%	0.003%
92	12.342	3511	3515	3517	rBV2	417	254	0.02%	0.003%
93	12.406	3532	3535	3539	rBV2	225	198	0.02%	0.003%
94	13.114	3751	3755	3759	rBV2	395	405	0.04%	0.005%
95	13.249	3795	3797	3800	rVB	356	115	0.01%	0.001%
96	13.651	3920	3922	3926	rBV2	271	200	0.02%	0.003%
97	13.876	3990	3992	3994	rVB	434	139	0.01%	0.002%
98	14.268	4111	4114	4119	rBV2	499	436	0.04%	0.006%
99	14.294	4120	4122	4126	rBV3	338	200	0.02%	0.003%
100	14.352	4138	4140	4142	rBV3	345	138	0.01%	0.002%

Sum of corrected areas: 7686784

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

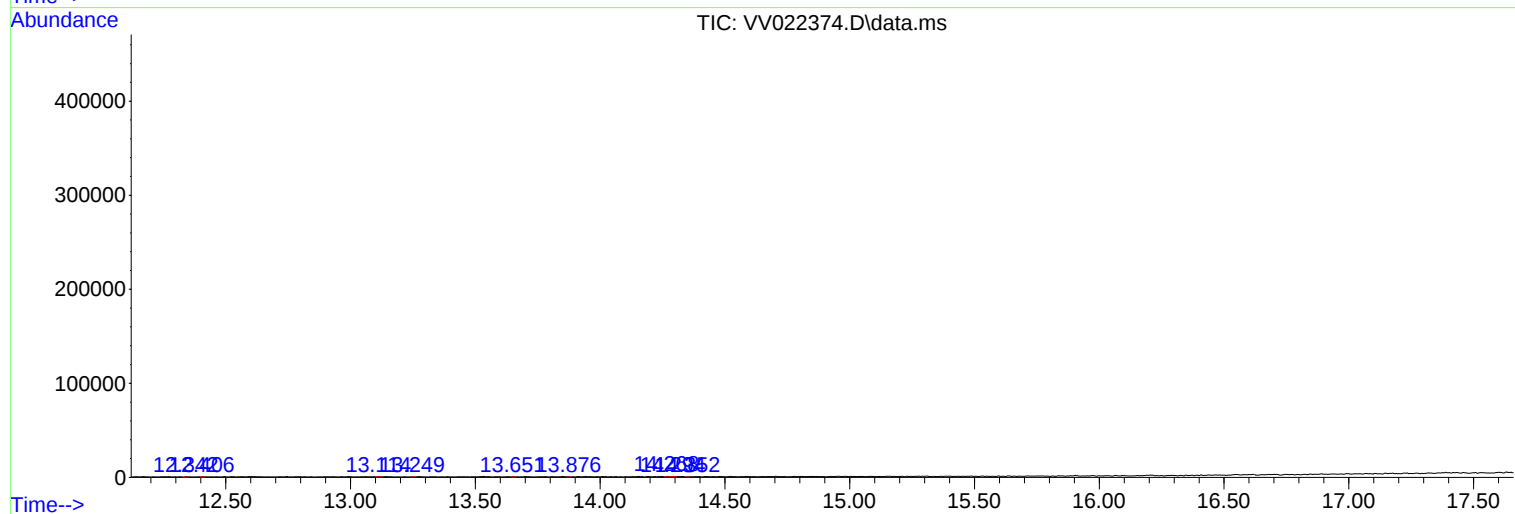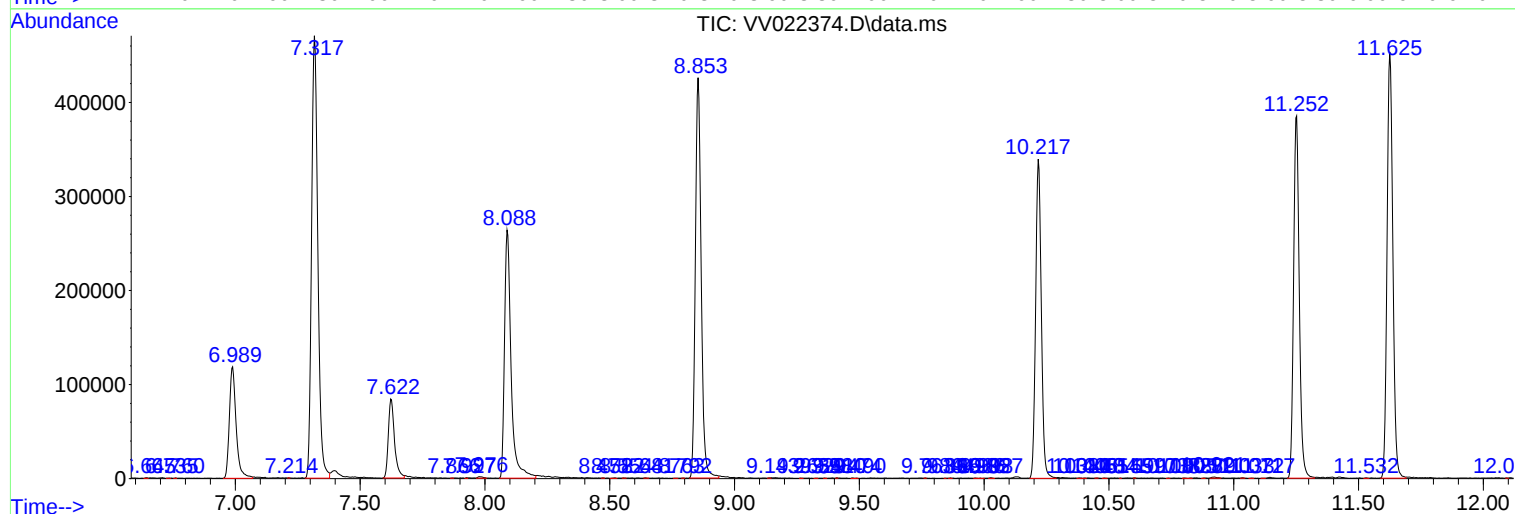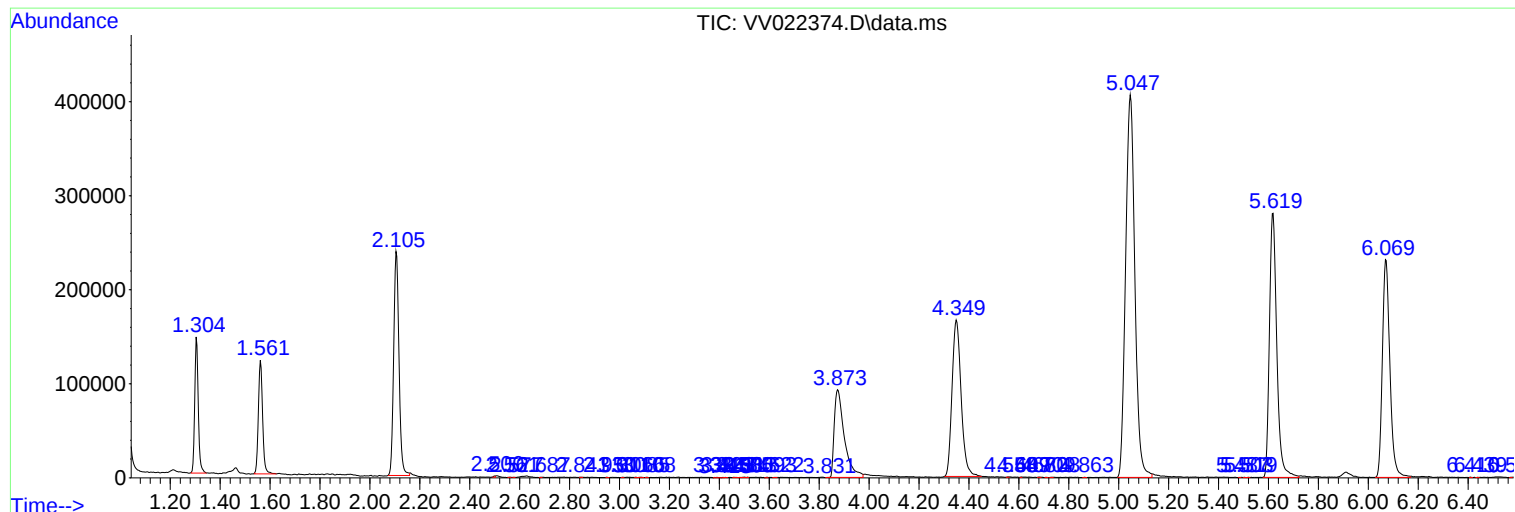

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022374.D
Acq On : 29 Sep 2021 13:44
Operator : SY/MD
Sample : M3978-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022374.D
Acq On : 29 Sep 2021 13:44
Operator : SY/MD
Sample : M3978-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
