

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022376.D
 Acq On : 29 Sep 2021 14:32
 Operator : SY/MD
 Sample : M3877-09ME
 Misc : 6.13g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2M5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	102	rVB	90435	139355	12.97%	1.758%
2	1.532	148	153	159	rBV	35883	38413	3.57%	0.485%
3	2.076	311	322	334	rBV	231253	336981	31.36%	4.251%
4	2.243	367	374	376	rBV4	894	771	0.07%	0.010%
5	2.346	403	406	410	rVB5	483	362	0.03%	0.005%
6	2.494	444	452	460	rBV5	2838	4713	0.44%	0.059%
7	2.626	491	493	496	rBV2	509	357	0.03%	0.005%
8	2.661	501	504	506	rBV2	452	276	0.03%	0.003%
9	2.690	511	513	516	rVB2	488	305	0.03%	0.004%
10	2.712	516	520	521	rBV	644	454	0.04%	0.006%
11	2.722	521	523	525	rVV	653	361	0.03%	0.005%
12	2.796	540	546	552	rVB4	573	565	0.05%	0.007%
13	2.825	552	555	558	rBV2	363	286	0.03%	0.004%
14	2.921	581	585	587	rBV2	436	293	0.03%	0.004%
15	2.941	587	591	595	rVB3	539	477	0.04%	0.006%
16	3.008	605	612	613	rBV2	359	294	0.03%	0.004%
17	3.021	613	616	620	rVB2	572	353	0.03%	0.004%
18	3.060	623	628	631	rVB3	383	347	0.03%	0.004%
19	3.092	636	638	641	rVB	582	338	0.03%	0.004%
20	3.124	645	648	654	rBV3	538	510	0.05%	0.006%
21	3.191	668	669	675	rVB2	376	284	0.03%	0.004%
22	3.227	675	680	683	rBV3	501	391	0.04%	0.005%
23	3.391	728	731	734	rBV2	425	274	0.03%	0.003%
24	3.436	741	745	748	rBV2	617	391	0.04%	0.005%
25	3.593	790	794	796	rBV2	559	459	0.04%	0.006%
26	3.670	814	818	822	rVB2	438	343	0.03%	0.004%
27	3.854	872	875	876	rBV	473	265	0.02%	0.003%
28	3.889	876	886	918	rBV2	60097	217560	20.25%	2.745%
29	4.243	993	996	999	rBV4	519	411	0.04%	0.005%
30	4.346	1010	1028	1062	rBV	158019	423053	39.37%	5.337%
31	4.899	1197	1200	1203	rVB	503	277	0.03%	0.003%
32	4.934	1207	1211	1213	rVB	364	268	0.02%	0.003%
33	4.963	1215	1220	1223	rBV3	318	321	0.03%	0.004%
34	5.037	1227	1243	1276	rBV2	432072	1074511	100.00%	13.556%
35	5.339	1326	1337	1349	rBV10	3749	10298	0.96%	0.130%
36	5.613	1410	1422	1451	rBV	285135	604991	56.30%	7.632%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022376.D
 Acq On : 29 Sep 2021 14:32
 Operator : SY/MD
 Sample : M3877-09ME
 Misc : 6.13g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2M5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	5.831	1487	1490	1495	rVB3	747	553	0.05%	0.007%
38	5.905	1504	1513	1529	rBV9	4626	10999	1.02%	0.139%
39	5.989	1532	1539	1547	rBV7	2292	3806	0.35%	0.048%
40	6.069	1551	1564	1586	rBV	223797	479388	44.61%	6.048%
41	6.307	1637	1638	1642	rBV	394	276	0.03%	0.003%
42	6.468	1686	1688	1692	rBV3	481	332	0.03%	0.004%
43	6.506	1697	1700	1701	rBV2	730	321	0.03%	0.004%
44	6.645	1737	1743	1744	rBV2	939	659	0.06%	0.008%
45	6.825	1797	1799	1803	rVB	626	343	0.03%	0.004%
46	6.912	1822	1826	1828	rVB	426	283	0.03%	0.004%
47	6.985	1836	1849	1871	rBV	109940	223020	20.76%	2.814%
48	7.137	1893	1896	1901	rVB3	457	297	0.03%	0.004%
49	7.217	1917	1921	1923	rBV4	687	542	0.05%	0.007%
50	7.313	1939	1951	1971	rBV	469232	847566	78.88%	10.693%
51	7.625	2037	2048	2071	rBV2	74556	150047	13.96%	1.893%
52	7.863	2119	2122	2126	rBV3	350	275	0.03%	0.003%
53	7.944	2142	2147	2152	rVB3	650	747	0.07%	0.009%
54	7.979	2155	2158	2162	rBV	430	312	0.03%	0.004%
55	8.104	2184	2197	2231	rVV2	197715	519039	48.30%	6.548%
56	8.503	2318	2321	2323	rBV2	697	398	0.04%	0.005%
57	8.657	2364	2369	2372	rBV4	511	463	0.04%	0.006%
58	8.854	2418	2430	2451	rBV	419812	731440	68.07%	9.228%
59	9.143	2517	2520	2521	rBV	876	400	0.04%	0.005%
60	9.381	2592	2594	2602	rVB3	504	513	0.05%	0.006%
61	9.432	2607	2610	2614	rBV2	556	348	0.03%	0.004%
62	9.481	2623	2625	2630	rVB3	436	278	0.03%	0.004%
63	9.966	2773	2776	2781	rBV2	391	286	0.03%	0.004%
64	10.127	2820	2826	2837	rVB4	3078	4971	0.46%	0.063%
65	10.223	2843	2856	2876	rBV	340001	571951	53.23%	7.216%
66	10.484	2934	2937	2940	rBV3	440	371	0.03%	0.005%
67	10.667	2989	2994	2997	rBV4	586	604	0.06%	0.008%
68	10.767	3022	3025	3026	rBV	447	298	0.03%	0.004%
69	10.828	3042	3044	3048	rBV4	556	412	0.04%	0.005%
70	10.918	3065	3072	3080	rVB5	2507	3787	0.35%	0.048%
71	11.037	3106	3109	3116	rVB2	1203	1075	0.10%	0.014%
72	11.069	3116	3119	3122	rBV2	684	513	0.05%	0.006%
73	11.143	3139	3142	3151	rVB6	1573	1985	0.18%	0.025%
74	11.252	3165	3176	3193	rVV	441594	696282	64.80%	8.784%
75	11.471	3242	3244	3247	rBV2	511	349	0.03%	0.004%
76	11.487	3247	3249	3256	rVB2	482	425	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022376.D
 Acq On : 29 Sep 2021 14:32
 Operator : SY/MD
 Sample : M3877-09ME
 Misc : 6.13g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2M5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.551	3264	3269	3272	rBV3	657	572	0.05%	0.007%
78	11.628	3280	3293	3316	rBV	503621	800809	74.53%	10.103%
79	11.722	3319	3322	3324	rBV4	658	330	0.03%	0.004%
80	11.779	3338	3340	3351	rVB5	1215	1780	0.17%	0.022%
81	11.866	3365	3367	3371	rVB	500	270	0.03%	0.003%
82	11.943	3387	3391	3395	rBV2	445	391	0.04%	0.005%
83	12.014	3410	3413	3416	rVB2	510	339	0.03%	0.004%
84	12.085	3433	3435	3438	rBV2	357	262	0.02%	0.003%
85	12.358	3517	3520	3522	rBV	521	270	0.03%	0.003%
86	12.384	3526	3528	3531	rVV2	427	284	0.03%	0.004%
87	12.561	3581	3583	3587	rVB2	599	319	0.03%	0.004%
88	12.635	3603	3606	3612	rBV3	421	510	0.05%	0.006%
89	12.799	3652	3657	3658	rBV	442	369	0.03%	0.005%
90	13.680	3928	3931	3936	rVV3	367	359	0.03%	0.005%
91	13.754	3952	3954	3958	rVB	724	363	0.03%	0.005%
92	13.818	3970	3974	3978	rBV3	403	420	0.04%	0.005%
93	13.841	3978	3981	3983	rBV	465	263	0.02%	0.003%
94	14.104	4061	4063	4068	rBV3	324	316	0.03%	0.004%
95	14.265	4110	4113	4116	rVB2	605	342	0.03%	0.004%
96	14.670	4235	4239	4245	rBV3	709	818	0.08%	0.010%
97	14.699	4245	4248	4251	rVV2	523	299	0.03%	0.004%
98	15.172	4391	4395	4399	rBV4	477	422	0.04%	0.005%
99	15.699	4557	4559	4561	rBV2	682	362	0.03%	0.005%
100	16.033	4661	4663	4665	rBV3	551	302	0.03%	0.004%




Sum of corrected areas: 7926633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022376.D
Acq On : 29 Sep 2021 14:32
Operator : SY/MD
Sample : M3877-09ME
Misc : 6.13g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2M5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

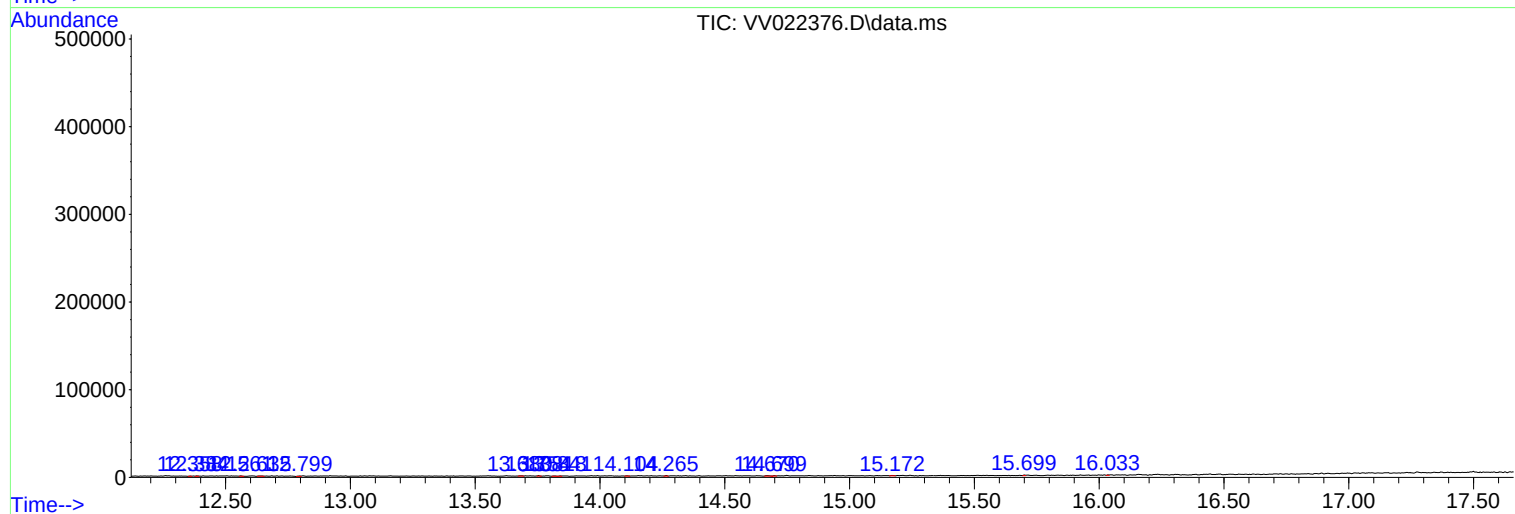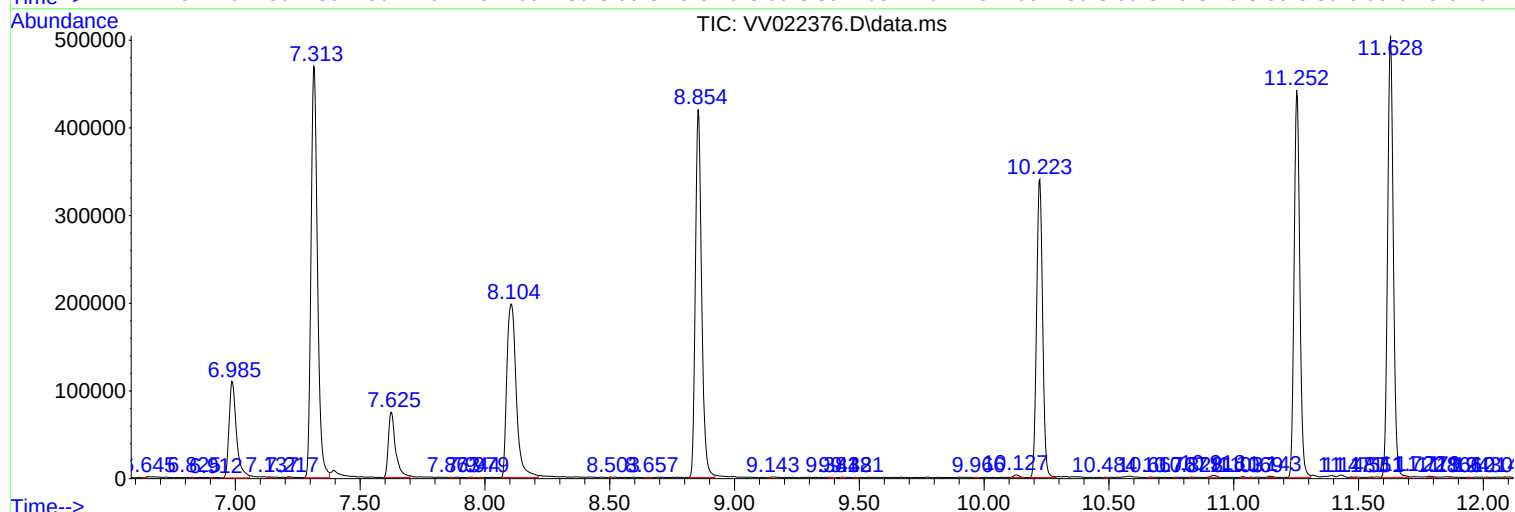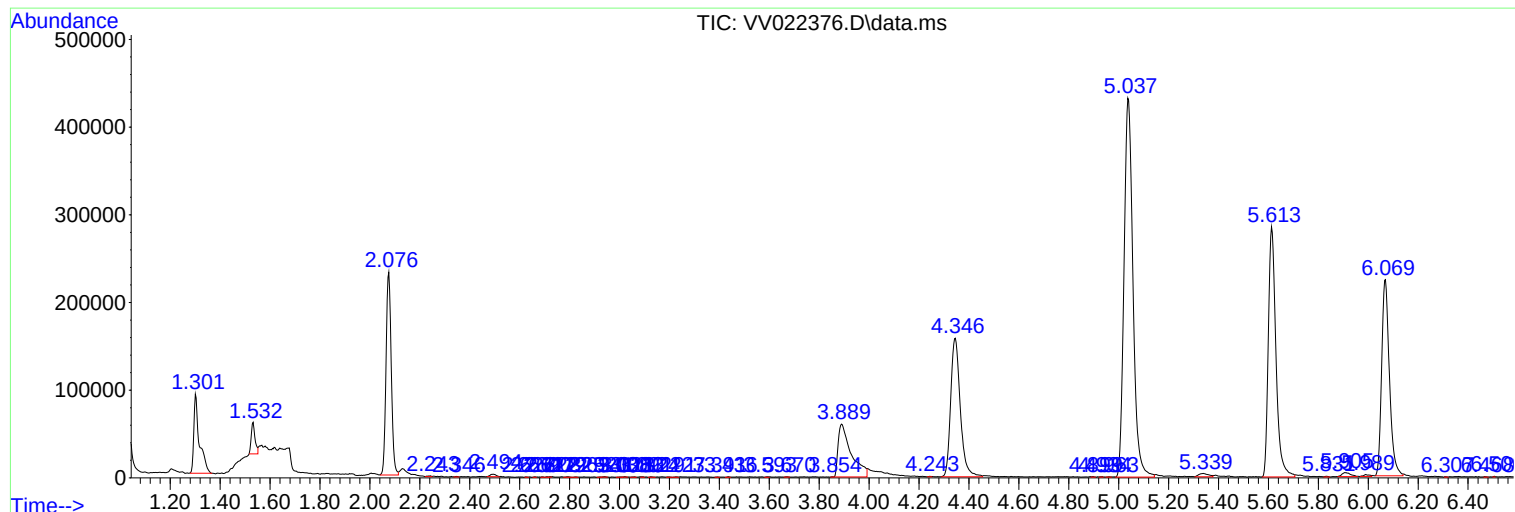

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022376.D
Acq On : 29 Sep 2021 14:32
Operator : SY/MD
Sample : M3877-09ME
Misc : 6.13g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2M5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022376.D
Acq On : 29 Sep 2021 14:32
Operator : SY/MD
Sample : M3877-09ME
Misc : 6.13g/5.0ml/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2M5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
