

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022377.D
 Acq On : 29 Sep 2021 14:56
 Operator : SY/MD
 Sample : M3979-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	142879	144557	13.61%	1.862%
2	1.561	155	162	175	rVB	123584	142014	13.37%	1.829%
3	2.105	322	331	344	rBV	240057	347094	32.69%	4.470%
4	2.953	593	595	597	rVB3	558	224	0.02%	0.003%
5	3.034	614	620	623	rVB2	415	357	0.03%	0.005%
6	3.233	678	682	684	rBV2	336	264	0.02%	0.003%
7	3.288	695	699	706	rBV2	322	265	0.02%	0.003%
8	3.622	799	803	804	rBV2	368	255	0.02%	0.003%
9	3.645	807	810	813	rBV2	520	256	0.02%	0.003%
10	3.748	838	842	843	rBV2	368	257	0.02%	0.003%
11	3.821	862	865	870	rBV2	601	552	0.05%	0.007%
12	3.876	872	882	915	rBV	88686	257826	24.28%	3.321%
13	4.349	1015	1029	1055	rBV	162975	415223	39.10%	5.348%
14	4.558	1091	1094	1096	rVB2	627	292	0.03%	0.004%
15	4.571	1096	1098	1101	rBV	443	248	0.02%	0.003%
16	4.622	1110	1114	1121	rBV5	450	562	0.05%	0.007%
17	4.915	1202	1205	1211	rVB2	286	290	0.03%	0.004%
18	5.047	1228	1246	1277	rBV2	409305	1061921	100.00%	13.677%
19	5.471	1375	1378	1379	rBV2	407	207	0.02%	0.003%
20	5.538	1397	1399	1402	rVB3	452	207	0.02%	0.003%
21	5.619	1411	1424	1450	rBV	285125	585370	55.12%	7.539%
22	5.908	1505	1514	1530	rVB5	7705	16462	1.55%	0.212%
23	6.011	1544	1546	1549	rBV3	495	343	0.03%	0.004%
24	6.069	1551	1564	1589	rBV	230225	483720	45.55%	6.230%
25	6.304	1633	1637	1639	rBV2	395	276	0.03%	0.004%
26	6.342	1645	1649	1652	rVB2	465	371	0.03%	0.005%
27	6.362	1652	1655	1659	rBV2	395	336	0.03%	0.004%
28	6.442	1675	1680	1684	rVB2	274	259	0.02%	0.003%
29	6.493	1692	1696	1698	rBV2	481	289	0.03%	0.004%
30	6.513	1698	1702	1706	rBV2	967	902	0.08%	0.012%
31	6.580	1720	1723	1724	rBV	521	294	0.03%	0.004%
32	6.616	1732	1734	1737	rBV3	330	230	0.02%	0.003%
33	6.815	1793	1796	1800	rBV3	384	327	0.03%	0.004%
34	6.989	1839	1850	1870	rBV	116318	218325	20.56%	2.812%
35	7.175	1905	1908	1909	rBV2	683	399	0.04%	0.005%
36	7.317	1939	1952	1971	rBV	480862	830782	78.23%	10.700%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022377.D
 Acq On : 29 Sep 2021 14:56
 Operator : SY/MD
 Sample : M3979-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 F4A58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	7.503	2008	2010	2011	rBV	956	389	0.04%	0.005%
38	7.622	2038	2047	2075	rBV	80694	145868	13.74%	1.879%
39	7.812	2102	2106	2109	rBV4	433	284	0.03%	0.004%
40	7.931	2138	2143	2145	rBV4	598	550	0.05%	0.007%
41	7.979	2150	2158	2170	rBV3	9538	16605	1.56%	0.214%
42	8.024	2170	2172	2175	rVB	400	209	0.02%	0.003%
43	8.091	2182	2193	2223	rBV2	251181	483363	45.52%	6.226%
44	8.442	2299	2302	2305	rBV2	277	245	0.02%	0.003%
45	8.503	2317	2321	2324	rVB4	750	494	0.05%	0.006%
46	8.567	2338	2341	2342	rBV	532	321	0.03%	0.004%
47	8.696	2378	2381	2385	rVB3	399	269	0.03%	0.003%
48	8.722	2385	2389	2391	rBV5	456	329	0.03%	0.004%
49	8.786	2406	2409	2413	rBV2	286	242	0.02%	0.003%
50	8.853	2418	2430	2457	rBV	424772	708140	66.68%	9.121%
51	9.114	2504	2511	2513	rBV2	451	465	0.04%	0.006%
52	9.152	2518	2523	2532	rVB4	1157	1354	0.13%	0.017%
53	9.435	2608	2611	2615	rVB2	554	350	0.03%	0.005%
54	9.474	2620	2623	2625	rBV2	321	221	0.02%	0.003%
55	9.493	2625	2629	2634	rVB	358	272	0.03%	0.004%
56	9.532	2637	2641	2644	rBV	229	198	0.02%	0.003%
57	9.599	2659	2662	2666	rVB2	387	211	0.02%	0.003%
58	9.638	2672	2674	2681	rVB2	389	248	0.02%	0.003%
59	9.689	2686	2690	2691	rBV2	320	233	0.02%	0.003%
60	9.783	2714	2719	2723	rVV2	297	292	0.03%	0.004%
61	9.824	2727	2732	2736	rBV3	425	489	0.05%	0.006%
62	9.850	2736	2740	2742	rBV2	271	205	0.02%	0.003%
63	9.902	2752	2756	2758	rBV2	444	292	0.03%	0.004%
64	10.021	2789	2793	2796	rBV3	366	288	0.03%	0.004%
65	10.133	2819	2828	2833	rVB6	1808	2608	0.25%	0.034%
66	10.217	2841	2854	2879	rBV	332109	527801	49.70%	6.798%
67	10.390	2903	2908	2910	rBV4	545	476	0.04%	0.006%
68	10.435	2920	2922	2928	rBV3	379	334	0.03%	0.004%
69	10.487	2936	2938	2943	rVB3	456	305	0.03%	0.004%
70	10.554	2952	2959	2964	rBV4	655	847	0.08%	0.011%
71	10.622	2978	2980	2986	rBV2	362	335	0.03%	0.004%
72	10.779	3026	3029	3031	rBV	488	253	0.02%	0.003%
73	10.972	3085	3089	3094	rBV3	322	386	0.04%	0.005%
74	11.149	3139	3144	3151	rVB5	954	1084	0.10%	0.014%
75	11.249	3163	3175	3195	rBV	392043	614306	57.85%	7.912%
76	11.577	3274	3277	3279	rBV	378	229	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022377.D
 Acq On : 29 Sep 2021 14:56
 Operator : SY/MD
 Sample : M3979-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.625	3280	3292	3316	rVV	464938	734261	69.14%	9.457%
78	11.738	3325	3327	3331	rBV3	612	391	0.04%	0.005%
79	11.850	3360	3362	3367	rVB4	428	230	0.02%	0.003%
80	12.143	3451	3453	3459	rVB	534	332	0.03%	0.004%
81	12.172	3459	3462	3465	rVB2	598	276	0.03%	0.004%
82	12.287	3494	3498	3500	rBV2	383	264	0.02%	0.003%
83	12.474	3554	3556	3559	rBV	307	217	0.02%	0.003%
84	12.609	3596	3598	3605	rVV3	398	376	0.04%	0.005%
85	12.789	3649	3654	3655	rBV	264	224	0.02%	0.003%
86	12.947	3700	3703	3706	rBV2	489	361	0.03%	0.005%
87	13.040	3729	3732	3735	rBV2	441	261	0.02%	0.003%
88	13.159	3767	3769	3775	rBV2	354	301	0.03%	0.004%
89	13.184	3775	3777	3779	rBV	424	198	0.02%	0.003%
90	13.246	3794	3796	3800	rVV2	347	237	0.02%	0.003%
91	13.374	3828	3836	3838	rBV4	449	509	0.05%	0.007%
92	13.422	3848	3851	3854	rBV2	471	317	0.03%	0.004%
93	13.635	3914	3917	3920	rBV2	252	196	0.02%	0.003%
94	13.766	3955	3958	3965	rVB2	419	389	0.04%	0.005%
95	13.969	4012	4021	4022	rBV3	471	575	0.05%	0.007%
96	13.995	4026	4029	4033	rVB2	470	367	0.03%	0.005%
97	14.114	4064	4066	4069	rVB2	406	195	0.02%	0.003%
98	14.278	4113	4117	4119	rBV3	246	239	0.02%	0.003%
99	14.503	4185	4187	4192	rVB3	338	266	0.03%	0.003%
100	14.721	4251	4255	4257	rBV2	338	304	0.03%	0.004%


Sum of corrected areas: 7764232

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022377.D
Acq On : 29 Sep 2021 14:56
Operator : SY/MD
Sample : M3979-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

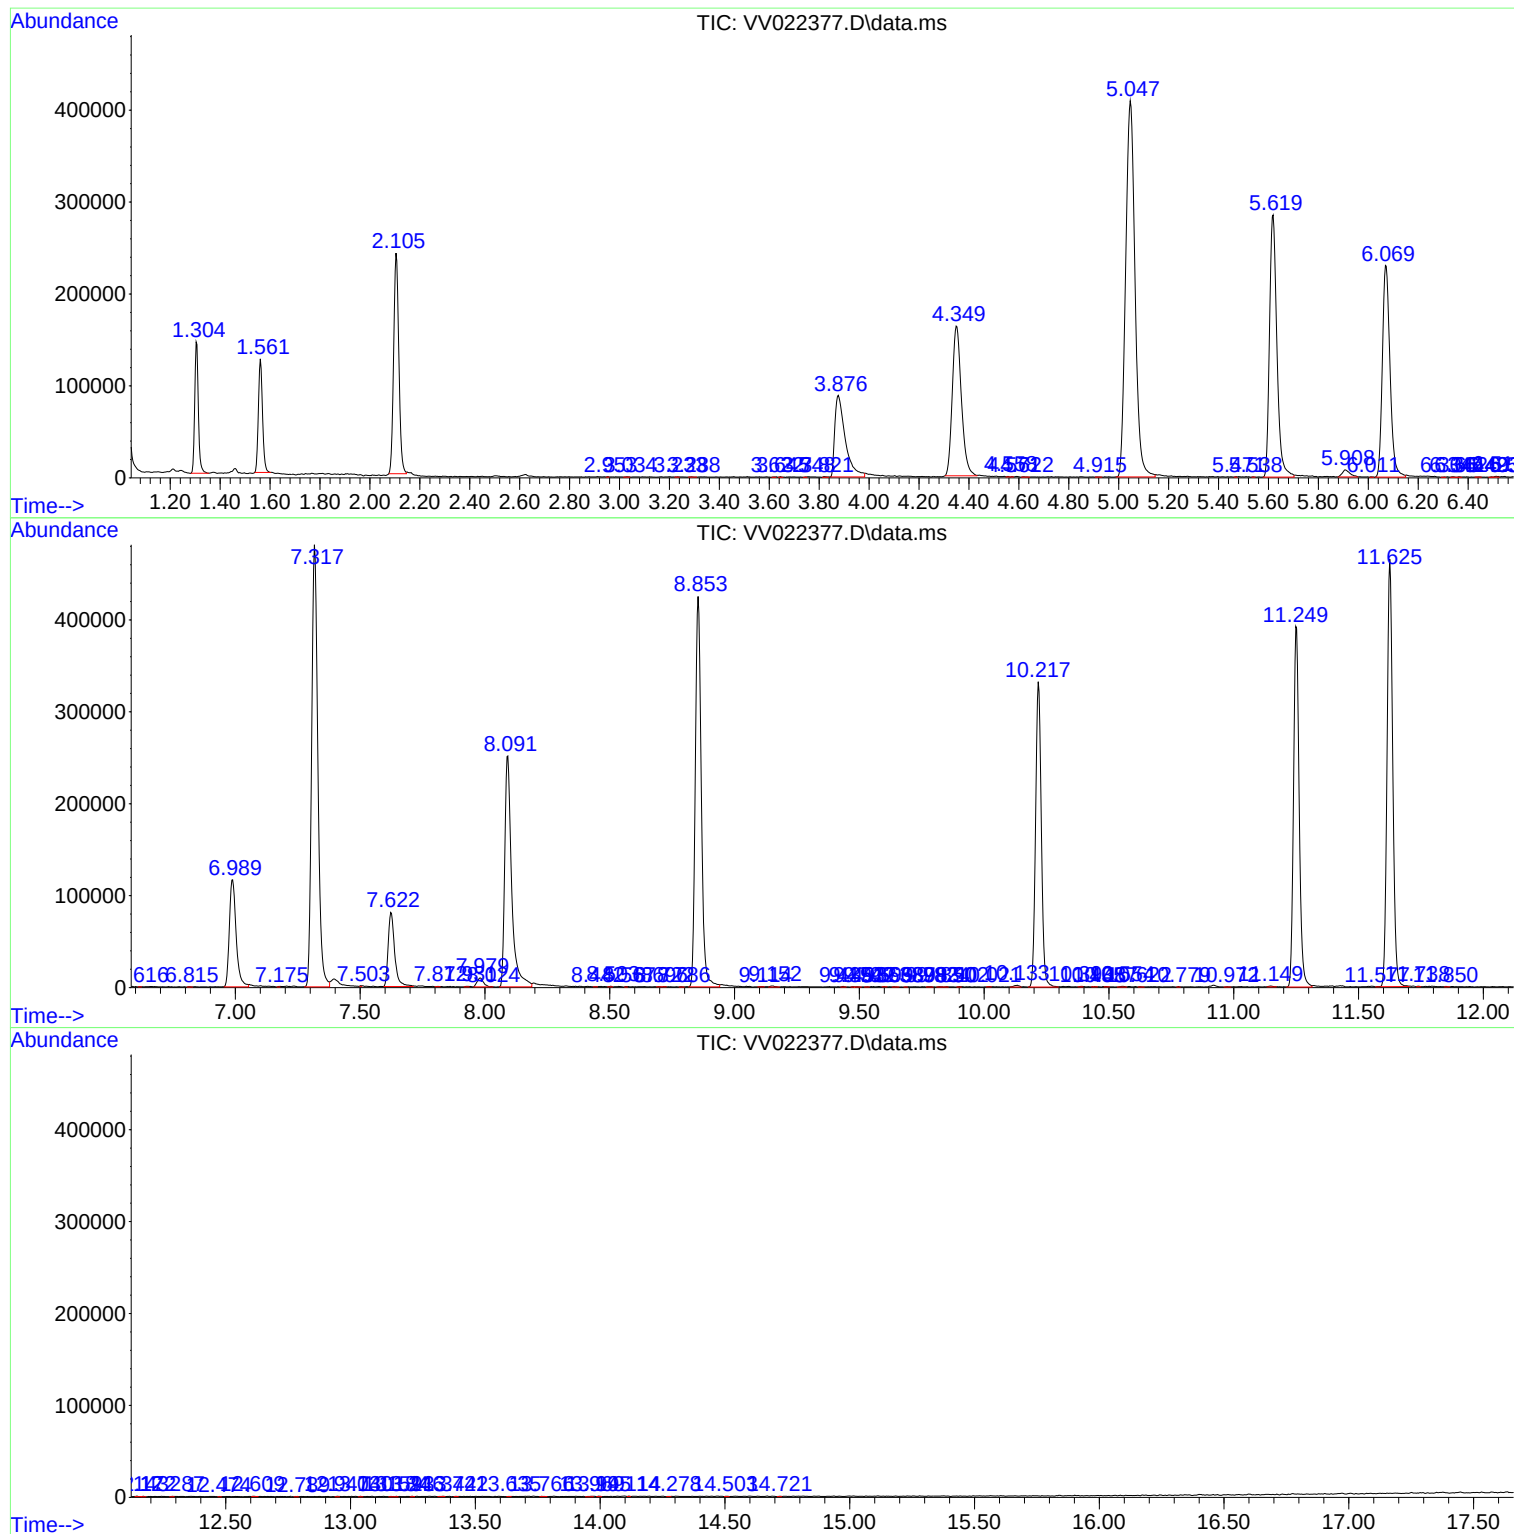

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022377.D
Acq On : 29 Sep 2021 14:56
Operator : SY/MD
Sample : M3979-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022377.D
Acq On : 29 Sep 2021 14:56
Operator : SY/MD
Sample : M3979-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------