

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022378.D
 Acq On : 29 Sep 2021 15:20
 Operator : SY/MD
 Sample : M3979-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	141613	142395	13.46%	1.825%
2	1.561	155	162	179	rVB	121101	142411	13.46%	1.825%
3	2.105	322	331	341	rBV	240774	347744	32.86%	4.457%
4	2.433	428	433	449	rVB3	6608	11724	1.11%	0.150%
5	2.603	484	486	487	rBV3	553	302	0.03%	0.004%
6	2.610	487	488	490	rVV2	595	284	0.03%	0.004%
7	2.838	557	559	562	rBV	211	129	0.01%	0.002%
8	2.938	588	590	595	rVB	342	253	0.02%	0.003%
9	3.124	646	648	650	rBV2	180	126	0.01%	0.002%
10	3.143	652	654	659	rVB2	267	123	0.01%	0.002%
11	3.179	662	665	668	rBV3	211	156	0.01%	0.002%
12	3.198	668	671	673	rVV2	375	198	0.02%	0.003%
13	3.253	685	688	690	rBV3	254	186	0.02%	0.002%
14	3.294	699	701	705	rVB2	504	324	0.03%	0.004%
15	3.317	705	708	709	rBV	270	109	0.01%	0.001%
16	3.394	724	732	733	rBV2	357	273	0.03%	0.003%
17	3.442	744	747	750	rBV2	350	286	0.03%	0.004%
18	3.523	770	772	775	rBV	308	191	0.02%	0.002%
19	3.606	795	798	803	rVB2	396	355	0.03%	0.005%
20	3.683	818	822	823	rBV2	459	262	0.02%	0.003%
21	3.799	854	858	860	rBV	246	150	0.01%	0.002%
22	3.818	863	864	868	rVB	379	140	0.01%	0.002%
23	3.873	871	881	907	rBV	90782	249647	23.59%	3.199%
24	4.349	1014	1029	1053	rBV2	167663	423172	39.99%	5.423%
25	4.552	1089	1092	1094	rBV2	673	429	0.04%	0.005%
26	4.571	1094	1098	1101	rVB5	407	331	0.03%	0.004%
27	4.671	1127	1129	1131	rBV	436	153	0.01%	0.002%
28	4.748	1149	1153	1154	rBV2	263	152	0.01%	0.002%
29	4.870	1187	1191	1193	rBV3	381	297	0.03%	0.004%
30	4.934	1209	1211	1213	rBV	309	148	0.01%	0.002%
31	4.966	1218	1221	1223	rBV	234	107	0.01%	0.001%
32	4.982	1225	1226	1229	rVB	424	150	0.01%	0.002%
33	5.047	1229	1246	1283	rBV2	409784	1058128	100.00%	13.560%
34	5.413	1357	1360	1366	rVB7	394	382	0.04%	0.005%
35	5.507	1387	1389	1390	rBV7	363	167	0.02%	0.002%
36	5.561	1402	1406	1407	rBV	243	194	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022378.D
 Acq On : 29 Sep 2021 15:20
 Operator : SY/MD
 Sample : M3979-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	5.619	1411	1424	1454	rBV	284118	587120	55.49%	7.524%
38	5.863	1497	1500	1502	rBV2	406	303	0.03%	0.004%
39	5.912	1504	1515	1529	rVV6	8104	17585	1.66%	0.225%
40	5.995	1540	1541	1544	rBV3	276	142	0.01%	0.002%
41	6.072	1548	1565	1588	rBV	232313	481567	45.51%	6.172%
42	6.243	1616	1618	1622	rVB4	761	355	0.03%	0.005%
43	6.304	1632	1637	1638	rBV3	607	438	0.04%	0.006%
44	6.458	1682	1685	1687	rVV2	467	266	0.03%	0.003%
45	6.519	1702	1704	1707	rVB2	606	283	0.03%	0.004%
46	6.625	1733	1737	1739	rBV2	419	257	0.02%	0.003%
47	6.645	1739	1743	1744	rBV2	465	304	0.03%	0.004%
48	6.757	1777	1778	1781	rVV	396	190	0.02%	0.002%
49	6.773	1781	1783	1785	rVV2	440	220	0.02%	0.003%
50	6.806	1789	1793	1795	rBV	311	234	0.02%	0.003%
51	6.908	1821	1825	1828	rBV2	157	134	0.01%	0.002%
52	6.944	1834	1836	1839	rBV3	205	116	0.01%	0.001%
53	6.989	1839	1850	1875	rBV	121884	222649	21.04%	2.853%
54	7.317	1940	1952	1971	rBV	471608	825377	78.00%	10.578%
55	7.622	2037	2047	2068	rBV	83154	147486	13.94%	1.890%
56	7.860	2118	2121	2123	rBV	425	269	0.03%	0.003%
57	7.973	2152	2156	2157	rBV	266	174	0.02%	0.002%
58	7.998	2162	2164	2166	rBV	273	125	0.01%	0.002%
59	8.088	2183	2192	2230	rBV2	261435	502693	47.51%	6.442%
60	8.342	2269	2271	2278	rVB5	690	565	0.05%	0.007%
61	8.432	2297	2299	2305	rVB3	469	236	0.02%	0.003%
62	8.548	2333	2335	2338	rBV	319	222	0.02%	0.003%
63	8.725	2388	2390	2393	rBV2	369	229	0.02%	0.003%
64	8.805	2412	2415	2419	rBV3	447	329	0.03%	0.004%
65	8.854	2419	2430	2455	rBV	431642	709812	67.08%	9.097%
66	9.214	2539	2542	2543	rBV	352	165	0.02%	0.002%
67	9.317	2572	2574	2577	rBV2	267	138	0.01%	0.002%
68	9.410	2598	2603	2606	rBV3	483	441	0.04%	0.006%
69	9.448	2612	2615	2617	rVB2	270	151	0.01%	0.002%
70	9.522	2636	2638	2642	rBV	357	165	0.02%	0.002%
71	9.725	2698	2701	2702	rBV2	612	271	0.03%	0.003%
72	9.751	2706	2709	2711	rVV3	487	195	0.02%	0.002%
73	9.793	2720	2722	2727	rBV	240	169	0.02%	0.002%
74	10.005	2785	2788	2790	rBV	204	132	0.01%	0.002%
75	10.040	2796	2799	2805	rBV3	446	408	0.04%	0.005%
76	10.088	2812	2814	2816	rBV2	384	172	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022378.D
 Acq On : 29 Sep 2021 15:20
 Operator : SY/MD
 Sample : M3979-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.172	2838	2840	2842	rBV	273	135	0.01%	0.002%
78	10.217	2842	2854	2877	rVV	333367	535312	50.59%	6.860%
79	10.365	2899	2900	2902	rBV	347	147	0.01%	0.002%
80	10.465	2926	2931	2938	rBV3	383	430	0.04%	0.006%
81	10.529	2949	2951	2952	rBV3	360	130	0.01%	0.002%
82	10.538	2952	2954	2957	rBV3	269	191	0.02%	0.002%
83	10.609	2974	2976	2979	rVB3	752	248	0.02%	0.003%
84	10.661	2990	2992	2994	rBV	375	187	0.02%	0.002%
85	10.802	3033	3036	3042	rBV2	352	381	0.04%	0.005%
86	10.918	3066	3072	3082	rVB3	2270	2760	0.26%	0.035%
87	11.252	3162	3176	3201	rBV	394326	624784	59.05%	8.007%
88	11.477	3244	3246	3248	rBV	336	155	0.01%	0.002%
89	11.538	3257	3265	3274	rBV4	5744	10619	1.00%	0.136%
90	11.625	3281	3292	3315	rVB	464704	741611	70.09%	9.504%
91	12.246	3483	3485	3486	rBV	368	126	0.01%	0.002%
92	12.268	3489	3492	3494	rVB	510	217	0.02%	0.003%
93	12.632	3603	3605	3608	rBV	383	233	0.02%	0.003%
94	12.776	3648	3650	3652	rBV	232	113	0.01%	0.001%
95	12.821	3661	3664	3665	rBV2	427	227	0.02%	0.003%
96	12.982	3713	3714	3717	rBV	384	185	0.02%	0.002%
97	13.870	3988	3990	3992	rBV3	378	167	0.02%	0.002%
98	14.072	4051	4053	4055	rBV2	353	159	0.02%	0.002%
99	14.329	4130	4133	4137	rBV4	572	440	0.04%	0.006%
100	14.390	4150	4152	4157	rBV3	642	438	0.04%	0.006%




Sum of corrected areas: 7803060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022378.D
Acq On : 29 Sep 2021 15:20
Operator : SY/MD
Sample : M3979-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

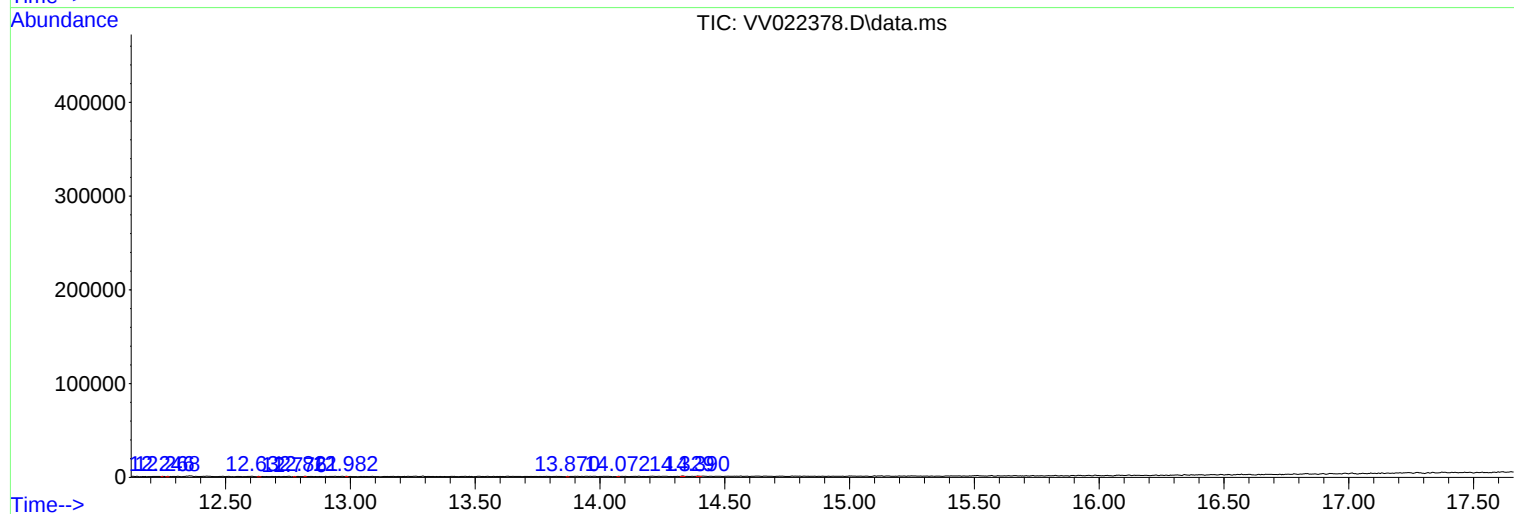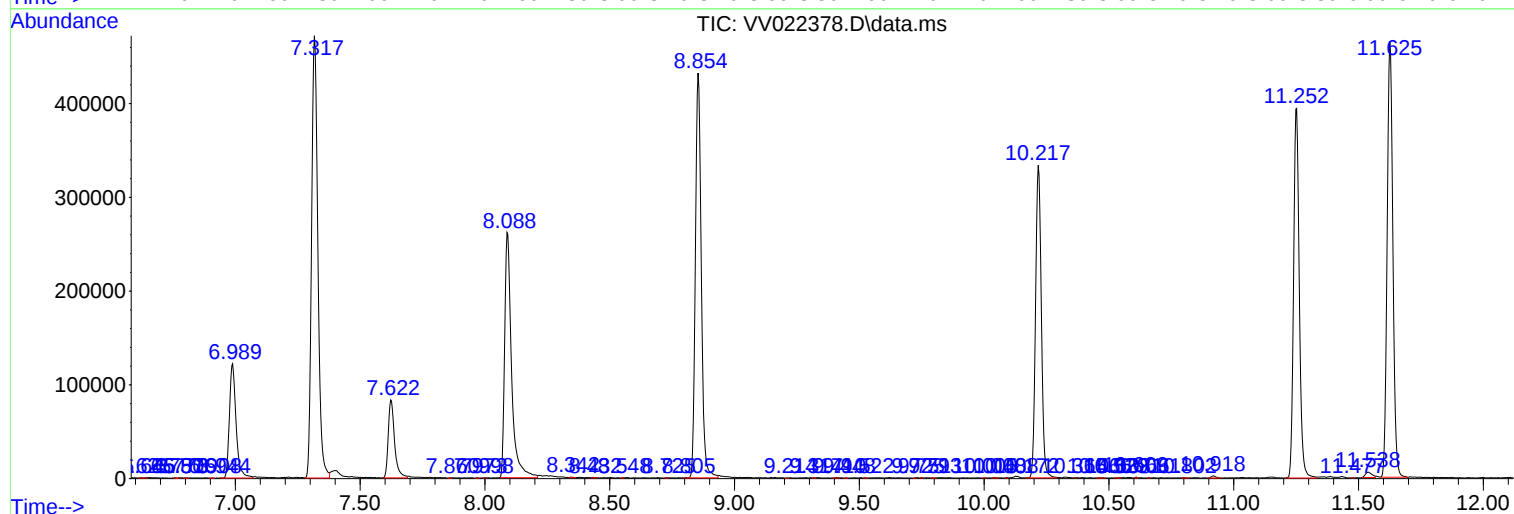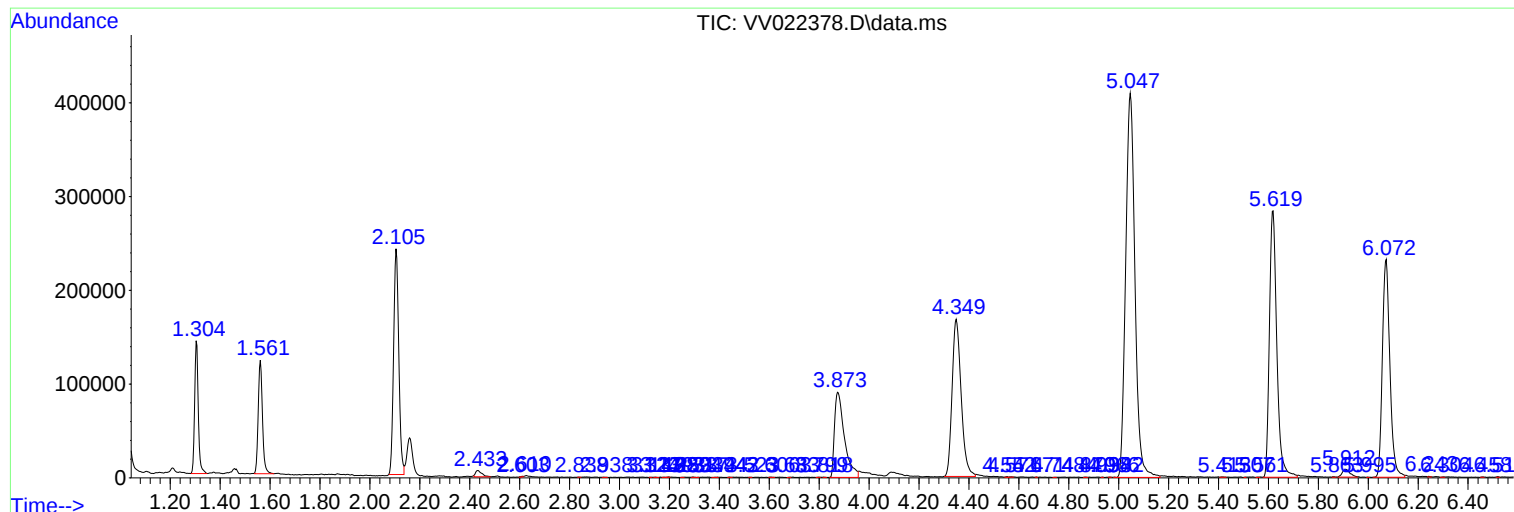

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022378.D
Acq On : 29 Sep 2021 15:20
Operator : SY/MD
Sample : M3979-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022378.D
Acq On : 29 Sep 2021 15:20
Operator : SY/MD
Sample : M3979-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
