

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022380.D
 Acq On : 29 Sep 2021 16:08
 Operator : SY/MD
 Sample : M3979-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	143148	142378	13.53%	1.844%
2	1.561	154	162	180	rBV	120889	143854	13.67%	1.863%
3	2.105	321	331	341	rBV	241358	352693	33.53%	4.568%
4	2.433	427	433	442	rBV3	5703	8862	0.84%	0.115%
5	2.609	482	488	489	rBV2	879	729	0.07%	0.009%
6	2.735	524	527	529	rBV2	271	207	0.02%	0.003%
7	2.793	541	545	551	rVB2	373	291	0.03%	0.004%
8	3.195	668	670	675	rVB2	352	228	0.02%	0.003%
9	3.301	697	703	705	rVB2	330	223	0.02%	0.003%
10	3.423	739	741	744	rVB	460	194	0.02%	0.003%
11	3.625	799	804	807	rVB3	289	302	0.03%	0.004%
12	3.802	855	859	861	rBV3	386	231	0.02%	0.003%
13	3.876	870	882	910	rBV	87649	244748	23.27%	3.170%
14	4.349	1015	1029	1056	rBV2	166387	421179	40.04%	5.455%
15	4.561	1092	1095	1098	rBV3	481	323	0.03%	0.004%
16	4.577	1098	1100	1106	rVB4	725	590	0.06%	0.008%
17	4.732	1145	1148	1151	rVB2	301	201	0.02%	0.003%
18	4.773	1157	1161	1163	rVV3	413	261	0.02%	0.003%
19	5.047	1228	1246	1278	rBV2	408103	1051992	100.00%	13.624%
20	5.246	1306	1308	1310	rBV2	542	218	0.02%	0.003%
21	5.384	1348	1351	1353	rBV3	337	199	0.02%	0.003%
22	5.471	1372	1378	1382	rBV3	446	572	0.05%	0.007%
23	5.542	1398	1400	1404	rVB2	326	195	0.02%	0.003%
24	5.574	1407	1410	1411	rBV	452	281	0.03%	0.004%
25	5.619	1412	1424	1447	rBV	281033	569831	54.17%	7.380%
26	5.844	1490	1494	1496	rBV3	367	259	0.02%	0.003%
27	5.908	1503	1514	1529	rBV4	9845	21693	2.06%	0.281%
28	5.976	1533	1535	1540	rVB3	567	312	0.03%	0.004%
29	6.069	1550	1564	1589	rBV	232990	481572	45.78%	6.237%
30	6.320	1640	1642	1645	rBV2	418	234	0.02%	0.003%
31	6.368	1655	1657	1660	rVB	592	265	0.03%	0.003%
32	6.391	1660	1664	1665	rBV	393	223	0.02%	0.003%
33	6.439	1675	1679	1680	rVV3	502	280	0.03%	0.004%
34	6.503	1694	1699	1700	rBV2	388	259	0.02%	0.003%
35	6.522	1701	1705	1707	rBV2	322	207	0.02%	0.003%
36	6.542	1707	1711	1713	rBV2	466	302	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022380.D
 Acq On : 29 Sep 2021 16:08
 Operator : SY/MD
 Sample : M3979-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.645	1739	1743	1745	rVV2	499	329	0.03%	0.004%
38	6.915	1822	1827	1829	rBV2	422	243	0.02%	0.003%
39	6.989	1837	1850	1868	rBV	121129	220413	20.95%	2.855%
40	7.317	1940	1952	1971	rBV	467886	818919	77.84%	10.606%
41	7.622	2038	2047	2068	rBV	81296	143071	13.60%	1.853%
42	7.850	2114	2118	2119	rBV	330	270	0.03%	0.003%
43	7.863	2120	2122	2126	rVV2	541	383	0.04%	0.005%
44	7.899	2130	2133	2137	rBV3	257	231	0.02%	0.003%
45	7.940	2143	2146	2148	rBV2	354	232	0.02%	0.003%
46	8.091	2183	2193	2222	rBV2	245769	491823	46.75%	6.370%
47	8.423	2294	2296	2300	rVV3	511	275	0.03%	0.004%
48	8.532	2327	2330	2333	rBV3	455	323	0.03%	0.004%
49	8.564	2338	2340	2346	rVB2	283	213	0.02%	0.003%
50	8.638	2360	2363	2365	rBV2	437	272	0.03%	0.004%
51	8.706	2378	2384	2386	rBV4	493	368	0.03%	0.005%
52	8.747	2394	2397	2403	rBV3	582	485	0.05%	0.006%
53	8.776	2403	2406	2409	rBV2	441	227	0.02%	0.003%
54	8.854	2419	2430	2462	rBV	425052	702429	66.77%	9.097%
55	9.091	2501	2504	2507	rVB2	323	234	0.02%	0.003%
56	9.149	2518	2522	2526	rBV4	987	916	0.09%	0.012%
57	9.284	2560	2564	2567	rVV2	360	305	0.03%	0.004%
58	9.583	2652	2657	2659	rBV2	294	249	0.02%	0.003%
59	9.603	2659	2663	2667	rVB3	423	322	0.03%	0.004%
60	9.693	2688	2691	2693	rBV	369	262	0.02%	0.003%
61	9.741	2699	2706	2710	rVB5	639	537	0.05%	0.007%
62	9.763	2710	2713	2716	rBV2	308	274	0.03%	0.004%
63	9.844	2736	2738	2746	rVB3	621	459	0.04%	0.006%
64	9.960	2769	2774	2776	rBV	306	233	0.02%	0.003%
65	10.030	2792	2796	2800	rVB	398	324	0.03%	0.004%
66	10.085	2809	2813	2814	rBV	304	193	0.02%	0.002%
67	10.133	2822	2828	2834	rVB3	1956	2275	0.22%	0.029%
68	10.217	2840	2854	2874	rBV	330519	523624	49.77%	6.781%
69	10.381	2903	2905	2910	rVB4	804	555	0.05%	0.007%
70	10.468	2930	2932	2936	rVB2	446	265	0.03%	0.003%
71	10.580	2965	2967	2970	rVV4	547	364	0.03%	0.005%
72	10.754	3017	3021	3023	rBV2	608	352	0.03%	0.005%
73	10.818	3036	3041	3043	rBV3	420	261	0.02%	0.003%
74	10.882	3058	3061	3064	rBV2	565	322	0.03%	0.004%
75	10.915	3064	3071	3072	rBV4	1178	1228	0.12%	0.016%
76	11.037	3104	3109	3112	rBV2	444	382	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022380.D
 Acq On : 29 Sep 2021 16:08
 Operator : SY/MD
 Sample : M3979-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.107	3128	3131	3136	rBV3	253	205	0.02%	0.003%
78	11.152	3138	3145	3148	rBV4	1345	1514	0.14%	0.020%
79	11.249	3165	3175	3200	rVV	382940	603514	57.37%	7.816%
80	11.471	3239	3244	3245	rBV	263	202	0.02%	0.003%
81	11.535	3254	3264	3273	rBV4	6562	12323	1.17%	0.160%
82	11.625	3281	3292	3317	rVB	466465	735481	69.91%	9.525%
83	11.792	3336	3344	3347	rBV2	1023	1156	0.11%	0.015%
84	11.972	3397	3400	3403	rVB3	420	219	0.02%	0.003%
85	12.101	3438	3440	3445	rVB	526	425	0.04%	0.006%
86	12.352	3513	3518	3519	rBV2	986	737	0.07%	0.010%
87	12.390	3527	3530	3536	rVB2	653	443	0.04%	0.006%
88	12.529	3563	3573	3575	rBV2	472	549	0.05%	0.007%
89	12.606	3594	3597	3603	rVB3	524	494	0.05%	0.006%
90	12.715	3628	3631	3633	rVV4	394	243	0.02%	0.003%
91	12.750	3638	3642	3646	rBV2	451	358	0.03%	0.005%
92	12.873	3677	3680	3685	rBV3	389	360	0.03%	0.005%
93	13.091	3745	3748	3750	rBV2	330	218	0.02%	0.003%
94	13.368	3827	3834	3837	rBV3	674	691	0.07%	0.009%
95	13.680	3926	3931	3933	rBV3	234	235	0.02%	0.003%
96	13.815	3970	3973	3977	rBV2	274	205	0.02%	0.003%
97	13.837	3977	3980	3982	rBV	443	238	0.02%	0.003%
98	14.130	4067	4071	4073	rBV2	535	330	0.03%	0.004%
99	14.750	4263	4264	4269	rVB	549	290	0.03%	0.004%
100	15.477	4489	4490	4492	rBV	505	208	0.02%	0.003%




Sum of corrected areas: 7721468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022380.D
Acq On : 29 Sep 2021 16:08
Operator : SY/MD
Sample : M3979-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

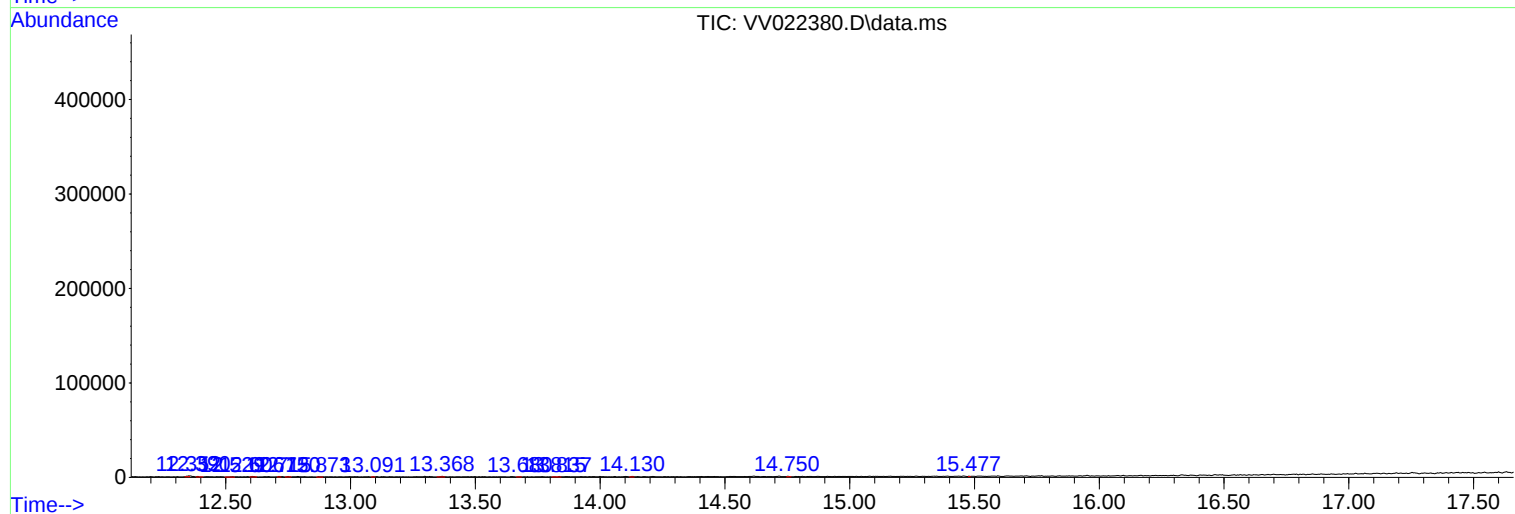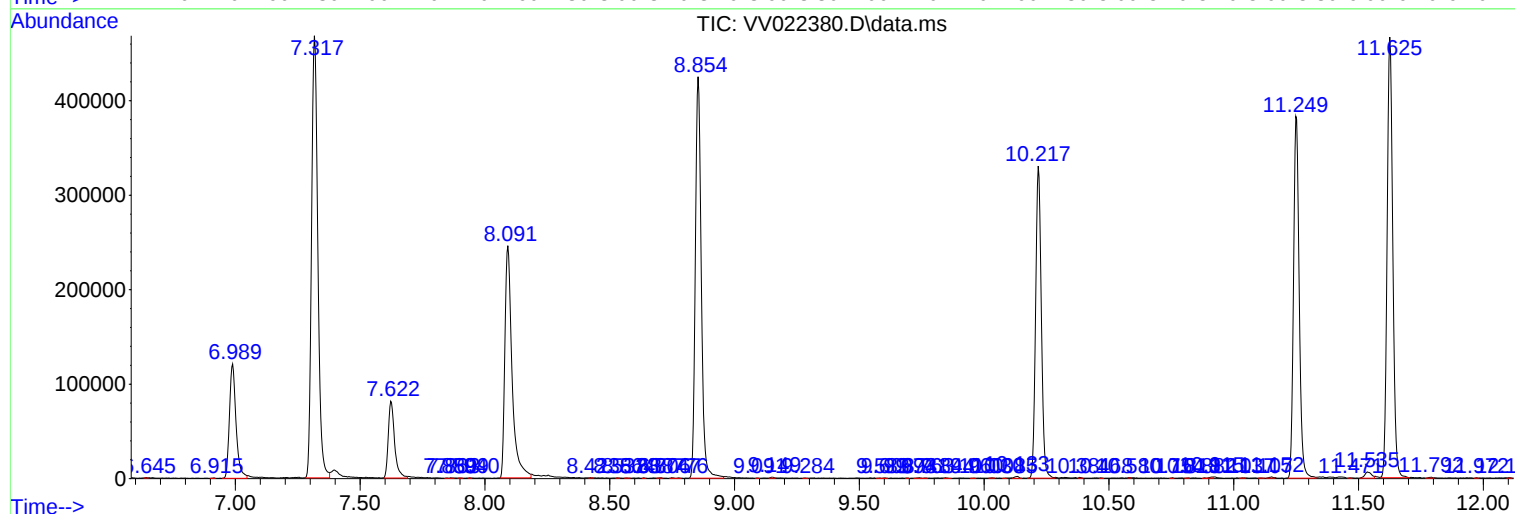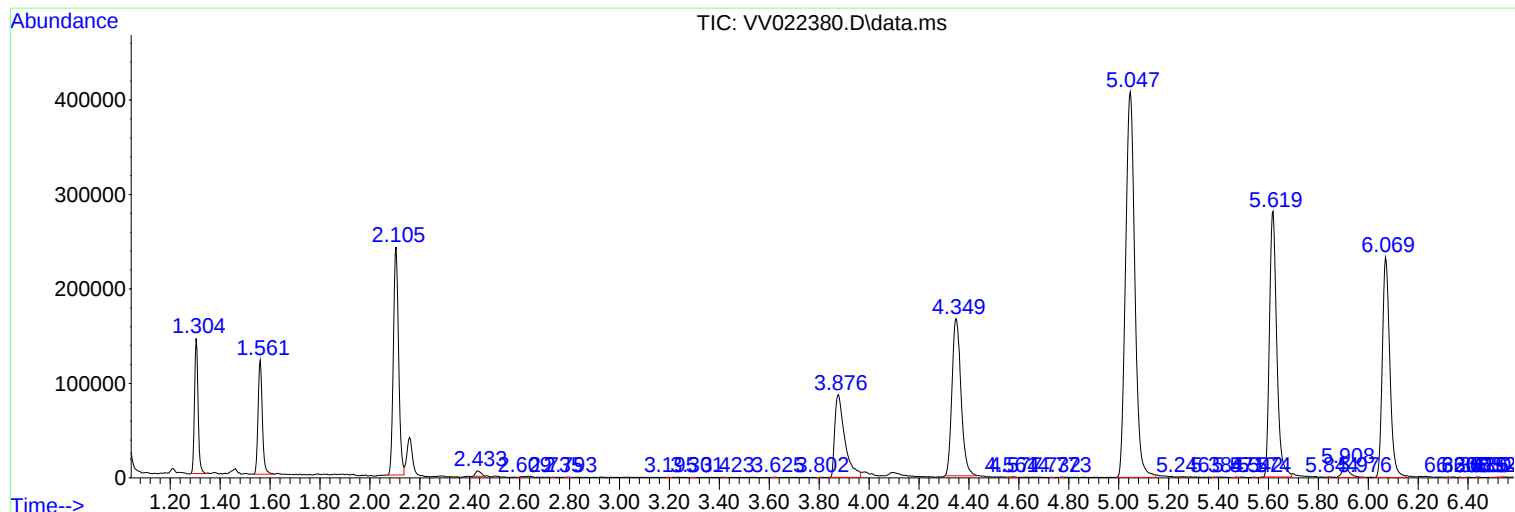

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022380.D
Acq On : 29 Sep 2021 16:08
Operator : SY/MD
Sample : M3979-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022380.D
Acq On : 29 Sep 2021 16:08
Operator : SY/MD
Sample : M3979-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------