

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022381.D
 Acq On : 29 Sep 2021 16:32
 Operator : SY/MD
 Sample : M3978-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	137843	142886	13.64%	1.711%
2	1.561	155	162	176	rVB	116914	137183	13.10%	1.643%
3	2.105	321	331	341	rBV	234898	342578	32.71%	4.103%
4	2.349	404	407	410	rBV2	458	342	0.03%	0.004%
5	2.384	415	418	419	rBV3	491	291	0.03%	0.003%
6	2.503	451	455	461	rBV5	845	915	0.09%	0.011%
7	2.622	481	492	506	rVB4	5404	11441	1.09%	0.137%
8	2.764	531	536	538	rBV2	369	287	0.03%	0.003%
9	2.809	547	550	553	rBV2	308	192	0.02%	0.002%
10	2.921	583	585	589	rBV2	289	204	0.02%	0.002%
11	3.201	667	672	675	rBV3	476	486	0.05%	0.006%
12	3.481	755	759	763	rBV2	206	223	0.02%	0.003%
13	3.529	770	774	776	rVB3	385	226	0.02%	0.003%
14	3.686	821	823	828	rVB3	317	176	0.02%	0.002%
15	3.712	828	831	833	rBV2	402	256	0.02%	0.003%
16	3.764	843	847	851	rVB3	299	278	0.03%	0.003%
17	3.876	871	882	917	rBV2	98715	308719	29.48%	3.698%
18	4.349	1014	1029	1056	rBV	162228	414808	39.61%	4.968%
19	4.571	1095	1098	1100	rVB2	483	287	0.03%	0.003%
20	4.590	1102	1104	1107	rVB2	792	375	0.04%	0.004%
21	4.612	1107	1111	1114	rBV3	759	550	0.05%	0.007%
22	4.831	1175	1179	1183	rBV3	441	388	0.04%	0.005%
23	5.047	1229	1246	1280	rBV2	407671	1047217	100.00%	12.543%
24	5.243	1306	1307	1313	rVB2	791	552	0.05%	0.007%
25	5.291	1320	1322	1327	rBV4	502	525	0.05%	0.006%
26	5.375	1345	1348	1353	rVB3	629	376	0.04%	0.005%
27	5.497	1385	1386	1391	rVB2	541	325	0.03%	0.004%
28	5.522	1391	1394	1400	rVB4	475	389	0.04%	0.005%
29	5.619	1411	1424	1453	rBV	278585	569332	54.37%	6.819%
30	5.918	1504	1517	1532	rBV3	36685	79218	7.56%	0.949%
31	6.072	1551	1565	1590	rBV	231442	478812	45.72%	5.735%
32	6.358	1650	1654	1660	rBV4	749	609	0.06%	0.007%
33	6.461	1684	1686	1689	rBV	370	244	0.02%	0.003%
34	6.616	1731	1734	1737	rBV3	328	209	0.02%	0.003%
35	6.657	1744	1747	1748	rBV2	433	213	0.02%	0.003%
36	6.915	1824	1827	1832	rBV3	341	231	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022381.D
 Acq On : 29 Sep 2021 16:32
 Operator : SY/MD
 Sample : M3978-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.989	1838	1850	1877	rBV	117417	218421	20.86%	2.616%
38	7.317	1939	1952	1969	rBV	471437	819237	78.23%	9.813%
39	7.574	2029	2032	2035	rBV4	493	320	0.03%	0.004%
40	7.622	2037	2047	2068	rBV	81052	146396	13.98%	1.754%
41	7.809	2102	2105	2108	rVB3	437	328	0.03%	0.004%
42	7.892	2128	2131	2133	rBV3	383	190	0.02%	0.002%
43	7.976	2145	2157	2174	rBV	313249	532150	50.82%	6.374%
44	8.088	2182	2192	2227	rBV	265882	500411	47.78%	5.994%
45	8.358	2274	2276	2279	rVB3	819	410	0.04%	0.005%
46	8.400	2286	2289	2290	rBV2	607	306	0.03%	0.004%
47	8.481	2310	2314	2316	rBV2	411	330	0.03%	0.004%
48	8.503	2319	2321	2324	rVV	424	225	0.02%	0.003%
49	8.545	2331	2334	2335	rBV3	342	208	0.02%	0.002%
50	8.574	2340	2343	2345	rBV2	468	202	0.02%	0.002%
51	8.677	2372	2375	2378	rBV	385	266	0.03%	0.003%
52	8.693	2378	2380	2383	rBV3	478	273	0.03%	0.003%
53	8.853	2418	2430	2452	rBV	424916	694149	66.29%	8.314%
54	9.075	2496	2499	2502	rBV3	254	181	0.02%	0.002%
55	9.233	2546	2548	2551	rVB3	370	206	0.02%	0.002%
56	9.323	2574	2576	2580	rBV3	217	209	0.02%	0.003%
57	9.429	2605	2609	2612	rBV3	271	238	0.02%	0.003%
58	9.542	2642	2644	2646	rVV	394	179	0.02%	0.002%
59	9.593	2658	2660	2666	rVB3	304	332	0.03%	0.004%
60	9.709	2694	2696	2702	rBV3	228	220	0.02%	0.003%
61	9.792	2719	2722	2730	rVB5	315	320	0.03%	0.004%
62	9.850	2736	2740	2744	rBV2	293	239	0.02%	0.003%
63	9.931	2761	2765	2767	rBV2	332	194	0.02%	0.002%
64	9.976	2772	2779	2781	rBV2	461	461	0.04%	0.006%
65	10.127	2819	2826	2833	rBV3	1750	2002	0.19%	0.024%
66	10.175	2837	2841	2843	rBV	335	264	0.03%	0.003%
67	10.217	2843	2854	2877	rBV	348940	542778	51.83%	6.501%
68	10.458	2925	2929	2932	rBV3	481	380	0.04%	0.005%
69	10.513	2944	2946	2950	rVB	413	284	0.03%	0.003%
70	10.532	2950	2952	2955	rBV2	326	244	0.02%	0.003%
71	10.574	2962	2965	2966	rBV2	509	211	0.02%	0.003%
72	10.587	2966	2969	2973	rVB4	419	298	0.03%	0.004%
73	10.677	2995	2997	3001	rVB2	386	272	0.03%	0.003%
74	10.725	3008	3012	3015	rVB	278	185	0.02%	0.002%
75	10.757	3018	3022	3025	rBV3	321	263	0.03%	0.003%
76	10.773	3025	3027	3031	rBV3	407	294	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022381.D
 Acq On : 29 Sep 2021 16:32
 Operator : SY/MD
 Sample : M3978-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.921	3064	3073	3080	rVB5	1878	2486	0.24%	0.030%
78	10.963	3084	3086	3088	rBV	306	176	0.02%	0.002%
79	11.027	3102	3106	3108	rBV2	406	294	0.03%	0.004%
80	11.143	3137	3142	3145	rBV3	907	867	0.08%	0.010%
81	11.191	3153	3157	3160	rBV2	438	297	0.03%	0.004%
82	11.252	3165	3176	3199	rBV	377857	601924	57.48%	7.210%
83	11.384	3212	3217	3221	rBV4	915	724	0.07%	0.009%
84	11.532	3260	3263	3264	rBV2	346	216	0.02%	0.003%
85	11.625	3279	3292	3314	rBV	463572	732259	69.92%	8.771%
86	11.979	3400	3402	3407	rVB	521	339	0.03%	0.004%
87	12.014	3410	3413	3416	rBV3	451	285	0.03%	0.003%
88	12.365	3520	3522	3526	rBV2	246	233	0.02%	0.003%
89	12.413	3533	3537	3539	rBV2	319	259	0.02%	0.003%
90	12.583	3582	3590	3595	rBV3	324	497	0.05%	0.006%
91	12.673	3615	3618	3620	rBV2	498	324	0.03%	0.004%
92	12.728	3633	3635	3637	rBV2	429	190	0.02%	0.002%
93	12.882	3681	3683	3690	rVB3	354	302	0.03%	0.004%
94	13.242	3793	3795	3798	rVB3	455	190	0.02%	0.002%
95	13.561	3891	3894	3897	rBV	305	186	0.02%	0.002%
96	13.619	3909	3912	3913	rBV	345	197	0.02%	0.002%
97	13.927	4004	4008	4011	rBV2	436	334	0.03%	0.004%
98	14.008	4030	4033	4036	rBV3	455	341	0.03%	0.004%
99	14.233	4100	4103	4104	rBV	354	214	0.02%	0.003%
100	14.303	4122	4125	4127	rBV2	357	220	0.02%	0.003%




Sum of corrected areas: 8348773

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022381.D
Acq On : 29 Sep 2021 16:32
Operator : SY/MD
Sample : M3978-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

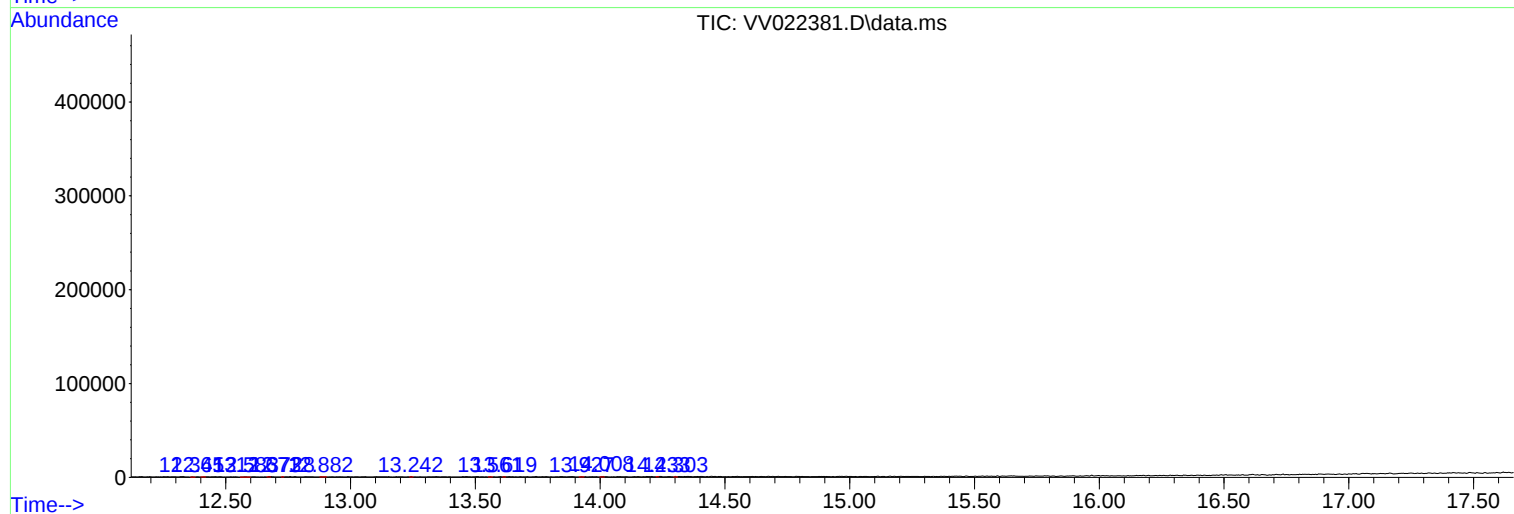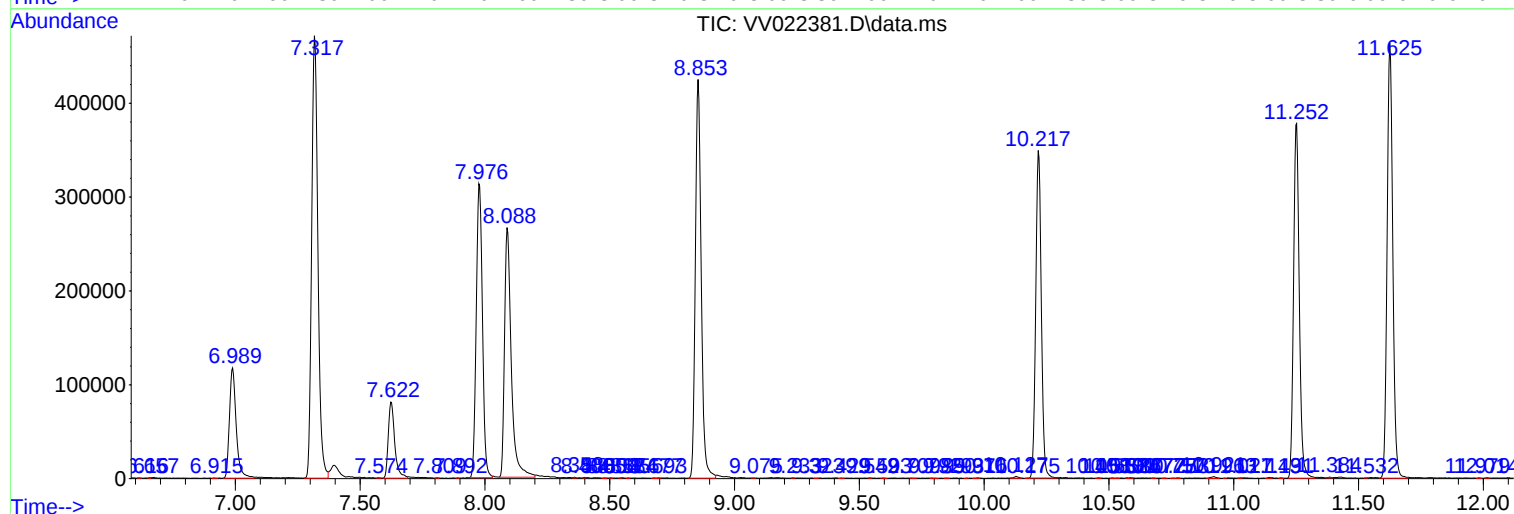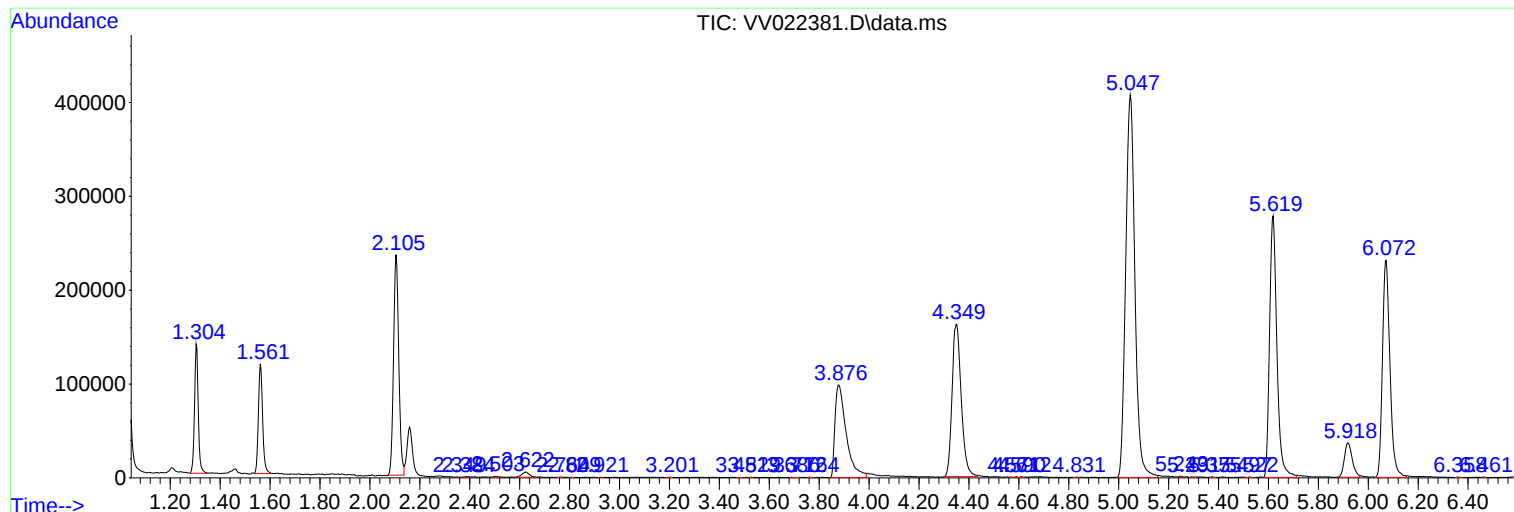

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022381.D
Acq On : 29 Sep 2021 16:32
Operator : SY/MD
Sample : M3978-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022381.D
Acq On : 29 Sep 2021 16:32
Operator : SY/MD
Sample : M3978-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
