

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022388.D
 Acq On : 29 Sep 2021 19:19
 Operator : SY/MD
 Sample : M3978-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	128034	126188	7.54%	1.394%
2	1.561	155	162	174	rVB	109273	129348	7.73%	1.429%
3	2.105	321	331	358	rVB	220319	335924	20.08%	3.711%
4	2.577	473	478	481	rBV3	310	314	0.02%	0.003%
5	2.683	509	511	515	rBV3	324	281	0.02%	0.003%
6	2.770	524	538	550	rBV4	4777	11201	0.67%	0.124%
7	2.905	578	580	583	rVB	407	234	0.01%	0.003%
8	3.027	615	618	621	rVB	480	277	0.02%	0.003%
9	3.082	631	635	638	rBV2	449	346	0.02%	0.004%
10	3.191	665	669	670	rBV3	331	215	0.01%	0.002%
11	3.224	675	679	684	rBV3	368	301	0.02%	0.003%
12	3.355	717	720	723	rVB	322	208	0.01%	0.002%
13	3.384	723	729	732	rBV2	401	363	0.02%	0.004%
14	3.417	732	739	742	rBV	401	439	0.03%	0.005%
15	3.455	747	751	757	rVV3	210	208	0.01%	0.002%
16	3.626	801	804	809	rVB4	468	354	0.02%	0.004%
17	3.716	828	832	836	rBV2	379	360	0.02%	0.004%
18	3.806	856	860	864	rBV2	409	314	0.02%	0.003%
19	3.873	872	881	916	rBV2	79764	234431	14.02%	2.590%
20	4.352	1013	1030	1053	rBV	151551	391756	23.42%	4.328%
21	4.564	1093	1096	1098	rBV2	413	244	0.01%	0.003%
22	4.844	1180	1183	1190	rBV3	384	345	0.02%	0.004%
23	4.902	1197	1201	1205	rBV2	351	235	0.01%	0.003%
24	4.934	1208	1211	1214	rVB2	327	265	0.02%	0.003%
25	4.957	1214	1218	1220	rBV	392	279	0.02%	0.003%
26	5.047	1227	1246	1285	rBV2	385659	997673	59.65%	11.021%
27	5.291	1319	1322	1324	rBV	459	238	0.01%	0.003%
28	5.355	1339	1342	1344	rBV	498	257	0.02%	0.003%
29	5.420	1358	1362	1363	rBV3	319	241	0.01%	0.003%
30	5.497	1383	1386	1389	rBV2	402	300	0.02%	0.003%
31	5.513	1389	1391	1394	rVB3	546	241	0.01%	0.003%
32	5.532	1394	1397	1398	rBV2	313	191	0.01%	0.002%
33	5.616	1410	1423	1454	rBV	269022	550811	32.93%	6.085%
34	5.918	1502	1517	1534	rBV6	15172	35444	2.12%	0.392%
35	6.069	1548	1564	1592	rBV	220059	455811	27.25%	5.035%
36	6.265	1623	1625	1626	rBV2	444	227	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022388.D
 Acq On : 29 Sep 2021 19:19
 Operator : SY/MD
 Sample : M3978-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.461	1682	1686	1690	rBV3	446	374	0.02%	0.004%
38	6.535	1708	1709	1712	rVB2	635	247	0.01%	0.003%
39	6.600	1725	1729	1731	rBV	318	198	0.01%	0.002%
40	6.989	1839	1850	1874	rBV	109356	204130	12.20%	2.255%
41	7.162	1902	1904	1907	rBV2	519	237	0.01%	0.003%
42	7.178	1907	1909	1911	rBV2	473	258	0.02%	0.003%
43	7.317	1940	1952	1972	rBV	439952	781531	46.73%	8.633%
44	7.539	2019	2021	2023	rBV2	376	201	0.01%	0.002%
45	7.622	2036	2047	2072	rBV	77045	138855	8.30%	1.534%
46	7.860	2119	2121	2125	rVB2	475	281	0.02%	0.003%
47	7.976	2143	2157	2178	rBV	998407	1672609	100.00%	18.477%
48	8.088	2183	2192	2226	rVB	263967	479925	28.69%	5.302%
49	8.371	2277	2280	2284	rVB3	693	408	0.02%	0.005%
50	8.387	2284	2285	2289	rBV4	347	198	0.01%	0.002%
51	8.423	2294	2296	2299	rBV2	356	208	0.01%	0.002%
52	8.854	2419	2430	2449	rBV	410531	668892	39.99%	7.389%
53	9.149	2514	2522	2525	rBV4	618	644	0.04%	0.007%
54	9.165	2525	2527	2531	rVV3	506	353	0.02%	0.004%
55	9.201	2536	2538	2541	rVB2	477	204	0.01%	0.002%
56	9.445	2613	2614	2618	rVB3	456	224	0.01%	0.002%
57	9.468	2618	2621	2623	rBV	308	230	0.01%	0.003%
58	9.555	2643	2648	2649	rVV3	255	211	0.01%	0.002%
59	9.767	2708	2714	2717	rBV3	471	449	0.03%	0.005%
60	9.796	2720	2723	2726	rBV	364	220	0.01%	0.002%
61	9.921	2760	2762	2765	rBV	399	229	0.01%	0.003%
62	10.030	2793	2796	2798	rVB2	380	210	0.01%	0.002%
63	10.127	2817	2826	2828	rBV5	1193	1257	0.08%	0.014%
64	10.217	2841	2854	2874	rBV	329689	527310	31.53%	5.825%
65	10.349	2892	2895	2898	rBV3	324	212	0.01%	0.002%
66	10.387	2903	2907	2912	rVB3	410	364	0.02%	0.004%
67	10.464	2929	2931	2935	rVB2	377	249	0.01%	0.003%
68	10.555	2957	2959	2961	rVV2	507	237	0.01%	0.003%
69	10.574	2961	2965	2969	rVB5	390	419	0.03%	0.005%
70	10.747	3015	3019	3022	rVB2	349	277	0.02%	0.003%
71	10.828	3039	3044	3047	rBV3	322	329	0.02%	0.004%
72	11.024	3103	3105	3108	rBV3	375	279	0.02%	0.003%
73	11.252	3164	3176	3203	rVV	371100	586388	35.06%	6.478%
74	11.390	3217	3219	3225	rVB3	942	693	0.04%	0.008%
75	11.503	3250	3254	3257	rBV	496	318	0.02%	0.004%
76	11.522	3257	3260	3262	rBV2	280	211	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022388.D
 Acq On : 29 Sep 2021 19:19
 Operator : SY/MD
 Sample : M3978-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.625	3280	3292	3316	rBV	445469	700021	41.85%	7.733%
78	11.763	3333	3335	3337	rBV2	513	201	0.01%	0.002%
79	11.780	3337	3340	3341	rBV2	518	221	0.01%	0.002%
80	11.844	3358	3360	3365	rVB	394	247	0.01%	0.003%
81	11.866	3365	3367	3370	rBV3	312	213	0.01%	0.002%
82	11.992	3400	3406	3408	rBV3	435	410	0.02%	0.005%
83	12.056	3423	3426	3429	rBV2	469	270	0.02%	0.003%
84	12.143	3450	3453	3455	rBV2	250	197	0.01%	0.002%
85	12.178	3462	3464	3468	rBV2	399	288	0.02%	0.003%
86	12.259	3484	3489	3492	rBV3	425	375	0.02%	0.004%
87	12.278	3493	3495	3499	rBV	334	280	0.02%	0.003%
88	12.493	3561	3562	3565	rBV	347	212	0.01%	0.002%
89	12.513	3565	3568	3575	rVB3	380	395	0.02%	0.004%
90	13.008	3718	3722	3723	rBV	334	256	0.02%	0.003%
91	13.124	3755	3758	3762	rBV2	324	262	0.02%	0.003%
92	13.233	3789	3792	3795	rBV2	339	249	0.01%	0.003%
93	13.677	3926	3930	3932	rVB	377	223	0.01%	0.002%
94	13.808	3967	3971	3974	rBV2	495	346	0.02%	0.004%
95	13.860	3984	3987	3992	rBV3	251	203	0.01%	0.002%
96	13.985	4022	4026	4027	rVB2	390	233	0.01%	0.003%
97	14.059	4046	4049	4054	rBV3	306	246	0.01%	0.003%
98	14.162	4079	4081	4086	rBV2	371	280	0.02%	0.003%
99	14.242	4100	4106	4110	rBV3	521	593	0.04%	0.007%
100	14.722	4252	4255	4256	rBV	467	255	0.02%	0.003%




Sum of corrected areas: 9052409

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022388.D
Acq On : 29 Sep 2021 19:19
Operator : SY/MD
Sample : M3978-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

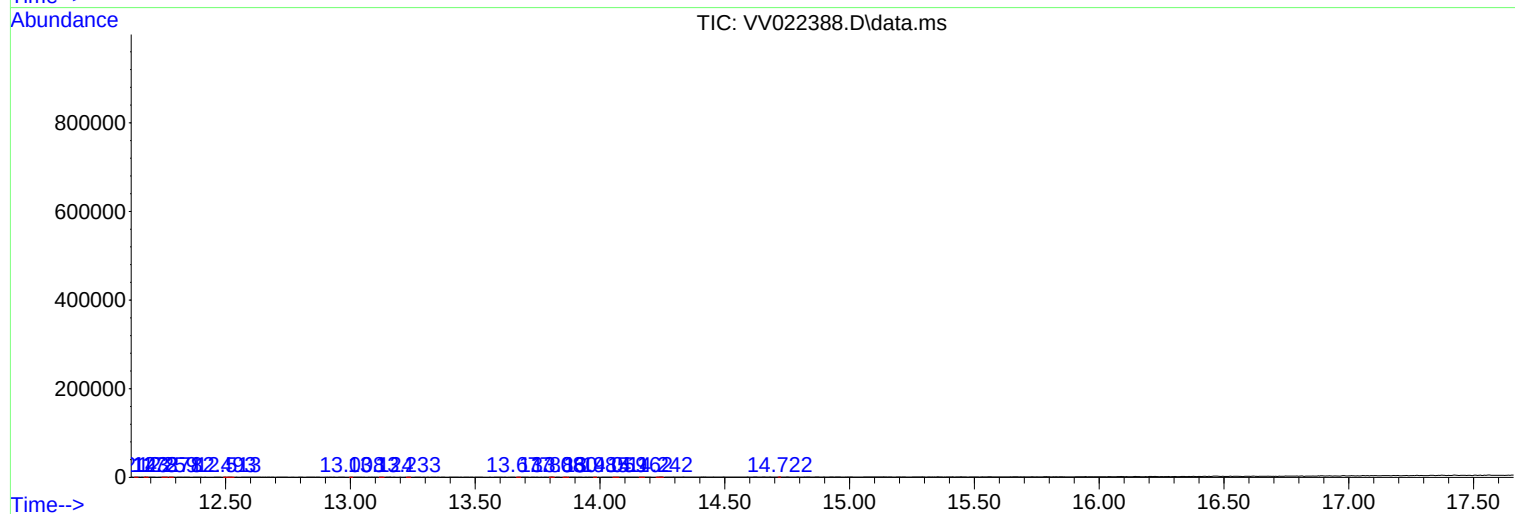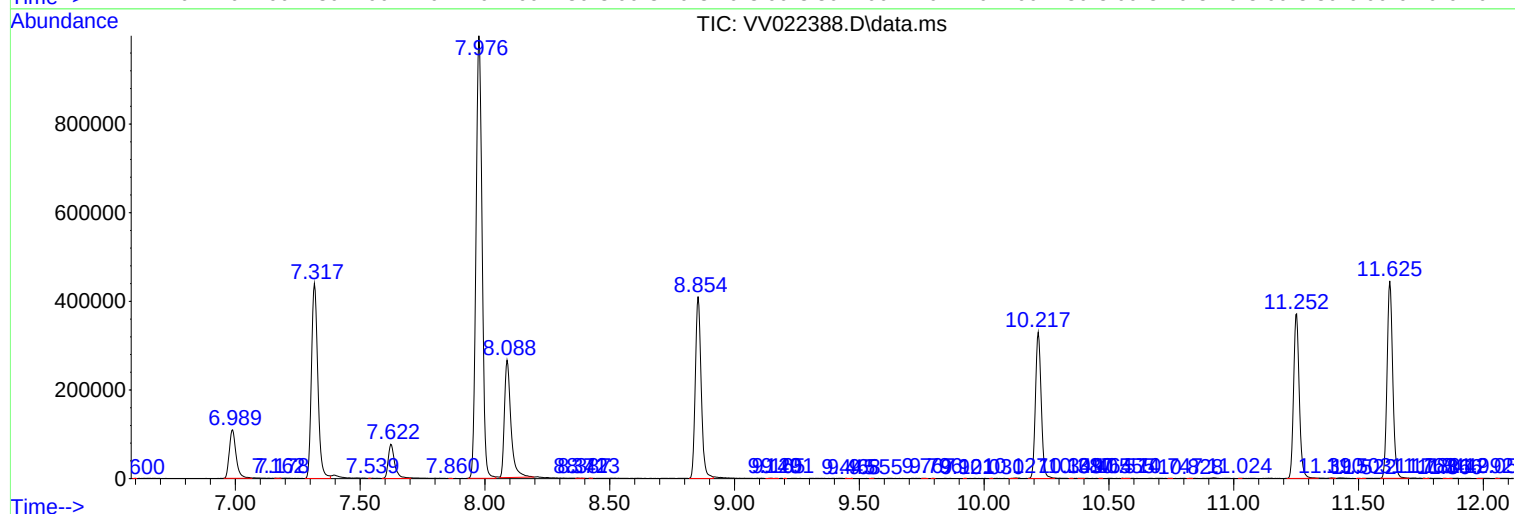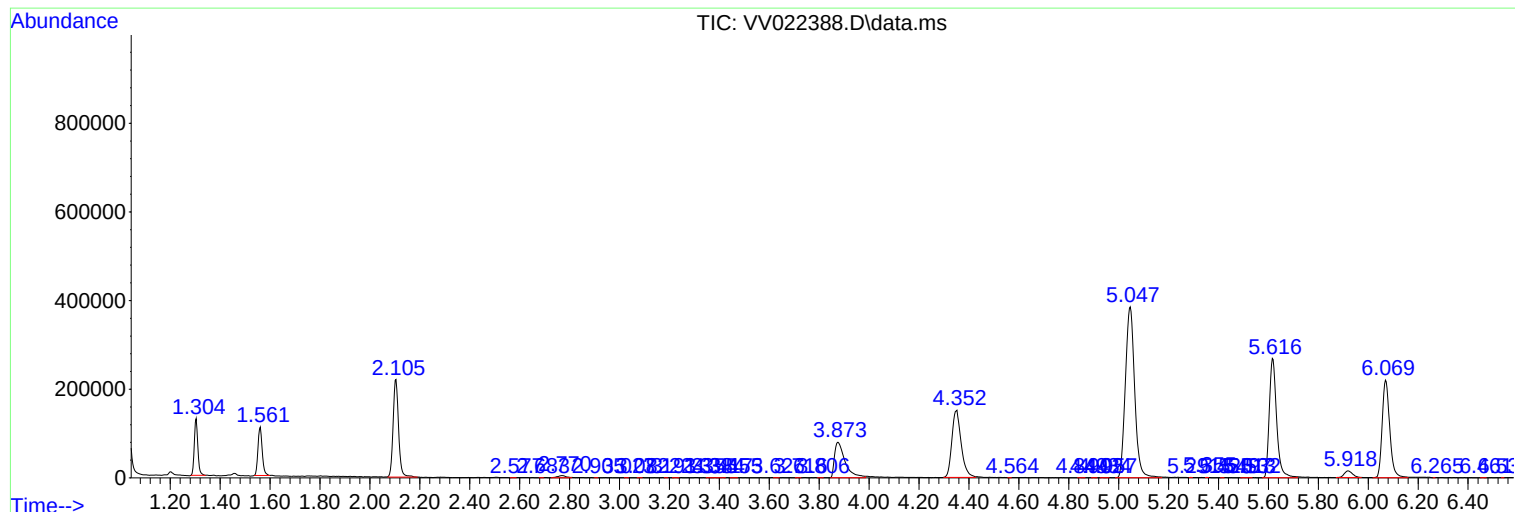

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022388.D
Acq On : 29 Sep 2021 19:19
Operator : SY/MD
Sample : M3978-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022388.D
Acq On : 29 Sep 2021 19:19
Operator : SY/MD
Sample : M3978-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
