

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022389.D
 Acq On : 29 Sep 2021 19:44
 Operator : SY/MD
 Sample : M3978-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	123750	126502	7.07%	1.404%
2	1.558	154	161	177	rVB	107481	124878	6.98%	1.386%
3	2.101	320	330	351	rBV	216988	323215	18.07%	3.588%
4	2.526	460	462	467	rVB2	577	433	0.02%	0.005%
5	2.555	467	471	475	rBV2	467	589	0.03%	0.007%
6	2.632	494	495	499	rVB	1126	440	0.02%	0.005%
7	2.654	499	502	503	rBV	359	171	0.01%	0.002%
8	2.706	513	518	520	rBV2	389	273	0.02%	0.003%
9	2.764	527	536	547	rBV3	4978	9979	0.56%	0.111%
10	2.857	561	565	570	rBV3	474	432	0.02%	0.005%
11	2.998	605	609	612	rBV2	417	248	0.01%	0.003%
12	3.021	612	616	618	rBV2	350	308	0.02%	0.003%
13	3.371	723	725	728	rVB2	509	237	0.01%	0.003%
14	3.400	730	734	736	rVV2	401	179	0.01%	0.002%
15	3.439	745	746	752	rVB2	369	227	0.01%	0.003%
16	3.873	871	881	909	rBV	81107	225078	12.58%	2.498%
17	4.349	1013	1029	1062	rBV	147177	384806	21.51%	4.271%
18	4.622	1112	1114	1116	rVB	466	207	0.01%	0.002%
19	4.638	1116	1119	1121	rBV	358	193	0.01%	0.002%
20	4.680	1128	1132	1136	rBV4	492	526	0.03%	0.006%
21	4.937	1209	1212	1215	rBV2	305	177	0.01%	0.002%
22	4.957	1215	1218	1223	rVB3	615	441	0.02%	0.005%
23	4.979	1223	1225	1228	rBV	221	170	0.01%	0.002%
24	5.043	1228	1245	1279	rBV2	380546	980666	54.82%	10.886%
25	5.468	1370	1377	1378	rBV3	330	273	0.02%	0.003%
26	5.526	1394	1395	1398	rBV	369	233	0.01%	0.003%
27	5.555	1401	1404	1407	rVB2	538	269	0.02%	0.003%
28	5.616	1407	1423	1454	rBV	262820	538485	30.10%	5.977%
29	5.918	1505	1517	1536	rVB7	16494	38742	2.17%	0.430%
30	6.069	1551	1564	1597	rVV	219857	451840	25.26%	5.016%
31	6.281	1625	1630	1636	rBV3	828	800	0.04%	0.009%
32	6.339	1645	1648	1651	rBV3	307	241	0.01%	0.003%
33	6.529	1704	1707	1709	rBV3	284	194	0.01%	0.002%
34	6.583	1722	1724	1726	rBV	378	158	0.01%	0.002%
35	6.606	1728	1731	1732	rBV2	407	200	0.01%	0.002%
36	6.696	1757	1759	1762	rBV2	327	164	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022389.D
 Acq On : 29 Sep 2021 19:44
 Operator : SY/MD
 Sample : M3978-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.780	1782	1785	1790	rBV2	261	184	0.01%	0.002%
38	6.985	1837	1849	1873	rBV	109525	203697	11.39%	2.261%
39	7.185	1908	1911	1913	rBV3	766	345	0.02%	0.004%
40	7.317	1940	1952	1970	rBV	439159	761726	42.58%	8.455%
41	7.622	2037	2047	2072	rBV	75522	135626	7.58%	1.505%
42	7.976	2143	2157	2182	rBV	1063640	1788970	100.00%	19.858%
43	8.088	2183	2192	2223	rVV	262899	466227	26.06%	5.175%
44	8.542	2329	2333	2334	rBV	466	312	0.02%	0.003%
45	8.657	2366	2369	2372	rBV2	451	351	0.02%	0.004%
46	8.722	2386	2389	2393	rVB3	359	190	0.01%	0.002%
47	8.744	2393	2396	2397	rBV3	356	206	0.01%	0.002%
48	8.854	2419	2430	2450	rBV	405822	655733	36.65%	7.279%
49	9.021	2479	2482	2488	rVB3	776	743	0.04%	0.008%
50	9.050	2488	2491	2495	rBV2	588	419	0.02%	0.005%
51	9.069	2495	2497	2501	rBV2	402	255	0.01%	0.003%
52	9.136	2514	2518	2519	rBV2	516	369	0.02%	0.004%
53	9.230	2544	2547	2550	rBV	412	269	0.02%	0.003%
54	9.358	2583	2587	2592	rBV3	382	373	0.02%	0.004%
55	9.464	2618	2620	2624	rBV	250	165	0.01%	0.002%
56	9.574	2652	2654	2656	rBV2	457	260	0.01%	0.003%
57	9.686	2684	2689	2691	rBV2	650	409	0.02%	0.005%
58	9.747	2706	2708	2709	rBV2	457	184	0.01%	0.002%
59	9.927	2761	2764	2766	rBV2	236	160	0.01%	0.002%
60	9.966	2773	2776	2777	rBV2	281	179	0.01%	0.002%
61	10.062	2804	2806	2809	rVB2	446	174	0.01%	0.002%
62	10.104	2814	2819	2821	rBV	372	291	0.02%	0.003%
63	10.217	2841	2854	2875	rBV	332673	515516	28.82%	5.722%
64	10.358	2896	2898	2902	rBV3	412	388	0.02%	0.004%
65	10.439	2919	2923	2924	rBV2	234	175	0.01%	0.002%
66	10.461	2928	2930	2932	rBV3	320	195	0.01%	0.002%
67	10.516	2945	2947	2950	rVB2	351	184	0.01%	0.002%
68	10.673	2993	2996	2998	rBV2	303	175	0.01%	0.002%
69	10.924	3068	3074	3079	rVV6	1079	1408	0.08%	0.016%
70	11.001	3096	3098	3100	rBV2	372	218	0.01%	0.002%
71	11.146	3139	3143	3144	rBV	483	279	0.02%	0.003%
72	11.252	3164	3176	3193	rBV	363801	570477	31.89%	6.332%
73	11.426	3225	3230	3233	rBV4	719	788	0.04%	0.009%
74	11.519	3257	3259	3262	rBV3	432	303	0.02%	0.003%
75	11.625	3281	3292	3308	rBV	435349	681654	38.10%	7.566%
76	11.734	3324	3326	3328	rBV2	414	247	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022389.D
 Acq On : 29 Sep 2021 19:44
 Operator : SY/MD
 Sample : M3978-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.908	3377	3380	3384	rBV4	361	294	0.02%	0.003%
78	12.014	3412	3413	3416	rBV	434	189	0.01%	0.002%
79	12.033	3416	3419	3422	rBV2	305	207	0.01%	0.002%
80	12.101	3438	3440	3445	rVB2	298	238	0.01%	0.003%
81	12.127	3446	3448	3451	rVB2	373	227	0.01%	0.003%
82	12.165	3451	3460	3467	rBV3	453	894	0.05%	0.010%
83	12.242	3481	3484	3487	rBV2	366	289	0.02%	0.003%
84	12.368	3520	3523	3528	rVB2	401	269	0.02%	0.003%
85	12.455	3547	3550	3553	rVB	326	209	0.01%	0.002%
86	12.516	3565	3569	3574	rBV2	268	374	0.02%	0.004%
87	12.911	3686	3692	3695	rBV2	409	388	0.02%	0.004%
88	12.927	3695	3697	3699	rBV	358	182	0.01%	0.002%
89	13.130	3757	3760	3762	rBV	328	163	0.01%	0.002%
90	13.439	3854	3856	3860	rBV2	402	218	0.01%	0.002%
91	13.529	3882	3884	3888	rBV3	325	205	0.01%	0.002%
92	13.795	3965	3967	3972	rVB2	446	345	0.02%	0.004%
93	13.824	3975	3976	3977	rBV2	552	185	0.01%	0.002%
94	13.889	3993	3996	3999	rBV3	388	265	0.01%	0.003%
95	14.024	4036	4038	4042	rVB2	437	294	0.02%	0.003%
96	14.265	4110	4113	4115	rVB2	434	264	0.01%	0.003%
97	14.287	4115	4120	4122	rBV2	411	421	0.02%	0.005%
98	14.352	4137	4140	4144	rBV3	439	280	0.02%	0.003%
99	14.500	4184	4186	4189	rVB3	514	244	0.01%	0.003%
100	15.072	4361	4364	4366	rVB2	705	414	0.02%	0.005%



Sum of corrected areas: 9008856

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022389.D
Acq On : 29 Sep 2021 19:44
Operator : SY/MD
Sample : M3978-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

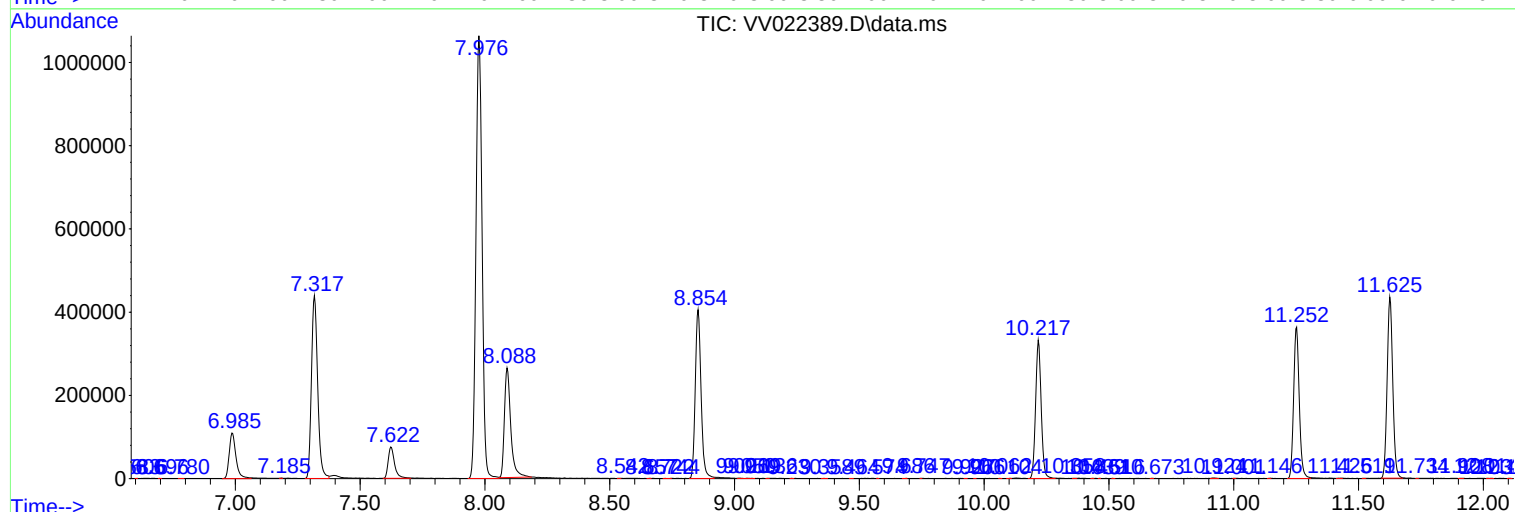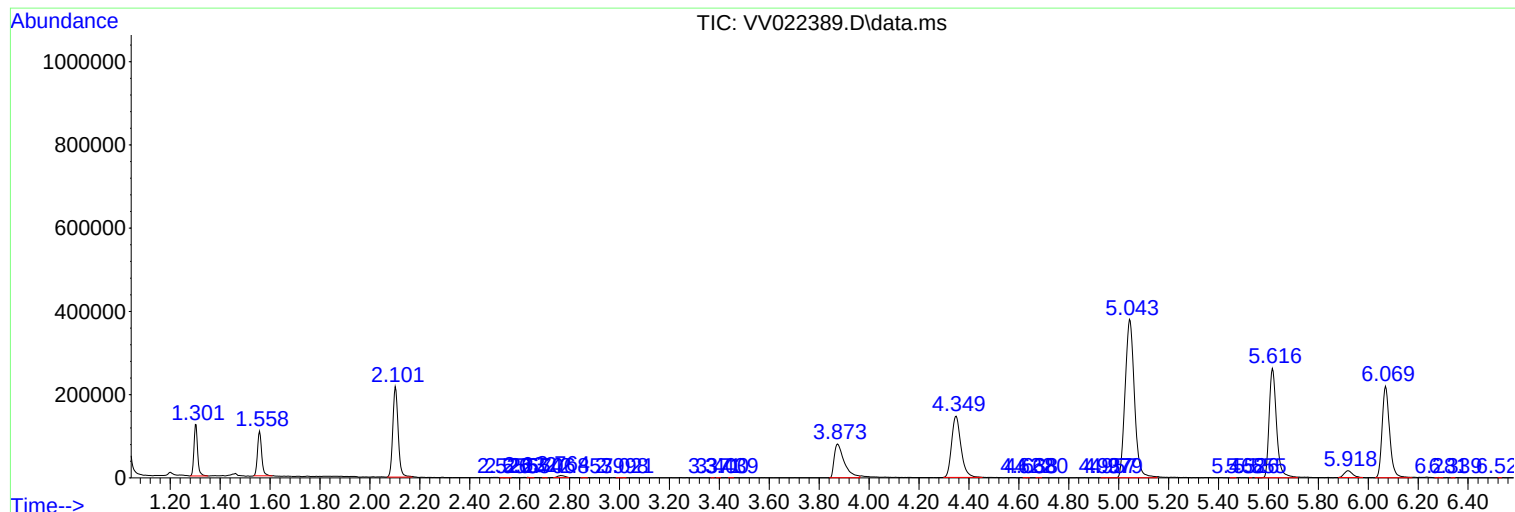

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022389.D
Acq On : 29 Sep 2021 19:44
Operator : SY/MD
Sample : M3978-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022389.D
Acq On : 29 Sep 2021 19:44
Operator : SY/MD
Sample : M3978-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc