

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022391.D
 Acq On : 29 Sep 2021 20:32
 Operator : SY/MD
 Sample : M3978-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	95	rVB	121610	124306	6.70%	1.330%
2	1.561	156	162	173	rVB	114216	128293	6.92%	1.373%
3	2.104	321	331	353	rBV	224855	335200	18.08%	3.587%
4	2.503	452	455	459	rBV2	673	527	0.03%	0.006%
5	2.561	469	473	476	rBV5	542	473	0.03%	0.005%
6	2.619	484	491	496	rBV4	717	988	0.05%	0.011%
7	2.767	530	537	552	rVB4	5341	11494	0.62%	0.123%
8	2.821	552	554	558	rBV2	327	200	0.01%	0.002%
9	2.838	558	559	564	rVV2	322	215	0.01%	0.002%
10	2.944	590	592	594	rVV	327	146	0.01%	0.002%
11	2.976	598	602	607	rBV3	283	263	0.01%	0.003%
12	3.104	638	642	643	rBV	447	306	0.02%	0.003%
13	3.143	647	654	655	rBV2	356	330	0.02%	0.004%
14	3.214	673	676	677	rBV2	402	174	0.01%	0.002%
15	3.339	713	715	718	rBV2	497	368	0.02%	0.004%
16	3.387	726	730	732	rBV2	237	188	0.01%	0.002%
17	3.532	770	775	780	rBV2	296	361	0.02%	0.004%
18	3.574	786	788	790	rBV3	326	137	0.01%	0.001%
19	3.648	807	811	815	rBV3	339	376	0.02%	0.004%
20	3.722	832	834	839	rBV2	180	134	0.01%	0.001%
21	3.805	859	860	864	rVB	302	123	0.01%	0.001%
22	3.825	864	866	868	rBV2	393	204	0.01%	0.002%
23	3.876	873	882	913	rBV	85905	236023	12.73%	2.526%
24	4.352	1015	1030	1057	rBV2	152282	396154	21.36%	4.240%
25	4.551	1090	1092	1097	rVB3	598	347	0.02%	0.004%
26	4.686	1133	1134	1136	rBV	326	142	0.01%	0.002%
27	4.744	1150	1152	1155	rBV2	336	161	0.01%	0.002%
28	4.812	1171	1173	1176	rVB2	509	227	0.01%	0.002%
29	4.883	1192	1195	1197	rBV	216	132	0.01%	0.001%
30	4.931	1204	1210	1215	rBV4	297	400	0.02%	0.004%
31	5.046	1229	1246	1276	rBV2	393887	1014308	54.70%	10.855%
32	5.272	1314	1316	1319	rBV	707	424	0.02%	0.005%
33	5.558	1403	1405	1409	rVB	325	203	0.01%	0.002%
34	5.619	1409	1424	1453	rBV	269817	555202	29.94%	5.942%
35	5.921	1506	1518	1538	rBV4	17156	39059	2.11%	0.418%
36	6.072	1550	1565	1594	rBV	229934	468409	25.26%	5.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022391.D
 Acq On : 29 Sep 2021 20:32
 Operator : SY/MD
 Sample : M3978-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.461	1683	1686	1687	rBV2	228	124	0.01%	0.001%
38	6.661	1746	1748	1750	rBV2	560	242	0.01%	0.003%
39	6.690	1755	1757	1761	rVB4	503	243	0.01%	0.003%
40	6.744	1772	1774	1778	rVB	417	167	0.01%	0.002%
41	6.773	1778	1783	1786	rVB3	514	362	0.02%	0.004%
42	6.792	1786	1789	1792	rBV	258	166	0.01%	0.002%
43	6.940	1833	1835	1839	rBV2	323	146	0.01%	0.002%
44	6.989	1839	1850	1872	rBV	114611	212151	11.44%	2.270%
45	7.143	1896	1898	1903	rVB3	832	485	0.03%	0.005%
46	7.194	1911	1914	1915	rBV3	408	251	0.01%	0.003%
47	7.316	1941	1952	1971	rBV	458775	796480	42.95%	8.524%
48	7.625	2038	2048	2066	rBV	80279	140538	7.58%	1.504%
49	7.818	2105	2108	2111	rBV2	228	194	0.01%	0.002%
50	7.895	2130	2132	2137	rVB4	415	266	0.01%	0.003%
51	7.927	2140	2142	2144	rBV2	410	259	0.01%	0.003%
52	7.976	2144	2157	2181	rBV	1094057	1854394	100.00%	19.845%
53	8.088	2183	2192	2222	rVV	275152	486835	26.25%	5.210%
54	8.619	2355	2357	2359	rBV	340	170	0.01%	0.002%
55	8.770	2401	2404	2410	rBV3	589	456	0.02%	0.005%
56	8.853	2419	2430	2456	rBV	408446	675569	36.43%	7.230%
57	9.101	2505	2507	2510	rBV3	405	209	0.01%	0.002%
58	9.210	2538	2541	2543	rBV2	363	236	0.01%	0.003%
59	9.236	2547	2549	2552	rBV2	192	140	0.01%	0.001%
60	9.252	2552	2554	2558	rBV3	483	219	0.01%	0.002%
61	9.284	2562	2564	2566	rBV2	260	148	0.01%	0.002%
62	9.310	2569	2572	2573	rBV	349	156	0.01%	0.002%
63	9.352	2583	2585	2588	rBV3	368	240	0.01%	0.003%
64	9.474	2620	2623	2625	rVV	352	157	0.01%	0.002%
65	9.516	2634	2636	2639	rBV	169	124	0.01%	0.001%
66	9.670	2682	2684	2691	rVB3	444	324	0.02%	0.003%
67	9.702	2691	2694	2695	rBV3	267	135	0.01%	0.001%
68	9.812	2726	2728	2731	rBV	218	121	0.01%	0.001%
69	9.837	2733	2736	2738	rBV2	367	265	0.01%	0.003%
70	9.879	2744	2749	2754	rVB2	369	392	0.02%	0.004%
71	10.127	2818	2826	2827	rBV4	1133	1253	0.07%	0.013%
72	10.178	2840	2842	2843	rBV	315	159	0.01%	0.002%
73	10.217	2843	2854	2873	rVV	348921	537167	28.97%	5.749%
74	10.313	2881	2884	2887	rBV2	724	467	0.03%	0.005%
75	10.397	2902	2910	2912	rBV5	912	1130	0.06%	0.012%
76	10.564	2958	2962	2963	rBV	524	314	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022391.D
 Acq On : 29 Sep 2021 20:32
 Operator : SY/MD
 Sample : M3978-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.596	2969	2972	2973	rBV	374	225	0.01%	0.002%
78	10.628	2980	2982	2987	rBV3	460	395	0.02%	0.004%
79	10.750	3018	3020	3022	rBV	369	155	0.01%	0.002%
80	10.921	3066	3073	3079	rBV4	1046	1528	0.08%	0.016%
81	11.040	3108	3110	3112	rBV4	242	161	0.01%	0.002%
82	11.098	3125	3128	3131	rBV2	299	203	0.01%	0.002%
83	11.149	3138	3144	3149	rVB3	573	674	0.04%	0.007%
84	11.175	3150	3152	3155	rBV	432	251	0.01%	0.003%
85	11.252	3164	3176	3196	rBV	366277	583936	31.49%	6.249%
86	11.625	3280	3292	3308	rBV	449427	724013	39.04%	7.748%
87	11.895	3373	3376	3379	rBV2	322	259	0.01%	0.003%
88	12.094	3434	3438	3445	rVB3	459	491	0.03%	0.005%
89	12.223	3475	3478	3481	rBV2	341	212	0.01%	0.002%
90	12.709	3625	3629	3632	rVB2	370	262	0.01%	0.003%
91	12.744	3637	3640	3642	rBV3	505	383	0.02%	0.004%
92	12.940	3699	3701	3704	rBV	345	215	0.01%	0.002%
93	13.059	3733	3738	3742	rBV3	508	513	0.03%	0.005%
94	13.329	3819	3822	3823	rBV	380	206	0.01%	0.002%
95	13.416	3844	3849	3853	rVB3	525	525	0.03%	0.006%
96	13.435	3853	3855	3857	rBV	364	186	0.01%	0.002%
97	13.448	3857	3859	3860	rBV	393	170	0.01%	0.002%
98	13.734	3946	3948	3951	rVB	428	176	0.01%	0.002%
99	13.821	3973	3975	3977	rBV	382	186	0.01%	0.002%
100	14.085	4054	4057	4059	rBV	226	135	0.01%	0.001%



Sum of corrected areas: 9344311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022391.D
Acq On : 29 Sep 2021 20:32
Operator : SY/MD
Sample : M3978-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

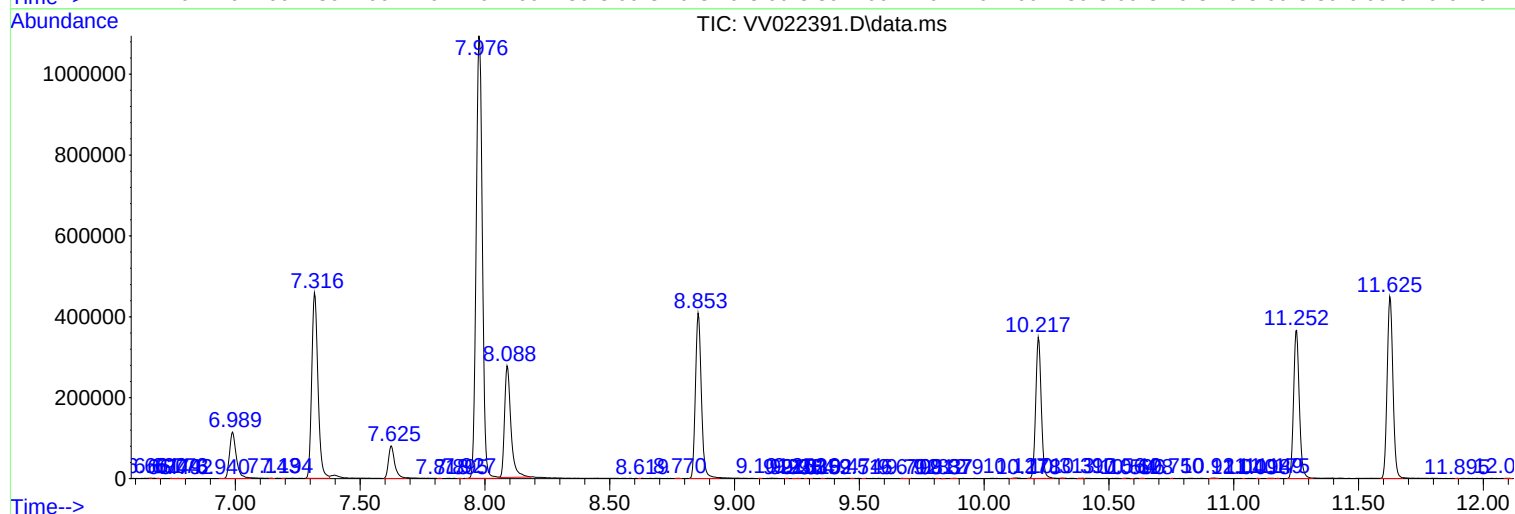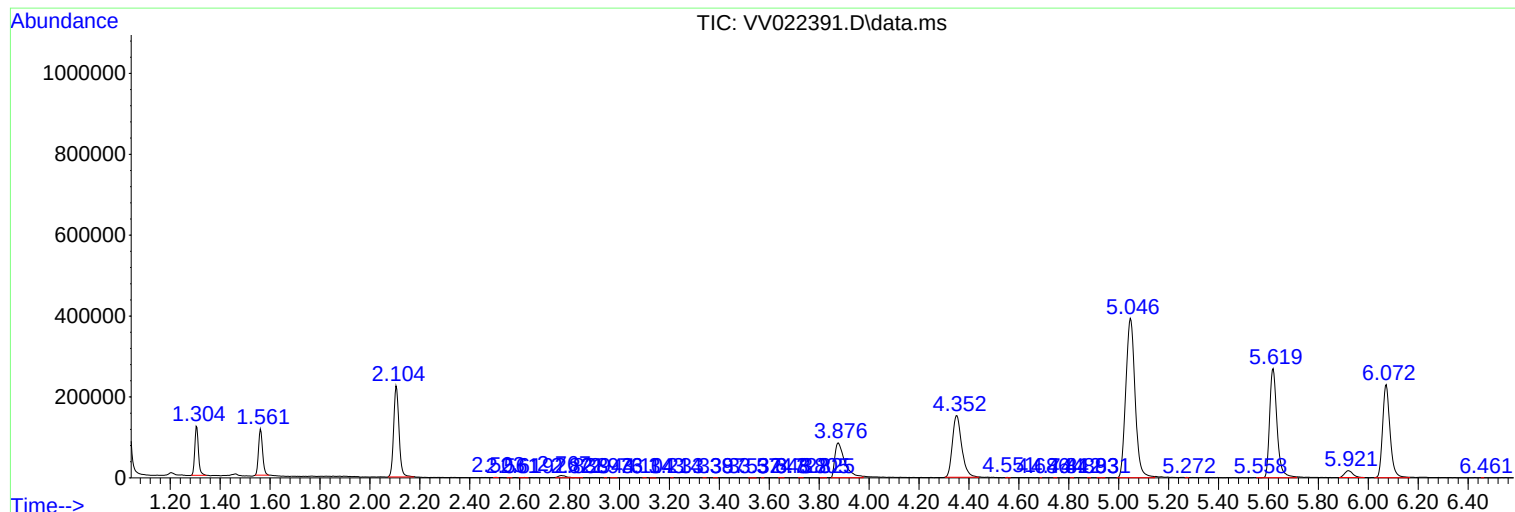

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022391.D
Acq On : 29 Sep 2021 20:32
Operator : SY/MD
Sample : M3978-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022391.D
Acq On : 29 Sep 2021 20:32
Operator : SY/MD
Sample : M3978-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------