

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022392.D
 Acq On : 29 Sep 2021 20:56
 Operator : SY/MD
 Sample : M3978-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	133444	133711	4.47%	1.252%
2	1.561	155	162	175	rBV	115675	135168	4.52%	1.266%
3	2.105	322	331	343	rBV	227181	328288	10.98%	3.075%
4	2.362	407	411	413	rBV	352	316	0.01%	0.003%
5	2.429	427	432	437	rBV4	812	962	0.03%	0.009%
6	2.625	486	493	494	rBV3	1326	1374	0.05%	0.013%
7	2.770	527	538	554	rVB2	9080	19266	0.64%	0.180%
8	2.873	565	570	573	rVB3	482	367	0.01%	0.003%
9	2.928	585	587	590	rBV	242	184	0.01%	0.002%
10	2.960	595	597	601	rBV2	286	180	0.01%	0.002%
11	3.043	621	623	625	rBV	366	195	0.01%	0.002%
12	3.166	657	661	664	rBV2	413	319	0.01%	0.003%
13	3.185	664	667	670	rBV2	195	154	0.01%	0.001%
14	3.240	682	684	689	rVB2	438	320	0.01%	0.003%
15	3.365	720	723	725	rBV2	306	185	0.01%	0.002%
16	3.481	755	759	764	rBV3	220	223	0.01%	0.002%
17	3.506	765	767	769	rVB3	338	149	0.00%	0.001%
18	3.619	797	802	804	rBV2	230	189	0.01%	0.002%
19	3.674	816	819	822	rVB	276	153	0.01%	0.001%
20	3.876	872	882	907	rBV	88178	241630	8.08%	2.263%
21	4.281	1005	1008	1012	rBV2	391	305	0.01%	0.003%
22	4.349	1012	1029	1062	rVV	156845	409530	13.70%	3.836%
23	4.674	1124	1130	1131	rBV	360	328	0.01%	0.003%
24	4.719	1141	1144	1146	rBV2	431	256	0.01%	0.002%
25	4.760	1154	1157	1161	rVV2	215	160	0.01%	0.001%
26	4.854	1184	1186	1188	rBV	469	290	0.01%	0.003%
27	4.895	1196	1199	1205	rVB3	303	201	0.01%	0.002%
28	4.982	1222	1226	1228	rBV	376	240	0.01%	0.002%
29	5.047	1228	1246	1279	rBV2	400400	1033467	34.57%	9.681%
30	5.265	1313	1314	1317	rBV	438	190	0.01%	0.002%
31	5.445	1367	1370	1373	rBV3	307	149	0.00%	0.001%
32	5.619	1412	1424	1456	rBV	280873	568487	19.02%	5.325%
33	5.921	1505	1518	1535	rBV5	22567	51296	1.72%	0.481%
34	6.011	1545	1546	1550	rVB2	380	185	0.01%	0.002%
35	6.072	1550	1565	1593	rBV	231582	478111	15.99%	4.479%
36	6.339	1645	1648	1649	rBV	414	222	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022392.D
 Acq On : 29 Sep 2021 20:56
 Operator : SY/MD
 Sample : M3978-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.381	1658	1661	1662	rBV	427	205	0.01%	0.002%
38	6.429	1674	1676	1679	rVV2	449	247	0.01%	0.002%
39	6.455	1682	1684	1688	rBV3	278	202	0.01%	0.002%
40	6.481	1688	1692	1695	rBV2	282	233	0.01%	0.002%
41	6.548	1710	1713	1717	rBV2	514	324	0.01%	0.003%
42	6.622	1732	1736	1739	rBV3	545	369	0.01%	0.003%
43	6.638	1739	1741	1743	rVV	398	217	0.01%	0.002%
44	6.677	1747	1753	1754	rBV4	520	447	0.01%	0.004%
45	6.792	1787	1789	1793	rVB2	313	163	0.01%	0.002%
46	6.812	1793	1795	1799	rBV2	296	220	0.01%	0.002%
47	6.902	1821	1823	1827	rVB2	370	193	0.01%	0.002%
48	6.989	1835	1850	1867	rBV	115470	213689	7.15%	2.002%
49	7.259	1929	1934	1936	rBV3	715	517	0.02%	0.005%
50	7.317	1940	1952	1972	rBV	464577	813358	27.21%	7.619%
51	7.583	2032	2035	2037	rBV2	369	263	0.01%	0.002%
52	7.622	2037	2047	2064	rBV	81307	140898	4.71%	1.320%
53	7.976	2139	2157	2182	rBV	1788368	2989250	100.00%	28.001%
54	8.088	2183	2192	2224	rVB	286154	505487	16.91%	4.735%
55	8.754	2397	2399	2402	rBV2	386	212	0.01%	0.002%
56	8.853	2418	2430	2449	rBV	423867	692818	23.18%	6.490%
57	9.008	2476	2478	2481	rVB4	755	346	0.01%	0.003%
58	9.043	2487	2489	2492	rBV2	469	335	0.01%	0.003%
59	9.152	2520	2523	2526	rVV2	933	796	0.03%	0.007%
60	9.198	2530	2537	2551	rVB5	4679	8216	0.27%	0.077%
61	9.275	2558	2561	2562	rBV	698	272	0.01%	0.003%
62	9.294	2562	2567	2569	rBV2	252	211	0.01%	0.002%
63	9.513	2630	2635	2636	rBV2	307	264	0.01%	0.002%
64	9.754	2707	2710	2716	rBV3	407	453	0.02%	0.004%
65	9.789	2719	2721	2724	rVV2	284	172	0.01%	0.002%
66	9.821	2728	2731	2734	rVB3	385	267	0.01%	0.003%
67	9.947	2764	2770	2773	rBV4	355	337	0.01%	0.003%
68	10.082	2809	2812	2814	rBV	400	277	0.01%	0.003%
69	10.133	2820	2828	2839	rBV4	2434	3949	0.13%	0.037%
70	10.217	2843	2854	2874	rVV	346567	544223	18.21%	5.098%
71	10.410	2912	2914	2917	rBV2	300	166	0.01%	0.002%
72	10.448	2923	2926	2930	rBV3	457	325	0.01%	0.003%
73	10.583	2966	2968	2974	rVB3	580	414	0.01%	0.004%
74	10.606	2974	2975	2978	rBV	357	176	0.01%	0.002%
75	10.876	3054	3059	3063	rBV2	419	387	0.01%	0.004%
76	10.918	3067	3072	3074	rBV3	1197	1165	0.04%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022392.D
 Acq On : 29 Sep 2021 20:56
 Operator : SY/MD
 Sample : M3978-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.021	3102	3104	3106	rBV	295	154	0.01%	0.001%
78	11.140	3139	3141	3145	rBV2	464	275	0.01%	0.003%
79	11.252	3164	3176	3202	rBV	377620	607682	20.33%	5.692%
80	11.625	3280	3292	3312	rBV	462929	732174	24.49%	6.858%
81	11.886	3369	3373	3375	rBV3	343	240	0.01%	0.002%
82	11.966	3395	3398	3400	rBV2	372	256	0.01%	0.002%
83	12.030	3416	3418	3421	rVB	351	193	0.01%	0.002%
84	12.053	3422	3425	3428	rBV3	292	174	0.01%	0.002%
85	12.358	3517	3520	3525	rBV3	372	253	0.01%	0.002%
86	12.422	3537	3540	3543	rBV	492	411	0.01%	0.004%
87	12.503	3562	3565	3566	rBV2	273	154	0.01%	0.001%
88	12.686	3616	3622	3624	rBV	394	315	0.01%	0.003%
89	12.718	3628	3632	3635	rVB2	409	275	0.01%	0.003%
90	12.738	3635	3638	3642	rBV	480	390	0.01%	0.004%
91	12.934	3693	3699	3701	rBV2	470	448	0.01%	0.004%
92	13.117	3754	3756	3762	rVB2	491	375	0.01%	0.004%
93	13.159	3765	3769	3770	rBV2	1294	900	0.03%	0.008%
94	13.255	3795	3799	3800	rBV2	439	325	0.01%	0.003%
95	13.458	3860	3862	3864	rVB2	408	172	0.01%	0.002%
96	13.593	3901	3904	3908	rBV	439	364	0.01%	0.003%
97	13.831	3975	3978	3979	rBV	361	165	0.01%	0.002%
98	13.921	4002	4006	4008	rBV2	719	501	0.02%	0.005%
99	14.069	4049	4052	4057	rVB3	489	373	0.01%	0.003%
100	14.361	4141	4143	4144	rBV3	407	162	0.01%	0.002%




Sum of corrected areas: 10675544

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022392.D
Acq On : 29 Sep 2021 20:56
Operator : SY/MD
Sample : M3978-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

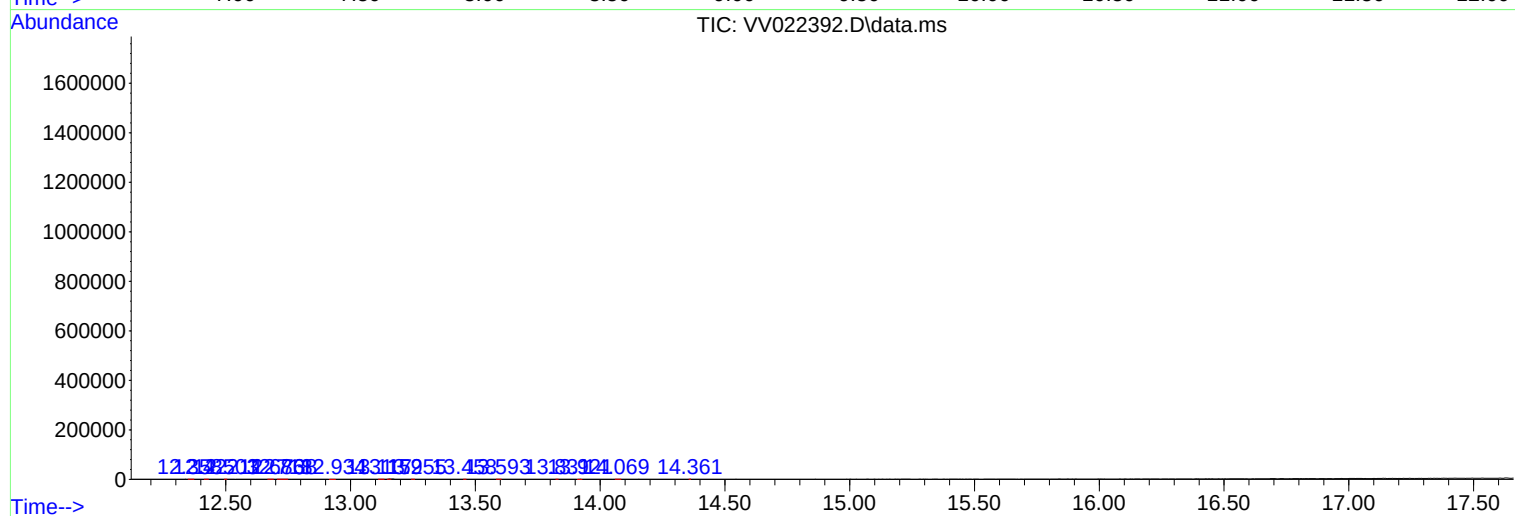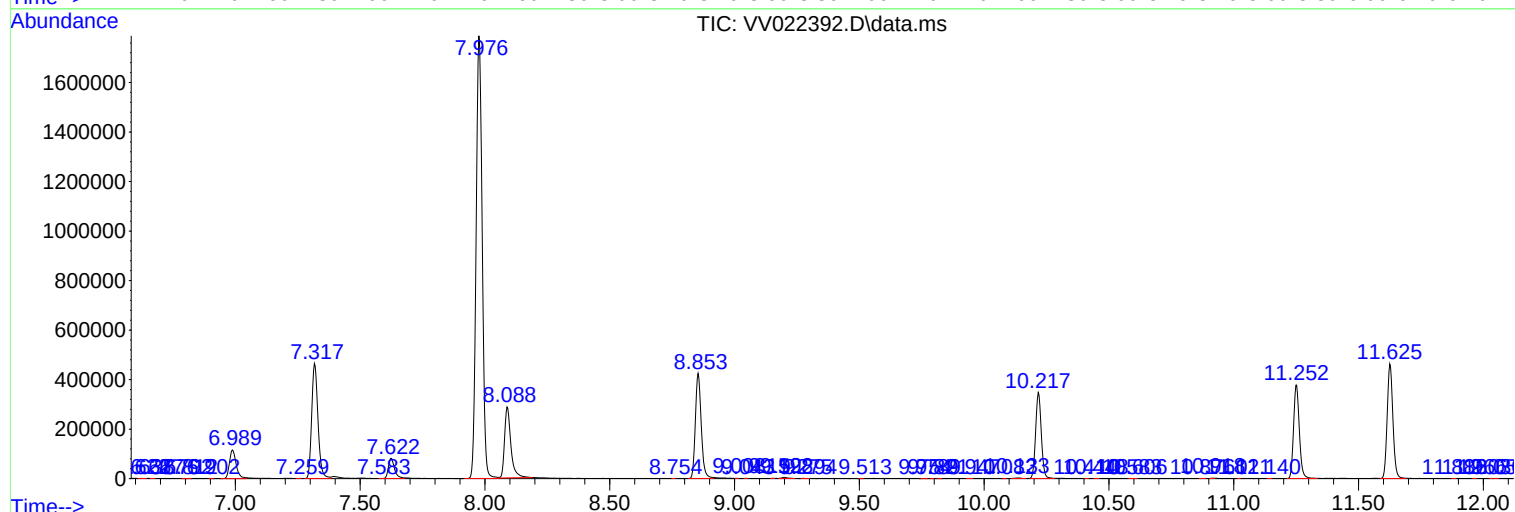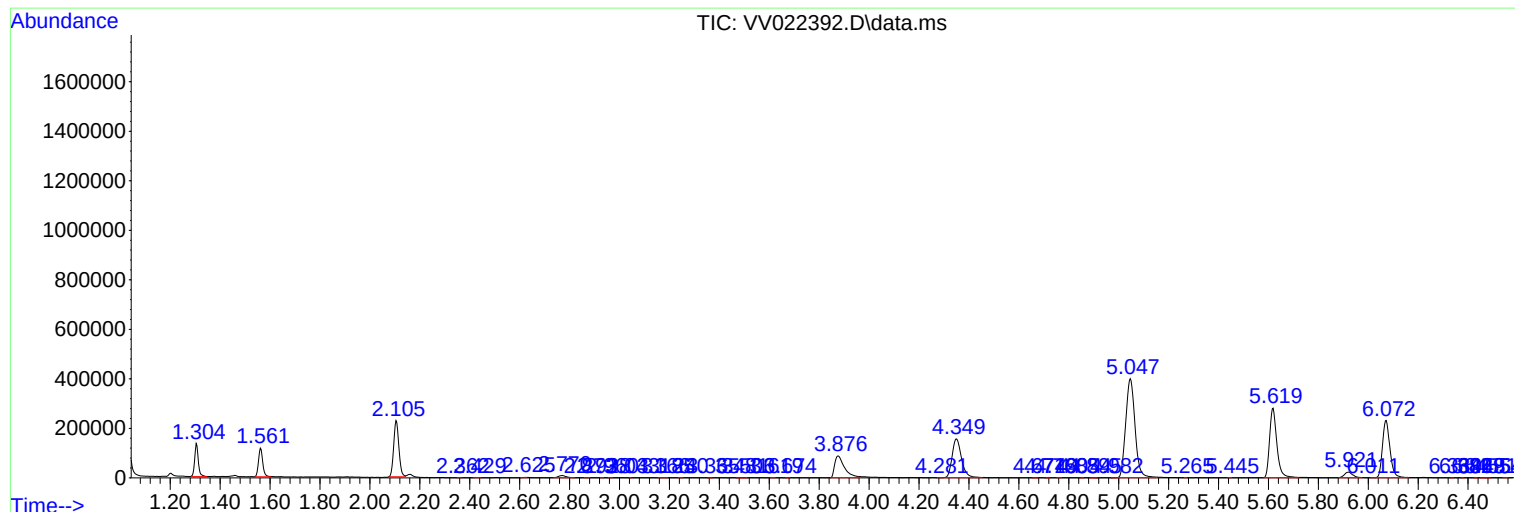

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022392.D
Acq On : 29 Sep 2021 20:56
Operator : SY/MD
Sample : M3978-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022392.D
Acq On : 29 Sep 2021 20:56
Operator : SY/MD
Sample : M3978-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc