

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022393.D
 Acq On : 29 Sep 2021 21:20
 Operator : SY/MD
 Sample : M3978-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	130990	129154	3.58%	1.150%
2	1.564	156	163	178	rVB	115527	129629	3.60%	1.154%
3	2.105	322	331	351	rBV	213670	312532	8.67%	2.783%
4	2.619	487	491	493	rBV2	271	215	0.01%	0.002%
5	2.693	511	514	518	rBV4	508	360	0.01%	0.003%
6	2.719	520	522	526	rVV2	746	481	0.01%	0.004%
7	2.770	527	538	553	rVV2	11378	24868	0.69%	0.221%
8	2.921	581	585	587	rBV2	300	238	0.01%	0.002%
9	3.011	609	613	615	rBV2	288	205	0.01%	0.002%
10	3.072	629	632	633	rBV	304	147	0.00%	0.001%
11	3.140	650	653	655	rBV2	243	191	0.01%	0.002%
12	3.198	670	671	675	rBV2	222	145	0.00%	0.001%
13	3.246	684	686	692	rVB2	279	240	0.01%	0.002%
14	3.404	730	735	740	rVB2	318	262	0.01%	0.002%
15	3.777	849	851	853	rBV	424	273	0.01%	0.002%
16	3.896	877	888	925	rBV	75584	252054	6.99%	2.245%
17	4.349	1013	1029	1051	rBV	157371	396311	10.99%	3.530%
18	4.551	1090	1092	1096	rBV2	491	274	0.01%	0.002%
19	4.651	1120	1123	1128	rVB2	530	403	0.01%	0.004%
20	4.677	1128	1131	1134	rBV2	530	351	0.01%	0.003%
21	4.732	1143	1148	1151	rBV3	434	416	0.01%	0.004%
22	4.770	1157	1160	1161	rBV	278	152	0.00%	0.001%
23	4.815	1171	1174	1177	rBV3	323	280	0.01%	0.002%
24	4.902	1199	1201	1203	rBV2	256	144	0.00%	0.001%
25	4.982	1224	1226	1229	rVB	233	146	0.00%	0.001%
26	5.047	1229	1246	1265	rBV2	392961	998441	27.70%	8.892%
27	5.429	1363	1365	1368	rBV3	353	183	0.01%	0.002%
28	5.474	1375	1379	1382	rBV2	184	137	0.00%	0.001%
29	5.490	1382	1384	1388	rBV2	269	231	0.01%	0.002%
30	5.542	1398	1400	1402	rBV	408	263	0.01%	0.002%
31	5.619	1411	1424	1440	rBV	272188	549542	15.25%	4.894%
32	5.918	1505	1517	1533	rBV2	32616	74691	2.07%	0.665%
33	6.024	1548	1550	1551	rBV	323	152	0.00%	0.001%
34	6.072	1551	1565	1594	rVV	225368	477727	13.25%	4.255%
35	6.375	1656	1659	1663	rVB2	562	363	0.01%	0.003%
36	6.436	1675	1678	1680	rBV3	422	284	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022393.D
 Acq On : 29 Sep 2021 21:20
 Operator : SY/MD
 Sample : M3978-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.474	1688	1690	1695	rBV3	388	291	0.01%	0.003%
38	6.577	1720	1722	1725	rBV	309	202	0.01%	0.002%
39	6.593	1725	1727	1730	rBV2	374	188	0.01%	0.002%
40	6.738	1767	1772	1773	rBV2	581	388	0.01%	0.003%
41	6.773	1779	1783	1784	rBV2	447	328	0.01%	0.003%
42	6.783	1784	1786	1788	rVV	497	200	0.01%	0.002%
43	6.847	1803	1806	1809	rVV	475	280	0.01%	0.002%
44	6.886	1815	1818	1822	rBV2	408	231	0.01%	0.002%
45	6.928	1828	1831	1833	rVV2	329	140	0.00%	0.001%
46	6.989	1839	1850	1875	rBV	112875	213838	5.93%	1.904%
47	7.246	1927	1930	1932	rVB	414	199	0.01%	0.002%
48	7.317	1941	1952	1974	rBV	452262	811853	22.52%	7.230%
49	7.622	2038	2047	2072	rBV	78427	144310	4.00%	1.285%
50	7.818	2106	2108	2110	rVB2	479	228	0.01%	0.002%
51	7.857	2118	2120	2125	rVB3	424	293	0.01%	0.003%
52	7.911	2132	2137	2140	rBV3	479	454	0.01%	0.004%
53	7.976	2143	2157	2183	rBV	2108754	3604499	100.00%	32.102%
54	8.092	2184	2193	2221	rVB	283363	514273	14.27%	4.580%
55	8.535	2329	2331	2334	rVB2	474	166	0.00%	0.001%
56	8.619	2355	2357	2361	rVB	425	141	0.00%	0.001%
57	8.699	2379	2382	2385	rBV2	443	344	0.01%	0.003%
58	8.854	2418	2430	2453	rBV	417024	697397	19.35%	6.211%
59	9.191	2533	2535	2539	rBV3	351	234	0.01%	0.002%
60	9.365	2585	2589	2594	rVB3	399	384	0.01%	0.003%
61	9.391	2595	2597	2601	rVB2	281	146	0.00%	0.001%
62	9.429	2604	2609	2610	rBV	291	199	0.01%	0.002%
63	9.648	2674	2677	2679	rBV2	180	153	0.00%	0.001%
64	9.677	2684	2686	2688	rBV	353	196	0.01%	0.002%
65	9.760	2709	2712	2714	rBV	343	218	0.01%	0.002%
66	9.809	2721	2727	2731	rBV2	373	466	0.01%	0.004%
67	9.841	2734	2737	2740	rVB	415	270	0.01%	0.002%
68	9.882	2747	2750	2751	rBV2	429	240	0.01%	0.002%
69	9.921	2759	2762	2763	rBV	296	141	0.00%	0.001%
70	10.050	2799	2802	2806	rVB2	280	202	0.01%	0.002%
71	10.127	2820	2826	2833	rBV5	1154	1702	0.05%	0.015%
72	10.217	2842	2854	2877	rBV	336249	534953	14.84%	4.764%
73	10.320	2884	2886	2887	rBV2	637	238	0.01%	0.002%
74	10.590	2965	2970	2971	rBV2	262	245	0.01%	0.002%
75	10.693	3000	3002	3006	rVB3	346	194	0.01%	0.002%
76	10.828	3042	3044	3051	rVB4	249	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022393.D
 Acq On : 29 Sep 2021 21:20
 Operator : SY/MD
 Sample : M3978-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.882	3056	3061	3064	rBV2	279	207	0.01%	0.002%
78	10.924	3067	3074	3078	rBV3	890	1073	0.03%	0.010%
79	11.252	3164	3176	3201	rBV	392417	609663	16.91%	5.430%
80	11.490	3245	3250	3251	rBV3	380	317	0.01%	0.003%
81	11.625	3280	3292	3310	rBV	461148	730571	20.27%	6.507%
82	11.789	3340	3343	3345	rBV3	439	214	0.01%	0.002%
83	12.268	3490	3492	3494	rBV2	331	176	0.00%	0.002%
84	12.374	3522	3525	3527	rBV2	280	150	0.00%	0.001%
85	12.493	3557	3562	3564	rVB3	208	164	0.00%	0.001%
86	12.506	3564	3566	3569	rBV	306	179	0.00%	0.002%
87	12.570	3584	3586	3590	rBV2	377	297	0.01%	0.003%
88	12.686	3620	3622	3627	rBV2	278	192	0.01%	0.002%
89	12.847	3669	3672	3674	rBV2	289	193	0.01%	0.002%
90	12.892	3684	3686	3689	rVB	578	263	0.01%	0.002%
91	12.988	3714	3716	3719	rBV2	288	137	0.00%	0.001%
92	13.152	3764	3767	3769	rBV2	324	214	0.01%	0.002%
93	13.217	3784	3787	3793	rBV2	261	254	0.01%	0.002%
94	13.538	3882	3887	3889	rBV3	460	380	0.01%	0.003%
95	13.664	3924	3926	3932	rBV2	316	201	0.01%	0.002%
96	13.927	4006	4008	4011	rBV	426	236	0.01%	0.002%
97	14.107	4062	4064	4067	rBV	397	287	0.01%	0.003%
98	14.172	4082	4084	4090	rVB	534	315	0.01%	0.003%
99	14.204	4090	4094	4095	rBV	419	214	0.01%	0.002%
100	14.310	4126	4127	4131	rBV2	392	287	0.01%	0.003%




Sum of corrected areas: 11228282

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022393.D
Acq On : 29 Sep 2021 21:20
Operator : SY/MD
Sample : M3978-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

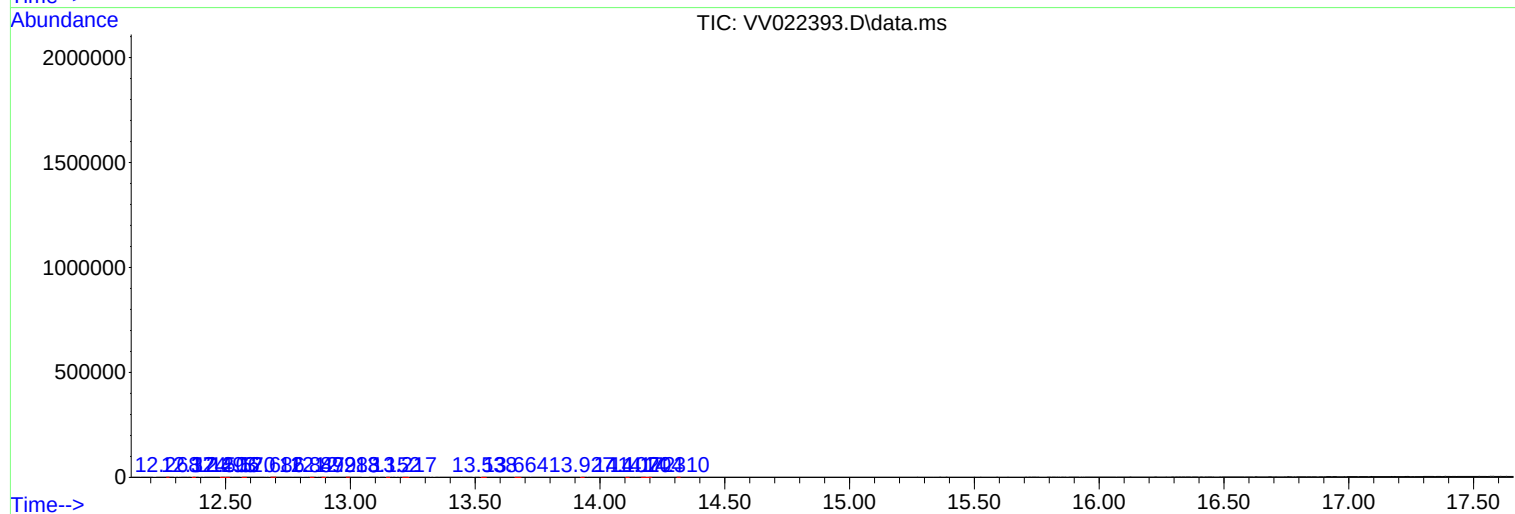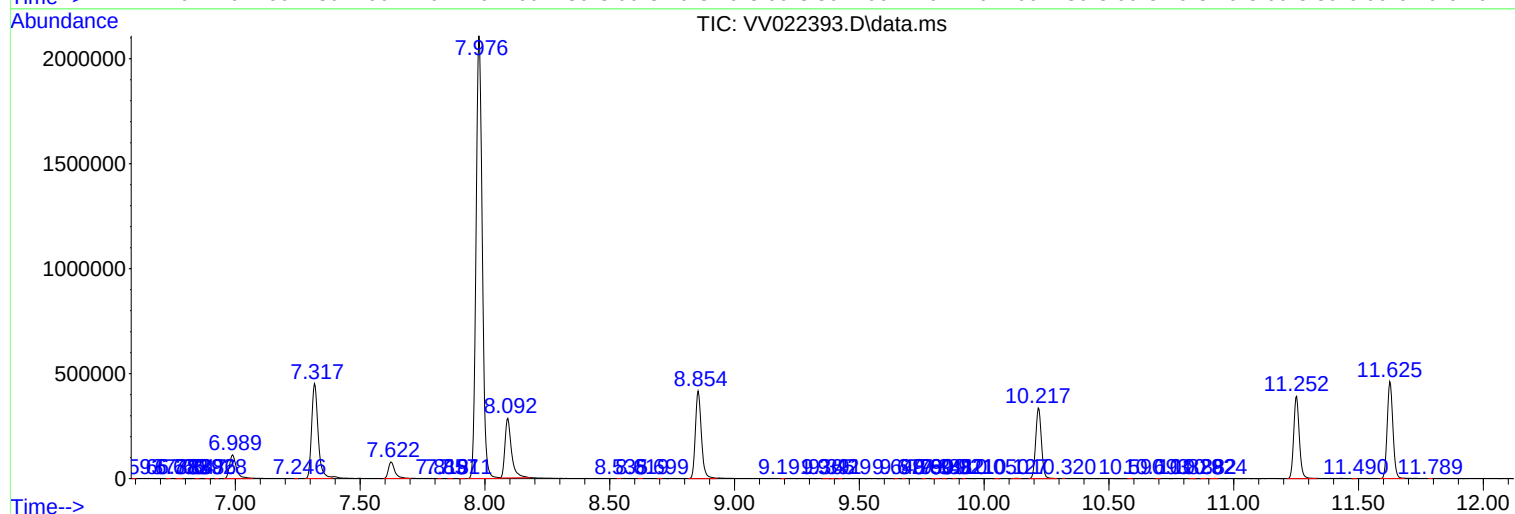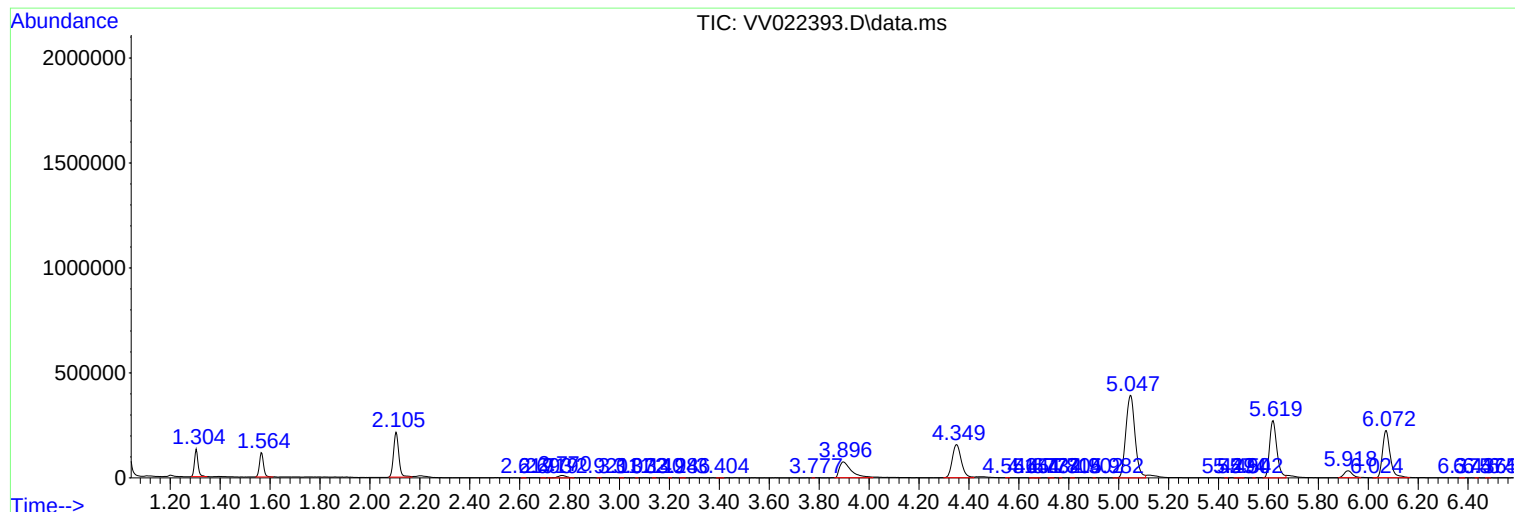

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022393.D
Acq On : 29 Sep 2021 21:20
Operator : SY/MD
Sample : M3978-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022393.D
Acq On : 29 Sep 2021 21:20
Operator : SY/MD
Sample : M3978-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
