

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022394.D
 Acq On : 29 Sep 2021 21:44
 Operator : SY/MD
 Sample : M3978-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	127070	126029	12.52%	1.532%
2	1.564	156	163	177	rBV	115194	129081	12.82%	1.569%
3	2.105	321	331	353	rBV	215847	320350	31.82%	3.895%
4	2.571	474	476	481	rVB3	646	342	0.03%	0.004%
5	2.613	486	489	494	rVB3	675	500	0.05%	0.006%
6	2.725	521	524	525	rBV	352	142	0.01%	0.002%
7	2.908	578	581	583	rBV2	252	187	0.02%	0.002%
8	3.008	608	612	616	rBV2	174	131	0.01%	0.002%
9	3.027	616	618	621	rBV2	241	169	0.02%	0.002%
10	3.079	630	634	638	rBV2	233	243	0.02%	0.003%
11	3.111	642	644	650	rVV3	368	245	0.02%	0.003%
12	3.150	654	656	658	rBV3	363	133	0.01%	0.002%
13	3.252	685	688	690	rBV2	332	211	0.02%	0.003%
14	3.391	729	731	736	rVB	358	225	0.02%	0.003%
15	3.423	739	741	745	rVB2	259	131	0.01%	0.002%
16	3.452	748	750	753	rBV	356	208	0.02%	0.003%
17	3.545	777	779	782	rVB2	382	177	0.02%	0.002%
18	3.645	808	810	814	rBV2	270	217	0.02%	0.003%
19	3.661	814	815	819	rVB	319	138	0.01%	0.002%
20	3.741	837	840	842	rVB2	217	122	0.01%	0.001%
21	3.854	872	875	878	rBV3	225	184	0.02%	0.002%
22	3.899	878	889	931	rBV	72701	258235	25.65%	3.139%
23	4.349	1014	1029	1052	rBV	160724	393736	39.11%	4.787%
24	4.625	1113	1115	1117	rVV3	708	308	0.03%	0.004%
25	4.654	1120	1124	1125	rBV2	440	257	0.03%	0.003%
26	5.047	1229	1246	1267	rBV2	399389	1006677	100.00%	12.238%
27	5.423	1362	1363	1365	rVB	400	144	0.01%	0.002%
28	5.519	1391	1393	1394	rBV	380	137	0.01%	0.002%
29	5.558	1402	1405	1409	rVB4	366	313	0.03%	0.004%
30	5.619	1411	1424	1458	rBV	279996	584776	58.09%	7.109%
31	5.818	1484	1486	1489	rVB3	596	290	0.03%	0.004%
32	5.918	1505	1517	1540	rBV7	23498	54049	5.37%	0.657%
33	6.069	1552	1564	1600	rBV	223739	475632	47.25%	5.782%
34	6.281	1627	1630	1634	rBV	309	272	0.03%	0.003%
35	6.378	1657	1660	1663	rBV2	348	278	0.03%	0.003%
36	6.397	1663	1666	1669	rVB3	455	269	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022394.D
 Acq On : 29 Sep 2021 21:44
 Operator : SY/MD
 Sample : M3978-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.439	1675	1679	1681	rBV2	326	301	0.03%	0.004%
38	6.497	1694	1697	1704	rBV2	279	279	0.03%	0.003%
39	6.529	1704	1707	1711	rBV3	353	248	0.02%	0.003%
40	6.603	1726	1730	1736	rVB2	510	537	0.05%	0.007%
41	6.690	1755	1757	1759	rBV	290	162	0.02%	0.002%
42	6.924	1827	1830	1835	rVB2	214	137	0.01%	0.002%
43	6.989	1839	1850	1877	rBV	115047	214773	21.33%	2.611%
44	7.169	1905	1906	1907	rBV	422	150	0.01%	0.002%
45	7.317	1939	1952	1971	rBV	448201	802949	79.76%	9.762%
46	7.622	2037	2047	2066	rBV	77983	141483	14.05%	1.720%
47	7.838	2112	2114	2116	rBV	367	195	0.02%	0.002%
48	7.915	2135	2138	2139	rBV	337	152	0.02%	0.002%
49	7.931	2139	2143	2144	rBV	378	301	0.03%	0.004%
50	7.976	2144	2157	2183	rVV	365885	633866	62.97%	7.706%
51	8.092	2183	2193	2224	rBV	273888	507468	50.41%	6.169%
52	8.471	2307	2311	2313	rBV3	426	316	0.03%	0.004%
53	8.574	2340	2343	2344	rBV2	444	243	0.02%	0.003%
54	8.664	2368	2371	2375	rVB2	460	315	0.03%	0.004%
55	8.693	2376	2380	2381	rBV2	229	122	0.01%	0.001%
56	8.792	2408	2411	2415	rBV3	292	255	0.03%	0.003%
57	8.854	2418	2430	2457	rBV	421397	703290	69.86%	8.550%
58	9.050	2489	2491	2493	rBV2	495	240	0.02%	0.003%
59	9.307	2570	2571	2576	rVB2	505	271	0.03%	0.003%
60	9.339	2576	2581	2583	rBV2	463	283	0.03%	0.003%
61	9.374	2589	2592	2593	rBV2	282	150	0.01%	0.002%
62	9.493	2625	2629	2632	rBV2	217	195	0.02%	0.002%
63	9.603	2660	2663	2667	rVB2	243	141	0.01%	0.002%
64	9.622	2667	2669	2671	rBV	250	119	0.01%	0.001%
65	9.741	2704	2706	2710	rBV3	469	336	0.03%	0.004%
66	9.792	2719	2722	2724	rBV2	346	179	0.02%	0.002%
67	9.802	2724	2725	2728	rVV	444	163	0.02%	0.002%
68	9.882	2747	2750	2752	rBV	335	185	0.02%	0.002%
69	9.911	2754	2759	2760	rBV2	372	275	0.03%	0.003%
70	9.972	2771	2778	2781	rBV2	595	653	0.06%	0.008%
71	10.024	2791	2794	2796	rBV2	301	180	0.02%	0.002%
72	10.066	2803	2807	2809	rBV2	236	204	0.02%	0.002%
73	10.124	2819	2825	2827	rBV3	1134	1040	0.10%	0.013%
74	10.153	2832	2834	2835	rBV	325	128	0.01%	0.002%
75	10.217	2842	2854	2876	rBV	334200	531758	52.82%	6.465%
76	10.352	2894	2896	2899	rBV2	297	220	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022394.D
 Acq On : 29 Sep 2021 21:44
 Operator : SY/MD
 Sample : M3978-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.368	2899	2901	2904	rVV3	611	358	0.04%	0.004%
78	10.490	2937	2939	2941	rBV	230	140	0.01%	0.002%
79	10.587	2967	2969	2972	rVB4	407	129	0.01%	0.002%
80	10.908	3066	3069	3070	rBV	609	352	0.03%	0.004%
81	11.037	3107	3109	3112	rVB2	362	145	0.01%	0.002%
82	11.075	3119	3121	3124	rVB2	432	216	0.02%	0.003%
83	11.143	3137	3142	3144	rBV3	901	754	0.07%	0.009%
84	11.169	3147	3150	3152	rBV2	244	176	0.02%	0.002%
85	11.249	3163	3175	3197	rBV	391239	606455	60.24%	7.373%
86	11.487	3247	3249	3251	rBV	230	130	0.01%	0.002%
87	11.525	3260	3261	3263	rVB	405	156	0.02%	0.002%
88	11.625	3278	3292	3312	rBV	451493	713924	70.92%	8.679%
89	11.815	3349	3351	3356	rVB2	455	257	0.03%	0.003%
90	11.960	3394	3396	3399	rBV	352	233	0.02%	0.003%
91	12.056	3423	3426	3430	rVB3	400	293	0.03%	0.004%
92	12.079	3431	3433	3436	rBV2	316	176	0.02%	0.002%
93	12.297	3499	3501	3506	rBV3	369	273	0.03%	0.003%
94	12.535	3572	3575	3581	rBV2	465	408	0.04%	0.005%
95	12.689	3620	3623	3626	rBV2	488	387	0.04%	0.005%
96	13.223	3787	3789	3792	rVB	428	189	0.02%	0.002%
97	13.271	3798	3804	3808	rBV2	489	625	0.06%	0.008%
98	13.342	3823	3826	3829	rBV2	256	213	0.02%	0.003%
99	14.606	4216	4219	4225	rBV2	542	515	0.05%	0.006%
100	15.014	4344	4346	4349	rBV2	446	240	0.02%	0.003%




Sum of corrected areas: 8225544

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022394.D
Acq On : 29 Sep 2021 21:44
Operator : SY/MD
Sample : M3978-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

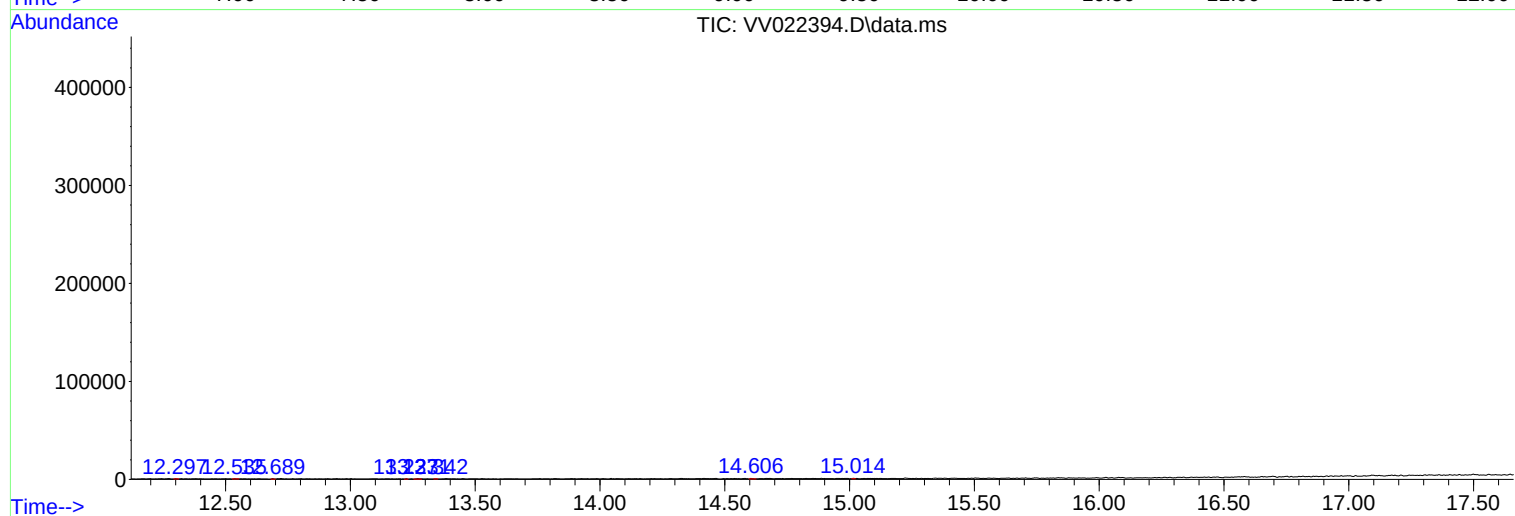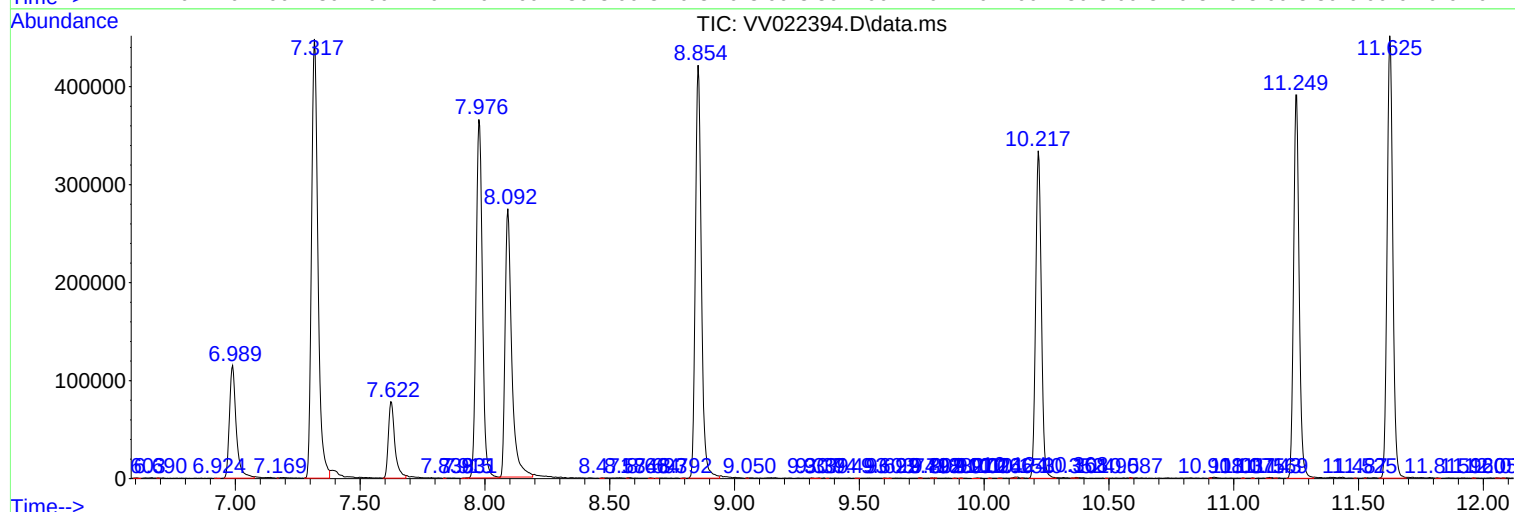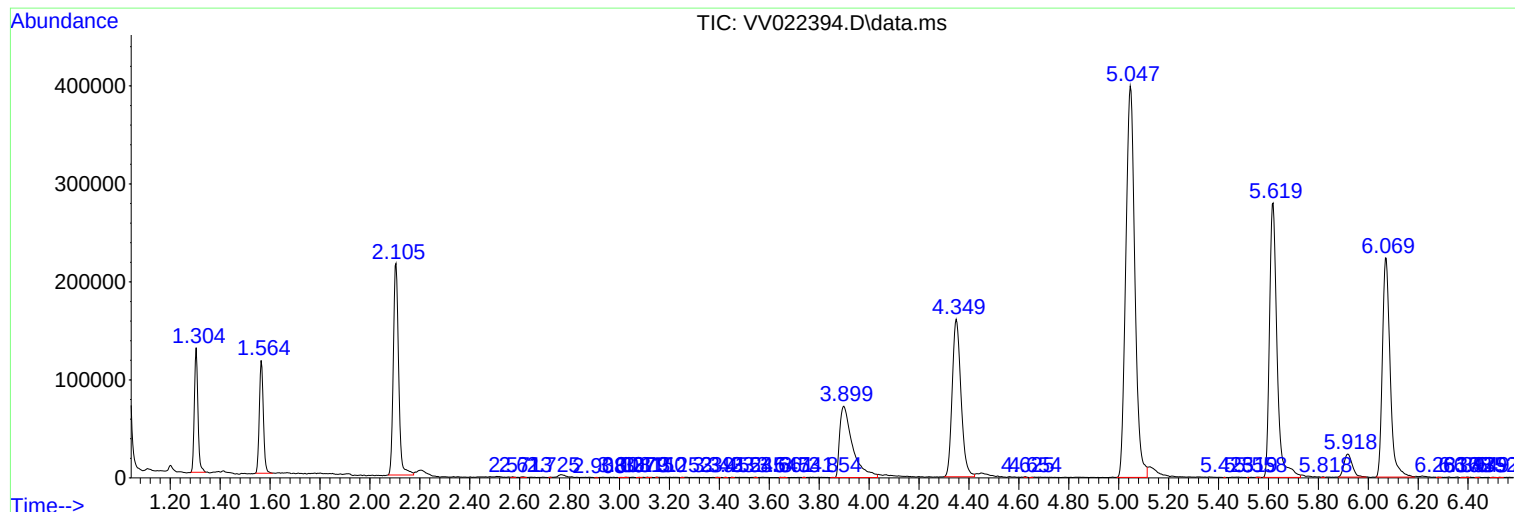

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022394.D
Acq On : 29 Sep 2021 21:44
Operator : SY/MD
Sample : M3978-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022394.D
Acq On : 29 Sep 2021 21:44
Operator : SY/MD
Sample : M3978-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------