

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022396.D
 Acq On : 29 Sep 2021 22:56
 Operator : SY/MD
 Sample : VV0929WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	142588	149639	13.74%	1.895%
2	1.564	156	163	174	rBV	127974	143586	13.19%	1.818%
3	2.105	321	331	348	rBV	248526	359719	33.04%	4.555%
4	2.600	482	485	488	rBV3	321	173	0.02%	0.002%
5	2.667	504	506	509	rVB3	239	134	0.01%	0.002%
6	2.683	509	511	512	rBV	279	132	0.01%	0.002%
7	2.712	518	520	525	rBV3	280	302	0.03%	0.004%
8	2.883	571	573	575	rBV2	307	130	0.01%	0.002%
9	2.912	580	582	587	rBV3	434	266	0.02%	0.003%
10	3.056	623	627	630	rBV3	339	288	0.03%	0.004%
11	3.137	650	652	655	rBV	418	210	0.02%	0.003%
12	3.227	677	680	685	rBV2	425	265	0.02%	0.003%
13	3.426	739	742	744	rBV	247	150	0.01%	0.002%
14	3.571	782	787	795	rBV4	441	652	0.06%	0.008%
15	3.709	828	830	833	rVB2	360	174	0.02%	0.002%
16	3.728	833	836	838	rBV	241	126	0.01%	0.002%
17	3.754	840	844	845	rBV2	370	237	0.02%	0.003%
18	3.796	854	857	860	rBV4	277	190	0.02%	0.002%
19	3.831	865	868	870	rBV	229	169	0.02%	0.002%
20	3.905	879	891	936	rBV	70753	272248	25.01%	3.448%
21	4.349	1014	1029	1053	rBV2	170466	423011	38.85%	5.357%
22	4.645	1117	1121	1125	rBV4	637	613	0.06%	0.008%
23	4.876	1192	1193	1195	rBV	335	129	0.01%	0.002%
24	5.047	1229	1246	1280	rBV2	425910	1088693	100.00%	13.787%
25	5.500	1384	1387	1390	rBV2	331	215	0.02%	0.003%
26	5.529	1394	1396	1403	rVB5	653	432	0.04%	0.005%
27	5.574	1407	1410	1411	rBV	235	151	0.01%	0.002%
28	5.619	1412	1424	1451	rBV	274887	563940	51.80%	7.142%
29	5.908	1504	1514	1531	rBV3	7910	17735	1.63%	0.225%
30	6.014	1545	1547	1549	rBV	298	144	0.01%	0.002%
31	6.069	1550	1564	1592	rVV	239883	500900	46.01%	6.343%
32	6.281	1628	1630	1633	rBV2	357	157	0.01%	0.002%
33	6.522	1702	1705	1710	rBV3	565	465	0.04%	0.006%
34	6.545	1710	1712	1714	rVB2	448	150	0.01%	0.002%
35	6.590	1721	1726	1727	rBV3	315	246	0.02%	0.003%
36	6.622	1734	1736	1738	rBV2	277	135	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022396.D
 Acq On : 29 Sep 2021 22:56
 Operator : SY/MD
 Sample : VV0929WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.635	1738	1740	1744	rBV	574	428	0.04%	0.005%
38	6.712	1761	1764	1768	rVB2	464	319	0.03%	0.004%
39	6.870	1809	1813	1822	rBV2	381	535	0.05%	0.007%
40	6.908	1822	1825	1827	rBV2	176	136	0.01%	0.002%
41	6.928	1829	1831	1834	rBV	254	150	0.01%	0.002%
42	6.989	1838	1850	1873	rBV	117332	219697	20.18%	2.782%
43	7.194	1911	1914	1916	rBV3	890	536	0.05%	0.007%
44	7.317	1939	1952	1971	rBV	491028	851541	78.22%	10.784%
45	7.622	2036	2047	2066	rBV	81352	148698	13.66%	1.883%
46	7.828	2107	2111	2114	rBV3	315	281	0.03%	0.004%
47	7.921	2136	2140	2142	rBV2	512	418	0.04%	0.005%
48	7.982	2152	2159	2169	rBV7	3588	6201	0.57%	0.079%
49	8.092	2183	2193	2226	rBV	295762	549406	50.46%	6.957%
50	8.606	2350	2353	2358	rBV5	618	605	0.06%	0.008%
51	8.712	2383	2386	2393	rBV2	438	454	0.04%	0.006%
52	8.764	2400	2402	2405	rBV	287	163	0.01%	0.002%
53	8.802	2412	2414	2417	rBV2	326	204	0.02%	0.003%
54	8.854	2419	2430	2455	rBV	411721	682985	62.73%	8.649%
55	9.149	2519	2522	2523	rBV	566	251	0.02%	0.003%
56	9.310	2568	2572	2574	rBV2	337	312	0.03%	0.004%
57	9.413	2601	2604	2608	rBV2	174	158	0.01%	0.002%
58	9.458	2613	2618	2619	rBV	358	226	0.02%	0.003%
59	9.577	2653	2655	2657	rBV	202	136	0.01%	0.002%
60	9.648	2675	2677	2683	rVB2	403	339	0.03%	0.004%
61	9.677	2683	2686	2688	rBV2	247	144	0.01%	0.002%
62	9.741	2703	2706	2712	rVB3	427	351	0.03%	0.004%
63	9.786	2718	2720	2722	rBV	410	178	0.02%	0.002%
64	9.969	2775	2777	2779	rBV2	285	139	0.01%	0.002%
65	10.040	2795	2799	2802	rVB2	441	304	0.03%	0.004%
66	10.066	2805	2807	2811	rVB2	275	128	0.01%	0.002%
67	10.095	2812	2816	2819	rBV3	280	237	0.02%	0.003%
68	10.127	2819	2826	2835	rBV3	1280	1538	0.14%	0.019%
69	10.217	2843	2854	2876	rBV	346132	545907	50.14%	6.913%
70	10.381	2903	2905	2907	rBV2	381	173	0.02%	0.002%
71	10.577	2962	2966	2969	rBV4	529	422	0.04%	0.005%
72	10.657	2988	2991	2995	rVB2	563	308	0.03%	0.004%
73	10.780	3026	3029	3031	rBV	233	173	0.02%	0.002%
74	10.799	3032	3035	3036	rBV	242	140	0.01%	0.002%
75	10.876	3055	3059	3063	rBV2	312	275	0.03%	0.003%
76	11.114	3130	3133	3135	rBV2	384	228	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022396.D
 Acq On : 29 Sep 2021 22:56
 Operator : SY/MD
 Sample : VV0929WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.194	3154	3158	3160	rBV3	413	325	0.03%	0.004%
78	11.249	3164	3175	3195	rBV	380668	592345	54.41%	7.501%
79	11.426	3226	3230	3236	rBV5	1219	1261	0.12%	0.016%
80	11.519	3254	3259	3260	rBV2	385	166	0.02%	0.002%
81	11.535	3260	3264	3267	rBV3	345	371	0.03%	0.005%
82	11.625	3280	3292	3311	rBV	484436	756503	69.49%	9.580%
83	11.818	3349	3352	3353	rBV	277	141	0.01%	0.002%
84	11.873	3367	3369	3372	rBV	316	166	0.02%	0.002%
85	12.098	3436	3439	3441	rBV2	387	241	0.02%	0.003%
86	12.191	3467	3468	3471	rBV	253	143	0.01%	0.002%
87	12.249	3483	3486	3487	rBV	354	191	0.02%	0.002%
88	12.355	3516	3519	3521	rBV2	299	232	0.02%	0.003%
89	12.419	3536	3539	3543	rVB3	503	333	0.03%	0.004%
90	12.468	3551	3554	3556	rBV2	357	234	0.02%	0.003%
91	12.548	3576	3579	3581	rBV	317	201	0.02%	0.003%
92	12.654	3610	3612	3617	rVB3	778	523	0.05%	0.007%
93	12.738	3636	3638	3642	rBV2	375	207	0.02%	0.003%
94	13.271	3802	3804	3808	rVB3	939	653	0.06%	0.008%
95	13.294	3808	3811	3814	rBV2	429	255	0.02%	0.003%
96	13.445	3855	3858	3861	rBV2	397	228	0.02%	0.003%
97	13.509	3876	3878	3881	rBV3	548	390	0.04%	0.005%
98	13.596	3900	3905	3906	rBV2	440	378	0.03%	0.005%
99	13.869	3987	3990	3993	rBV2	339	274	0.03%	0.003%
100	14.371	4144	4146	4148	rBV2	286	141	0.01%	0.002%




Sum of corrected areas: 7896632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022396.D
Acq On : 29 Sep 2021 22:56
Operator : SY/MD
Sample : VV0929WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

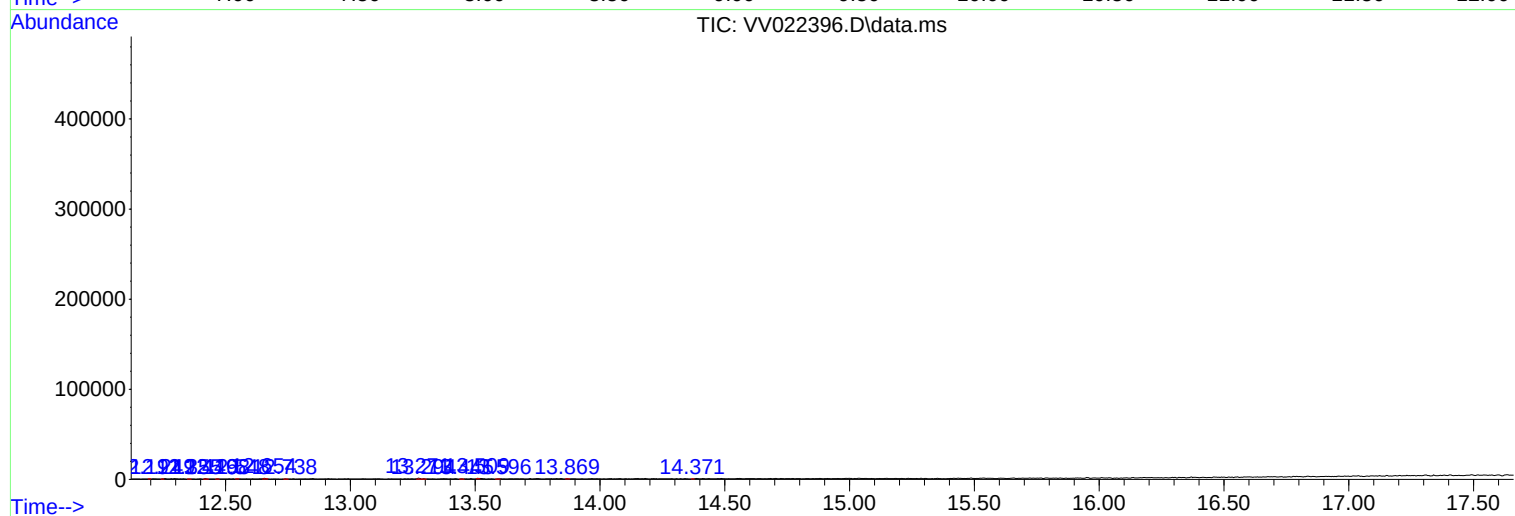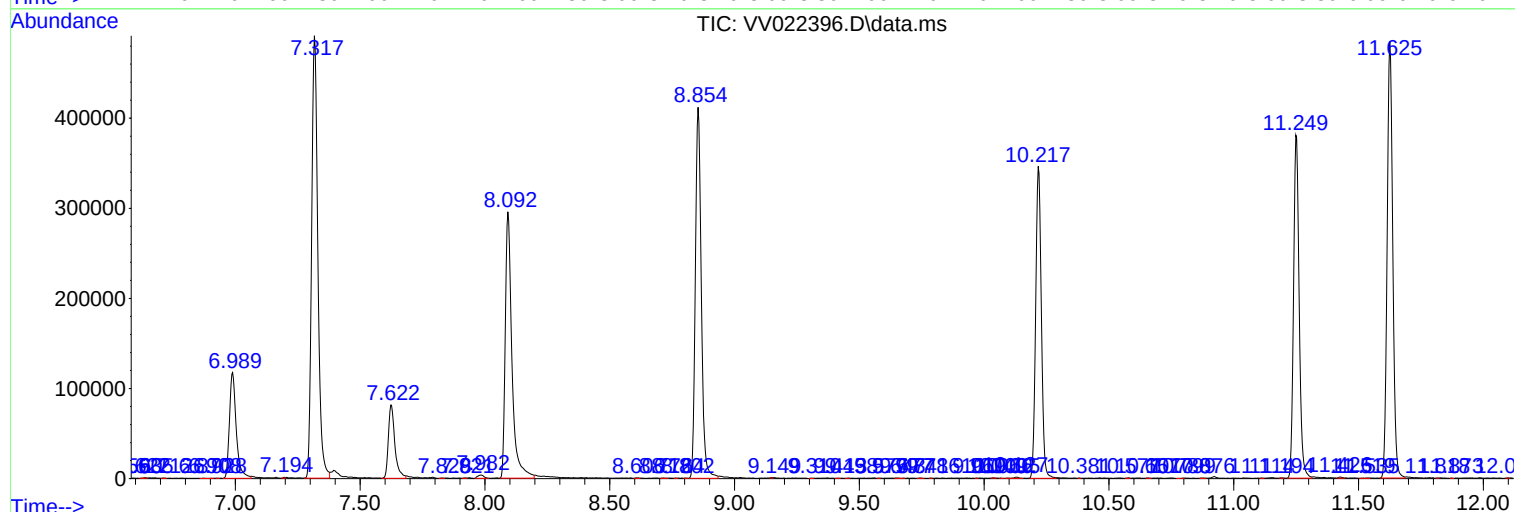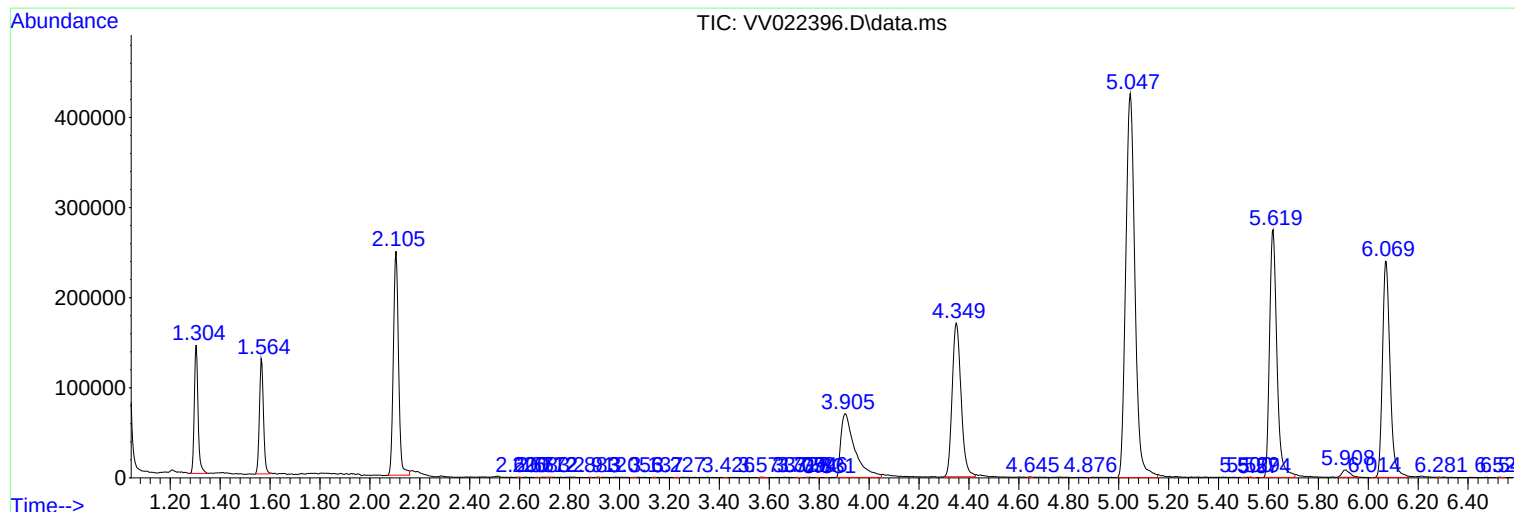

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022396.D
Acq On : 29 Sep 2021 22:56
Operator : SY/MD
Sample : VV0929WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022396.D
Acq On : 29 Sep 2021 22:56
Operator : SY/MD
Sample : VV0929WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
