

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022398.D
 Acq On : 29 Sep 2021 23:44
 Operator : SY/MD
 Sample : M3979-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	121900	124868	5.06%	1.254%
2	1.561	156	162	176	rVB	112166	128433	5.20%	1.290%
3	2.104	322	331	345	rVB	217127	314930	12.76%	3.162%
4	2.722	518	523	525	rBV3	532	383	0.02%	0.004%
5	2.767	525	537	554	rVV3	21315	43226	1.75%	0.434%
6	2.889	573	575	578	rVB	497	246	0.01%	0.002%
7	3.072	628	632	635	rBV3	307	213	0.01%	0.002%
8	3.178	661	665	669	rBV3	286	298	0.01%	0.003%
9	3.246	683	686	692	rVV2	409	413	0.02%	0.004%
10	3.310	704	706	708	rVV2	351	185	0.01%	0.002%
11	3.336	712	714	720	rBV3	496	360	0.01%	0.004%
12	3.516	765	770	773	rVB2	455	377	0.02%	0.004%
13	3.661	813	815	818	rVB3	309	185	0.01%	0.002%
14	3.690	821	824	827	rVV2	370	251	0.01%	0.003%
15	3.796	855	857	860	rVB2	308	190	0.01%	0.002%
16	3.873	870	881	919	rBV	85191	247627	10.03%	2.486%
17	4.349	1013	1029	1065	rBV	154808	402330	16.30%	4.040%
18	4.747	1150	1153	1155	rBV	269	193	0.01%	0.002%
19	4.809	1169	1172	1175	rBV2	570	408	0.02%	0.004%
20	4.825	1175	1177	1180	rBV	414	196	0.01%	0.002%
21	4.850	1183	1185	1188	rVB2	463	255	0.01%	0.003%
22	4.966	1220	1221	1225	rVB2	368	175	0.01%	0.002%
23	5.046	1229	1246	1283	rBV2	385999	1009108	40.88%	10.132%
24	5.378	1347	1349	1354	rBV3	392	262	0.01%	0.003%
25	5.413	1357	1360	1362	rBV	342	213	0.01%	0.002%
26	5.471	1375	1378	1382	rVB3	412	294	0.01%	0.003%
27	5.493	1382	1385	1387	rBV2	667	348	0.01%	0.003%
28	5.619	1412	1424	1447	rBV	267679	548232	22.21%	5.505%
29	5.921	1506	1518	1540	rBV4	30499	67320	2.73%	0.676%
30	6.072	1550	1565	1590	rBV	223763	461932	18.71%	4.638%
31	6.268	1624	1626	1630	rBV2	427	221	0.01%	0.002%
32	6.313	1637	1640	1643	rBV4	559	406	0.02%	0.004%
33	6.378	1656	1660	1663	rBV3	451	361	0.01%	0.004%
34	6.442	1674	1680	1681	rBV3	334	278	0.01%	0.003%
35	6.468	1686	1688	1696	rVB2	266	276	0.01%	0.003%
36	6.516	1698	1703	1704	rBV2	281	181	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022398.D
 Acq On : 29 Sep 2021 23:44
 Operator : SY/MD
 Sample : M3979-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.580	1716	1723	1725	rBV5	659	598	0.02%	0.006%
38	6.622	1733	1736	1739	rBV2	444	305	0.01%	0.003%
39	6.641	1739	1742	1746	rVV2	523	523	0.02%	0.005%
40	6.673	1750	1752	1755	rVB3	480	197	0.01%	0.002%
41	6.706	1758	1762	1764	rVB3	449	272	0.01%	0.003%
42	6.747	1773	1775	1779	rBV2	391	201	0.01%	0.002%
43	6.821	1794	1798	1800	rBV2	356	256	0.01%	0.003%
44	6.989	1839	1850	1870	rBV	110631	205570	8.33%	2.064%
45	7.259	1931	1934	1937	rBV2	478	349	0.01%	0.004%
46	7.316	1940	1952	1972	rBV	448985	791043	32.04%	7.943%
47	7.622	2038	2047	2067	rBV2	76182	137599	5.57%	1.382%
48	7.834	2110	2113	2116	rBV3	491	292	0.01%	0.003%
49	7.873	2120	2125	2131	rBV5	446	605	0.02%	0.006%
50	7.911	2131	2137	2143	rBV4	356	387	0.02%	0.004%
51	7.976	2143	2157	2183	rBV	1488033	2468612	100.00%	24.787%
52	8.088	2183	2192	2225	rVB	264543	470159	19.05%	4.721%
53	8.368	2277	2279	2280	rBV	416	178	0.01%	0.002%
54	8.509	2321	2323	2325	rBV2	315	174	0.01%	0.002%
55	8.754	2395	2399	2401	rBV3	383	336	0.01%	0.003%
56	8.853	2419	2430	2456	rBV	415480	677737	27.45%	6.805%
57	9.062	2493	2495	2499	rBV3	473	357	0.01%	0.004%
58	9.152	2518	2523	2527	rBV3	580	772	0.03%	0.008%
59	9.214	2539	2542	2544	rBV3	457	280	0.01%	0.003%
60	9.313	2568	2573	2574	rBV2	317	208	0.01%	0.002%
61	9.397	2597	2599	2602	rBV2	326	219	0.01%	0.002%
62	9.477	2621	2624	2626	rVB3	427	218	0.01%	0.002%
63	9.500	2626	2631	2632	rBV3	285	199	0.01%	0.002%
64	9.558	2646	2649	2653	rVB2	421	260	0.01%	0.003%
65	9.628	2667	2671	2676	rVB3	253	193	0.01%	0.002%
66	9.705	2692	2695	2699	rBV3	274	235	0.01%	0.002%
67	9.728	2699	2702	2704	rBV	314	203	0.01%	0.002%
68	9.738	2704	2705	2709	rVB2	488	178	0.01%	0.002%
69	9.799	2720	2724	2726	rVV2	239	197	0.01%	0.002%
70	10.011	2782	2790	2799	rBV5	2091	3871	0.16%	0.039%
71	10.066	2805	2807	2811	rVB3	694	428	0.02%	0.004%
72	10.130	2822	2827	2832	rVB6	1205	1394	0.06%	0.014%
73	10.217	2843	2854	2878	rBV	334454	530469	21.49%	5.326%
74	10.355	2894	2897	2898	rBV2	358	221	0.01%	0.002%
75	10.419	2914	2917	2921	rVB3	363	246	0.01%	0.002%
76	10.651	2986	2989	2991	rBV2	262	179	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022398.D
 Acq On : 29 Sep 2021 23:44
 Operator : SY/MD
 Sample : M3979-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.760	3019	3023	3025	rBV2	277	208	0.01%	0.002%
78	10.789	3028	3032	3034	rBV	356	258	0.01%	0.003%
79	10.921	3067	3073	3082	rVV6	1146	1766	0.07%	0.018%
80	11.143	3140	3142	3145	rVV2	356	206	0.01%	0.002%
81	11.252	3164	3176	3200	rBV	372954	584997	23.70%	5.874%
82	11.545	3264	3267	3270	rBV2	713	599	0.02%	0.006%
83	11.625	3280	3292	3315	rBV	449502	715707	28.99%	7.186%
84	11.773	3334	3338	3342	rBV2	424	399	0.02%	0.004%
85	11.985	3402	3404	3407	rVB	450	232	0.01%	0.002%
86	12.175	3460	3463	3465	rBV3	420	276	0.01%	0.003%
87	12.348	3515	3517	3520	rBV3	291	216	0.01%	0.002%
88	12.474	3554	3556	3561	rVB3	279	201	0.01%	0.002%
89	12.596	3590	3594	3596	rBV2	315	273	0.01%	0.003%
90	12.754	3639	3643	3645	rBV	263	193	0.01%	0.002%
91	12.802	3655	3658	3660	rBV2	266	217	0.01%	0.002%
92	12.905	3688	3690	3693	rBV	359	202	0.01%	0.002%
93	13.017	3721	3725	3730	rBV3	416	552	0.02%	0.006%
94	13.062	3734	3739	3741	rBV3	305	306	0.01%	0.003%
95	13.339	3821	3825	3829	rBV2	361	295	0.01%	0.003%
96	13.451	3858	3860	3864	rBV	293	211	0.01%	0.002%
97	13.676	3926	3930	3933	rBV2	493	328	0.01%	0.003%
98	13.747	3950	3952	3954	rBV	537	236	0.01%	0.002%
99	14.033	4038	4041	4043	rBV2	397	213	0.01%	0.002%
100	14.165	4080	4082	4088	rVB4	352	305	0.01%	0.003%




Sum of corrected areas: 9959290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022398.D
Acq On : 29 Sep 2021 23:44
Operator : SY/MD
Sample : M3979-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

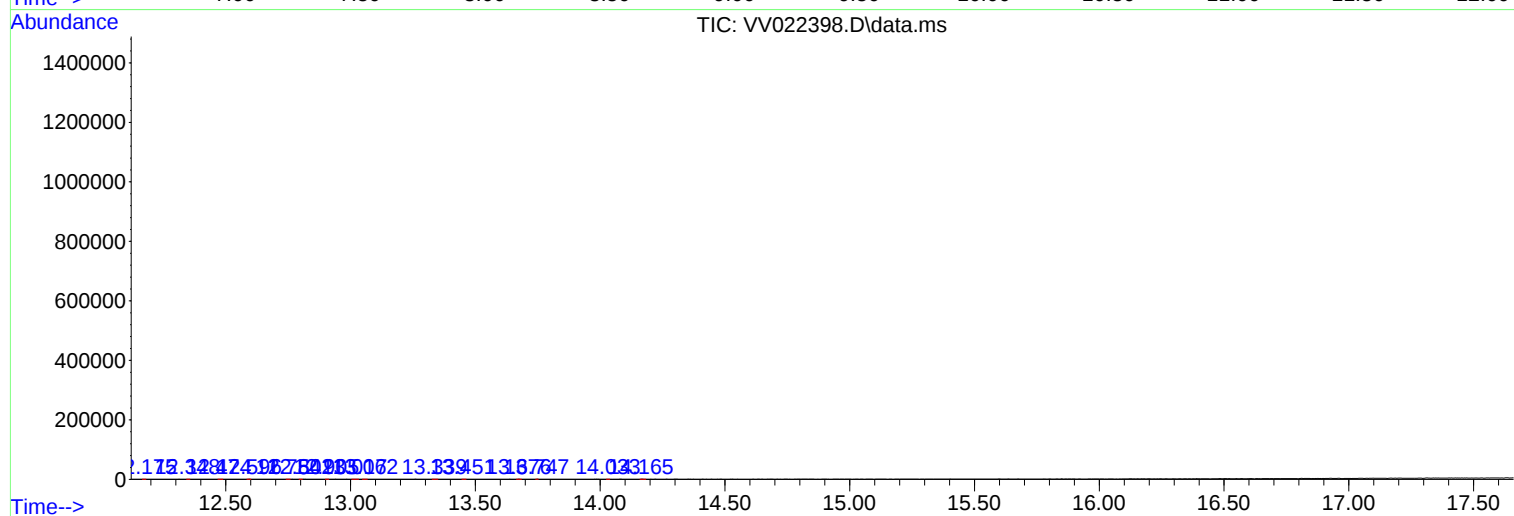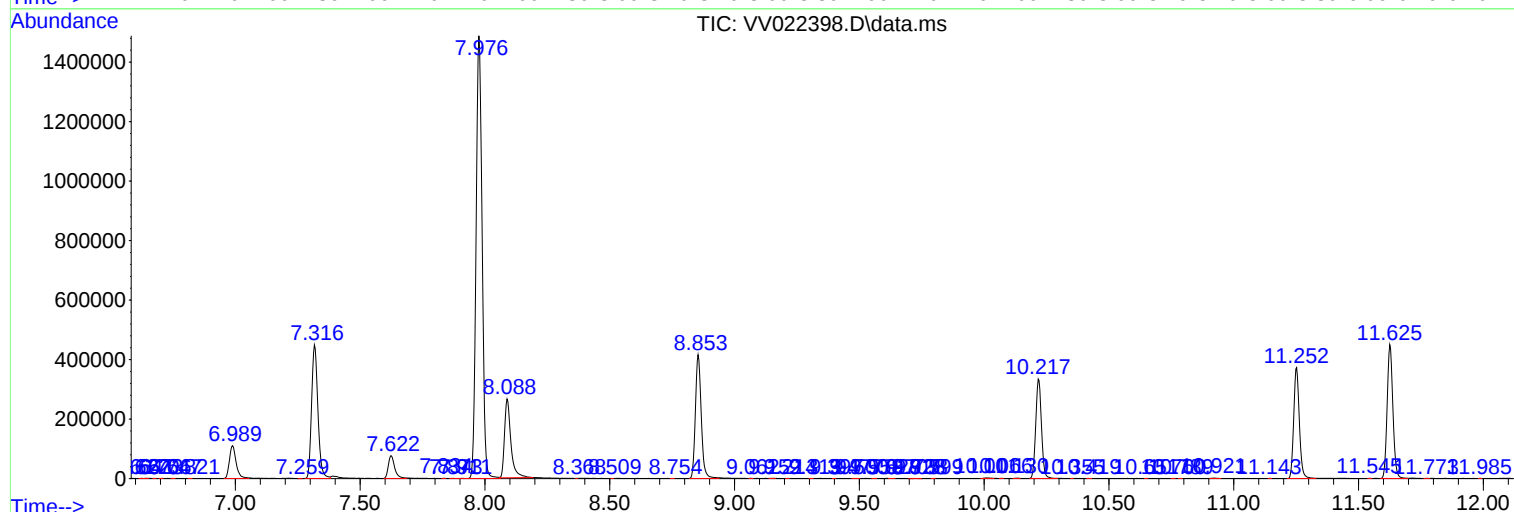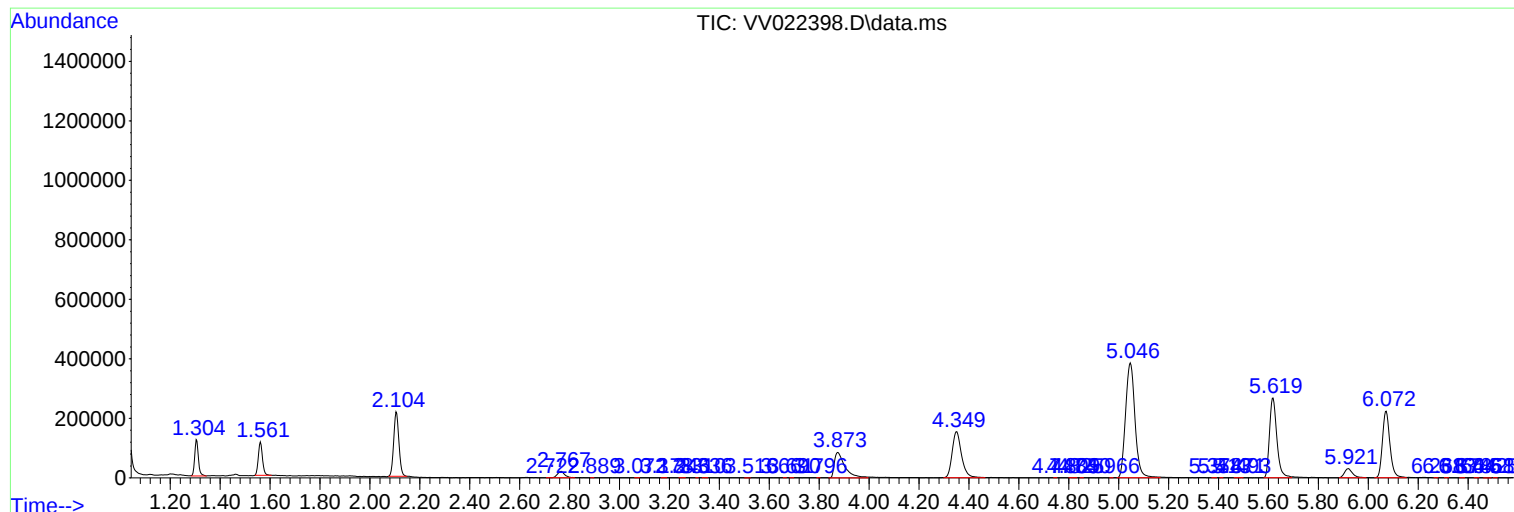

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022398.D
Acq On : 29 Sep 2021 23:44
Operator : SY/MD
Sample : M3979-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022398.D
Acq On : 29 Sep 2021 23:44
Operator : SY/MD
Sample : M3979-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
