

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022399.D
 Acq On : 30 Sep 2021 00:08
 Operator : SY/MD
 Sample : M3979-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	118389	120935	4.55%	1.185%
2	1.565	157	163	177	rVB	111714	126056	4.75%	1.235%
3	2.105	322	331	343	rBV	210285	296987	11.18%	2.910%
4	2.394	419	421	423	rBV2	533	302	0.01%	0.003%
5	2.458	439	441	443	rBV	529	274	0.01%	0.003%
6	2.545	465	468	470	rBV2	399	307	0.01%	0.003%
7	2.767	527	537	554	rVB5	11574	25188	0.95%	0.247%
8	2.892	574	576	580	rVB	341	259	0.01%	0.003%
9	2.918	582	584	587	rVB2	335	126	0.00%	0.001%
10	2.941	587	591	593	rBV2	396	365	0.01%	0.004%
11	3.053	624	626	631	rVB2	536	223	0.01%	0.002%
12	3.230	679	681	683	rBV2	163	89	0.00%	0.001%
13	3.400	733	734	736	rBV	230	101	0.00%	0.001%
14	3.420	736	740	743	rVV3	341	291	0.01%	0.003%
15	3.455	746	751	754	rBV2	454	300	0.01%	0.003%
16	3.513	766	769	773	rVB4	429	278	0.01%	0.003%
17	3.699	825	827	830	rBV2	160	92	0.00%	0.001%
18	3.732	834	837	839	rVB2	428	219	0.01%	0.002%
19	3.902	878	890	936	rBV	72801	287023	10.81%	2.813%
20	4.349	1014	1029	1051	rBV	158119	388972	14.64%	3.812%
21	4.613	1109	1111	1113	rBV2	310	123	0.00%	0.001%
22	4.651	1121	1123	1125	rBV	393	163	0.01%	0.002%
23	4.706	1137	1140	1141	rBV2	259	141	0.01%	0.001%
24	4.789	1164	1166	1169	rBV2	407	201	0.01%	0.002%
25	4.812	1171	1173	1175	rBV	397	220	0.01%	0.002%
26	4.905	1198	1202	1203	rBV	253	152	0.01%	0.001%
27	5.047	1230	1246	1268	rBV2	385179	990137	37.27%	9.703%
28	5.314	1328	1329	1330	rBV2	340	107	0.00%	0.001%
29	5.436	1365	1367	1371	rVB2	583	306	0.01%	0.003%
30	5.461	1374	1375	1378	rBV	228	98	0.00%	0.001%
31	5.523	1389	1394	1395	rBV3	189	190	0.01%	0.002%
32	5.571	1407	1409	1411	rBV	332	142	0.01%	0.001%
33	5.619	1411	1424	1458	rBV	275248	576150	21.69%	5.646%
34	5.918	1504	1517	1537	rBV4	30946	71497	2.69%	0.701%
35	6.014	1545	1547	1548	rBV	239	86	0.00%	0.001%
36	6.072	1550	1565	1593	rBV	221854	465028	17.51%	4.557%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022399.D
 Acq On : 30 Sep 2021 00:08
 Operator : SY/MD
 Sample : M3979-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.391	1660	1664	1669	rVV4	400	366	0.01%	0.004%
38	6.413	1669	1671	1673	rVB	297	115	0.00%	0.001%
39	6.445	1679	1681	1684	rVV2	415	138	0.01%	0.001%
40	6.494	1694	1696	1700	rBV2	238	143	0.01%	0.001%
41	6.513	1700	1702	1703	rBV2	315	102	0.00%	0.001%
42	6.786	1785	1787	1790	rBV2	328	212	0.01%	0.002%
43	6.799	1790	1791	1793	rVV2	292	103	0.00%	0.001%
44	6.831	1798	1801	1802	rBV	245	133	0.01%	0.001%
45	6.918	1825	1828	1833	rVB3	359	270	0.01%	0.003%
46	6.989	1839	1850	1873	rBV2	107761	205313	7.73%	2.012%
47	7.317	1940	1952	1972	rBV	442826	789712	29.73%	7.739%
48	7.577	2029	2033	2034	rBV	459	339	0.01%	0.003%
49	7.625	2038	2048	2072	rVV	73205	136458	5.14%	1.337%
50	7.821	2107	2109	2113	rVB2	323	146	0.01%	0.001%
51	7.844	2113	2116	2118	rBV2	466	309	0.01%	0.003%
52	7.924	2138	2141	2143	rBV	335	222	0.01%	0.002%
53	7.976	2143	2157	2183	rBV	1556556	2656341	100.00%	26.032%
54	8.092	2184	2193	2224	rVB	277233	513699	19.34%	5.034%
55	8.555	2335	2337	2338	rBV	271	100	0.00%	0.001%
56	8.629	2359	2360	2365	rBV3	242	178	0.01%	0.002%
57	8.680	2374	2376	2377	rBV3	259	107	0.00%	0.001%
58	8.809	2414	2416	2417	rBV3	309	94	0.00%	0.001%
59	8.854	2418	2430	2450	rBV	410528	691769	26.04%	6.779%
60	9.146	2519	2521	2524	rBV4	686	538	0.02%	0.005%
61	9.333	2577	2579	2582	rBV2	280	148	0.01%	0.001%
62	9.487	2620	2627	2630	rBV2	411	447	0.02%	0.004%
63	9.522	2637	2638	2640	rBV2	400	142	0.01%	0.001%
64	9.596	2659	2661	2663	rBV	298	110	0.00%	0.001%
65	9.764	2710	2713	2717	rVB2	392	317	0.01%	0.003%
66	9.786	2717	2720	2723	rBV2	292	211	0.01%	0.002%
67	9.989	2780	2783	2784	rBV	225	106	0.00%	0.001%
68	10.008	2785	2789	2792	rBV4	915	846	0.03%	0.008%
69	10.066	2805	2807	2812	rVB	379	229	0.01%	0.002%
70	10.127	2822	2826	2830	rBV5	1023	1057	0.04%	0.010%
71	10.217	2842	2854	2879	rBV	336990	528062	19.88%	5.175%
72	10.490	2936	2939	2944	rBV3	407	412	0.02%	0.004%
73	10.538	2952	2954	2955	rBV	290	118	0.00%	0.001%
74	10.661	2990	2992	2995	rVB3	503	244	0.01%	0.002%
75	10.686	2998	3000	3003	rVV	192	112	0.00%	0.001%
76	10.706	3003	3006	3010	rVB2	397	339	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022399.D
 Acq On : 30 Sep 2021 00:08
 Operator : SY/MD
 Sample : M3979-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.744	3015	3018	3021	rBV3	345	259	0.01%	0.003%
78	10.789	3028	3032	3036	rBV3	370	376	0.01%	0.004%
79	10.818	3039	3041	3045	rVB2	437	170	0.01%	0.002%
80	10.837	3045	3047	3048	rBV2	289	142	0.01%	0.001%
81	10.921	3070	3073	3080	rVB3	1557	1388	0.05%	0.014%
82	10.966	3085	3087	3090	rBV2	184	113	0.00%	0.001%
83	11.037	3106	3109	3111	rBV3	378	223	0.01%	0.002%
84	11.111	3130	3132	3134	rBV	252	108	0.00%	0.001%
85	11.136	3138	3140	3142	rVV2	316	115	0.00%	0.001%
86	11.194	3156	3158	3162	rBB2	294	108	0.00%	0.001%
87	11.252	3165	3176	3199	rVV	382691	603561	22.72%	5.915%
88	11.577	3274	3277	3279	rVB2	669	376	0.01%	0.004%
89	11.625	3279	3292	3311	rBV	452061	712135	26.81%	6.979%
90	11.853	3361	3363	3366	rVB2	509	160	0.01%	0.002%
91	11.895	3374	3376	3378	rBV2	379	211	0.01%	0.002%
92	11.947	3389	3392	3394	rBV2	293	143	0.01%	0.001%
93	12.066	3427	3429	3431	rBV	290	188	0.01%	0.002%
94	12.644	3606	3609	3611	rBV	367	265	0.01%	0.003%
95	12.873	3679	3680	3683	rBV	230	116	0.00%	0.001%
96	13.551	3889	3891	3894	rVB	334	159	0.01%	0.002%
97	13.866	3987	3989	3991	rBV	402	205	0.01%	0.002%
98	14.014	4033	4035	4036	rBV	352	151	0.01%	0.001%
99	14.056	4046	4048	4053	rBV2	306	203	0.01%	0.002%
100	14.085	4054	4057	4059	rBV	375	270	0.01%	0.003%




Sum of corrected areas: 10204080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022399.D
Acq On : 30 Sep 2021 00:08
Operator : SY/MD
Sample : M3979-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

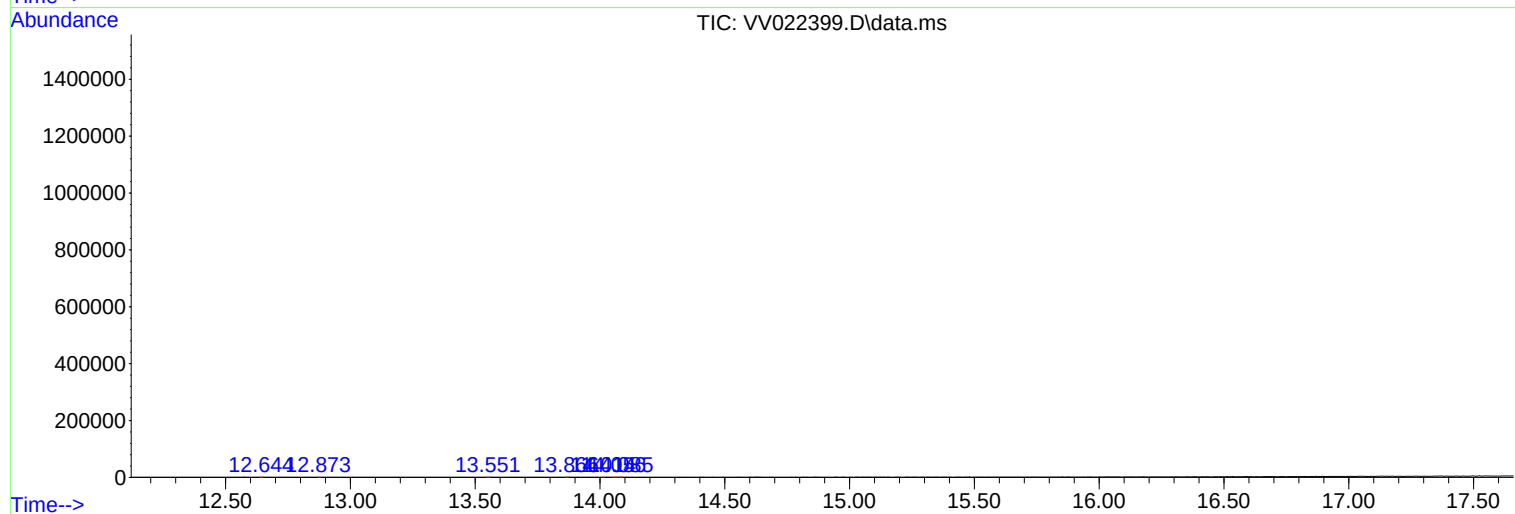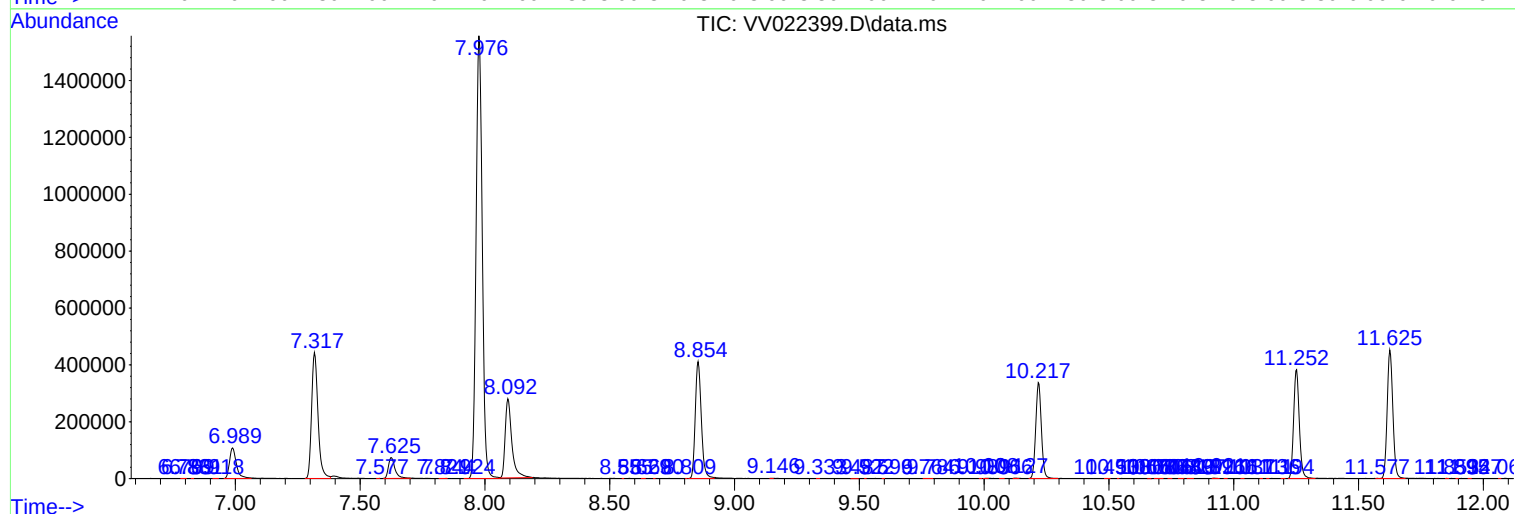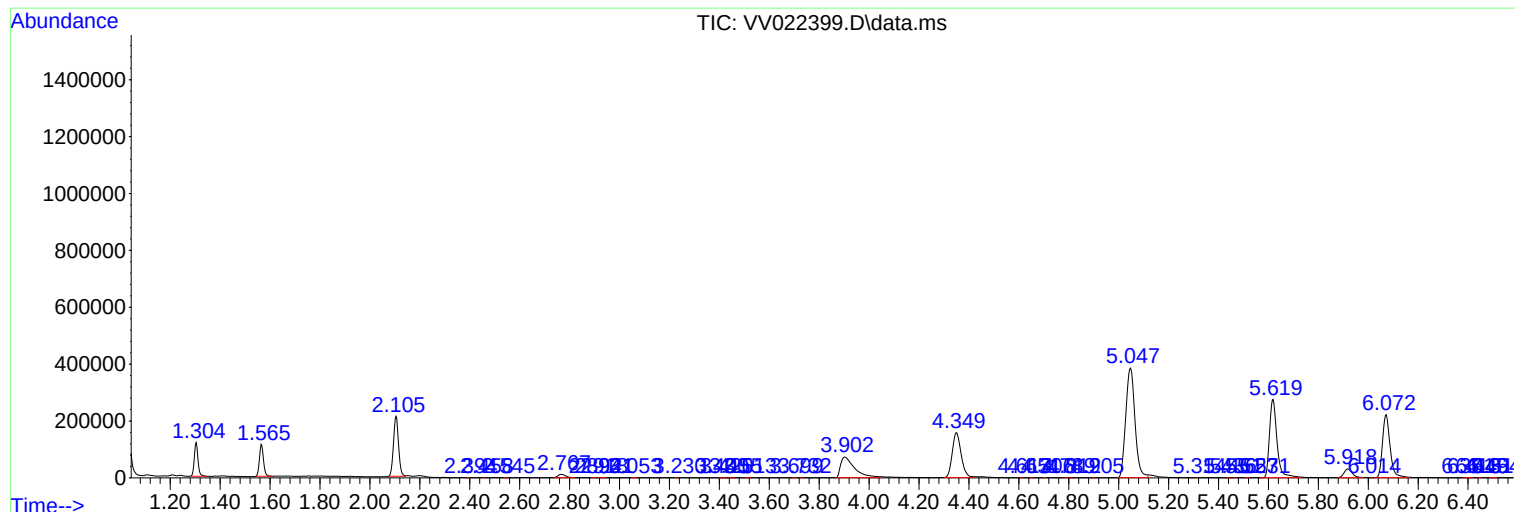

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022399.D
Acq On : 30 Sep 2021 00:08
Operator : SY/MD
Sample : M3979-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022399.D
Acq On : 30 Sep 2021 00:08
Operator : SY/MD
Sample : M3979-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------