

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022400.D
 Acq On : 30 Sep 2021 00:32
 Operator : SY/MD
 Sample : M3979-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	123751	123911	4.49%	1.197%
2	1.564	157	163	177	rVB	108537	124984	4.53%	1.207%
3	2.105	322	331	371	rVB	220750	337210	12.23%	3.258%
4	2.343	403	405	409	rBV2	489	371	0.01%	0.004%
5	2.429	430	432	436	rBV3	485	368	0.01%	0.004%
6	2.506	453	456	458	rVB2	814	491	0.02%	0.005%
7	2.564	472	474	477	rBV2	491	235	0.01%	0.002%
8	2.613	482	489	493	rBV6	1511	1917	0.07%	0.019%
9	2.690	507	513	516	rBV3	400	411	0.01%	0.004%
10	2.715	519	521	524	rBV	369	199	0.01%	0.002%
11	2.770	528	538	552	rVV2	9016	19200	0.70%	0.185%
12	2.873	568	570	572	rBV2	407	200	0.01%	0.002%
13	2.912	577	582	584	rVB	524	392	0.01%	0.004%
14	2.928	584	587	589	rBV	340	237	0.01%	0.002%
15	3.156	655	658	663	rBV2	245	297	0.01%	0.003%
16	3.243	681	685	688	rBV2	307	244	0.01%	0.002%
17	3.339	711	715	717	rBV2	249	200	0.01%	0.002%
18	3.365	722	723	726	rVB	685	234	0.01%	0.002%
19	3.387	726	730	733	rBV	294	222	0.01%	0.002%
20	3.423	737	741	744	rBV	383	299	0.01%	0.003%
21	3.625	802	804	811	rBV2	299	324	0.01%	0.003%
22	3.799	854	858	862	rBV2	277	190	0.01%	0.002%
23	3.844	866	872	876	rVB2	218	235	0.01%	0.002%
24	3.902	876	890	940	rBV2	76518	299929	10.88%	2.897%
25	4.349	1014	1029	1060	rBV	159944	396079	14.36%	3.826%
26	4.786	1161	1165	1168	rVB2	404	232	0.01%	0.002%
27	4.828	1176	1178	1180	rBV2	305	194	0.01%	0.002%
28	4.860	1185	1188	1191	rBB2	339	202	0.01%	0.002%
29	4.963	1216	1220	1223	rVB2	372	319	0.01%	0.003%
30	5.047	1229	1246	1270	rBV2	392468	997197	36.16%	9.633%
31	5.291	1320	1322	1327	rVB3	959	519	0.02%	0.005%
32	5.371	1344	1347	1355	rBV4	549	600	0.02%	0.006%
33	5.410	1355	1359	1364	rBV3	437	551	0.02%	0.005%
34	5.619	1411	1424	1462	rBV	276399	573706	20.80%	5.542%
35	5.918	1505	1517	1537	rBV5	31673	72898	2.64%	0.704%
36	6.069	1551	1564	1592	rBV	221871	464566	16.85%	4.488%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022400.D
 Acq On : 30 Sep 2021 00:32
 Operator : SY/MD
 Sample : M3979-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.249	1618	1620	1626	rVB4	1180	948	0.03%	0.009%
38	6.320	1638	1642	1644	rBV3	559	325	0.01%	0.003%
39	6.381	1659	1661	1666	rVB3	498	375	0.01%	0.004%
40	6.535	1704	1709	1710	rBV2	383	288	0.01%	0.003%
41	6.583	1717	1724	1728	rBV4	454	547	0.02%	0.005%
42	6.629	1735	1738	1739	rBV2	520	243	0.01%	0.002%
43	6.812	1793	1795	1798	rBV2	381	205	0.01%	0.002%
44	6.985	1839	1849	1873	rBV	109012	204126	7.40%	1.972%
45	7.317	1940	1952	1972	rBV	449532	785766	28.49%	7.591%
46	7.622	2036	2047	2066	rBV	75369	134115	4.86%	1.296%
47	7.873	2122	2125	2127	rVV	385	223	0.01%	0.002%
48	7.976	2143	2157	2179	rBV	1637535	2757689	100.00%	26.641%
49	8.091	2184	2193	2231	rVB	272860	510221	18.50%	4.929%
50	8.535	2326	2331	2335	rBV4	458	525	0.02%	0.005%
51	8.554	2335	2337	2340	rBV2	452	285	0.01%	0.003%
52	8.661	2367	2370	2373	rBV3	532	354	0.01%	0.003%
53	8.731	2390	2392	2396	rVB2	629	286	0.01%	0.003%
54	8.854	2418	2430	2451	rBV	421107	692440	25.11%	6.689%
55	9.085	2500	2502	2505	rBV3	465	222	0.01%	0.002%
56	9.143	2517	2520	2523	rBV3	901	769	0.03%	0.007%
57	9.407	2599	2602	2604	rBV2	399	181	0.01%	0.002%
58	9.452	2613	2616	2621	rVB4	307	187	0.01%	0.002%
59	9.487	2621	2627	2629	rBV3	456	360	0.01%	0.003%
60	9.561	2646	2650	2654	rVB3	273	190	0.01%	0.002%
61	9.734	2699	2704	2706	rBV3	524	425	0.02%	0.004%
62	9.792	2718	2722	2728	rBV3	251	253	0.01%	0.002%
63	9.860	2741	2743	2747	rVB	304	184	0.01%	0.002%
64	10.120	2816	2824	2826	rBV5	829	1011	0.04%	0.010%
65	10.217	2842	2854	2877	rBV	336339	522238	18.94%	5.045%
66	10.400	2907	2911	2914	rBV2	597	497	0.02%	0.005%
67	10.455	2924	2928	2934	rVB3	503	480	0.02%	0.005%
68	10.497	2938	2941	2945	rBV2	189	206	0.01%	0.002%
69	10.570	2962	2964	2967	rBV2	426	180	0.01%	0.002%
70	10.661	2988	2992	2994	rBV2	432	242	0.01%	0.002%
71	10.715	3007	3009	3014	rBV2	295	232	0.01%	0.002%
72	10.786	3026	3031	3036	rBV4	469	353	0.01%	0.003%
73	11.037	3105	3109	3113	rBV3	518	437	0.02%	0.004%
74	11.056	3113	3115	3116	rBV	479	189	0.01%	0.002%
75	11.069	3116	3119	3122	rVB	304	208	0.01%	0.002%
76	11.252	3164	3176	3196	rBV	386880	602187	21.84%	5.817%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022400.D
 Acq On : 30 Sep 2021 00:32
 Operator : SY/MD
 Sample : M3979-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.387	3213	3218	3221	rBV4	746	786	0.03%	0.008%
78	11.493	3247	3251	3256	rBV2	400	369	0.01%	0.004%
79	11.625	3281	3292	3318	rBV	445974	704692	25.55%	6.808%
80	11.824	3351	3354	3356	rBV	332	243	0.01%	0.002%
81	11.908	3375	3380	3381	rBV2	301	231	0.01%	0.002%
82	11.976	3400	3401	3406	rBV	328	278	0.01%	0.003%
83	12.204	3470	3472	3476	rBV2	337	224	0.01%	0.002%
84	12.361	3519	3521	3525	rVV	388	242	0.01%	0.002%
85	12.468	3552	3554	3559	rVB2	399	270	0.01%	0.003%
86	12.509	3562	3567	3569	rBV3	381	272	0.01%	0.003%
87	12.648	3607	3610	3613	rBV2	397	260	0.01%	0.003%
88	12.667	3613	3616	3620	rVB2	398	257	0.01%	0.002%
89	12.786	3647	3653	3655	rBV2	379	330	0.01%	0.003%
90	12.902	3685	3689	3690	rBV2	532	298	0.01%	0.003%
91	13.043	3729	3733	3736	rBV	279	271	0.01%	0.003%
92	13.201	3780	3782	3784	rBV2	335	177	0.01%	0.002%
93	13.268	3801	3803	3805	rBV	371	203	0.01%	0.002%
94	13.300	3810	3813	3818	rBV2	373	321	0.01%	0.003%
95	13.429	3850	3853	3858	rBV3	457	349	0.01%	0.003%
96	13.612	3906	3910	3912	rBV2	405	249	0.01%	0.002%
97	13.664	3922	3926	3930	rBV3	485	495	0.02%	0.005%
98	13.847	3980	3983	3985	rBV	325	198	0.01%	0.002%
99	13.937	4008	4011	4015	rBV2	346	285	0.01%	0.003%
100	14.310	4125	4127	4133	rVB2	729	560	0.02%	0.005%




Sum of corrected areas: 10351415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022400.D
Acq On : 30 Sep 2021 00:32
Operator : SY/MD
Sample : M3979-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

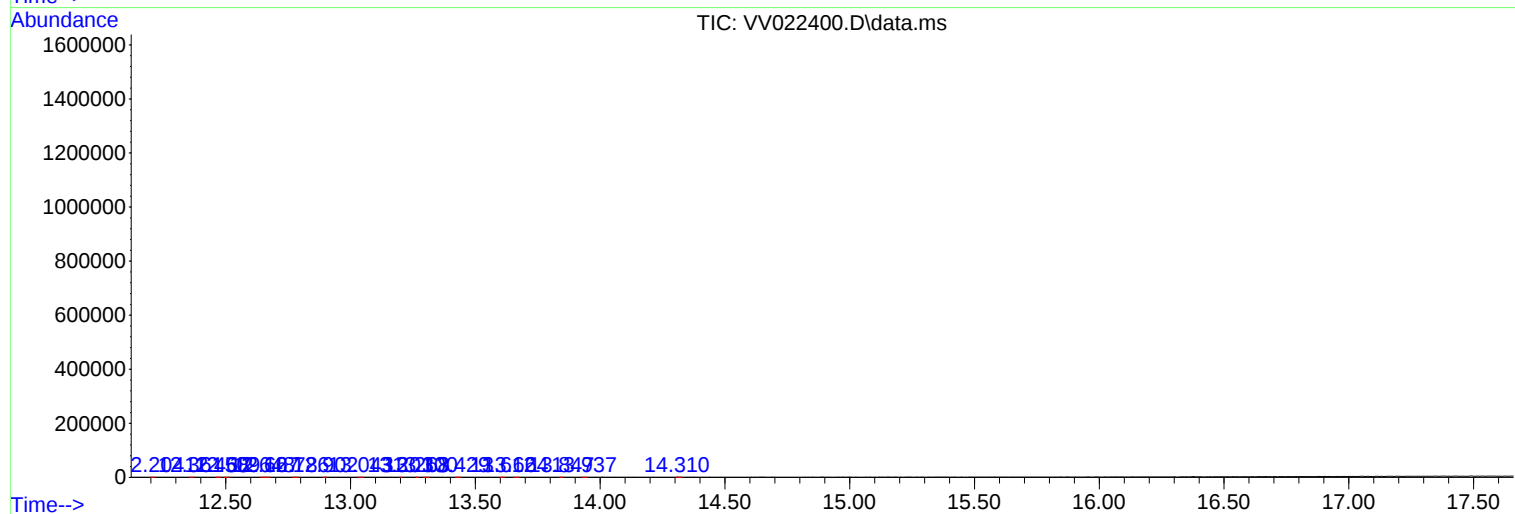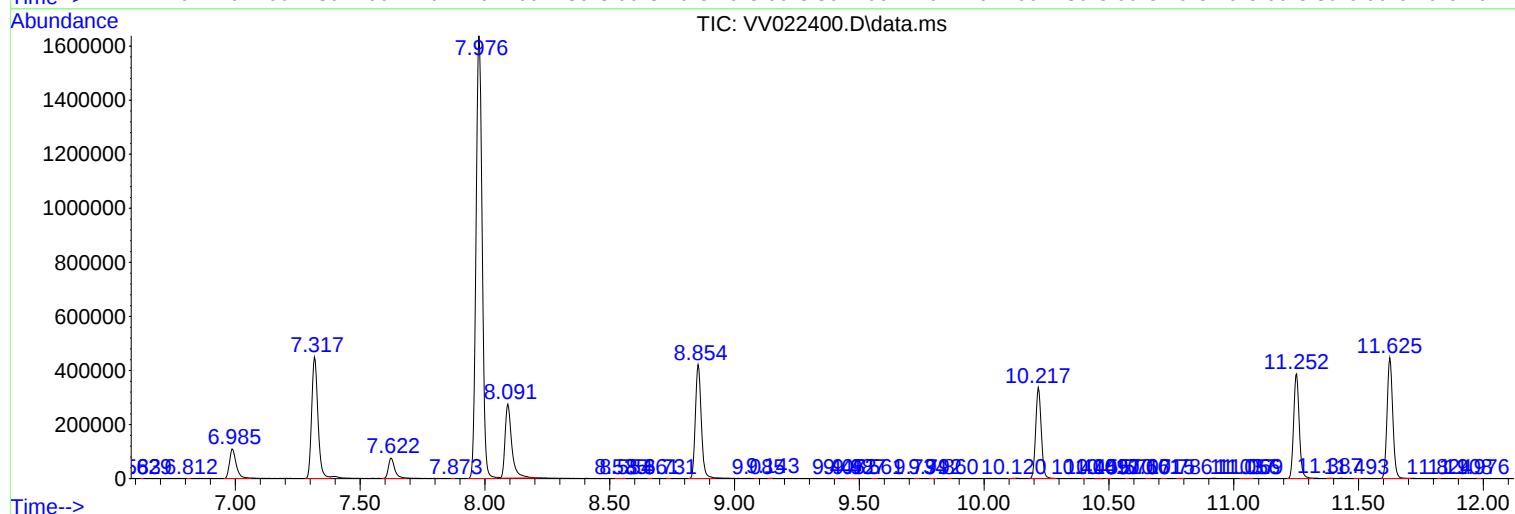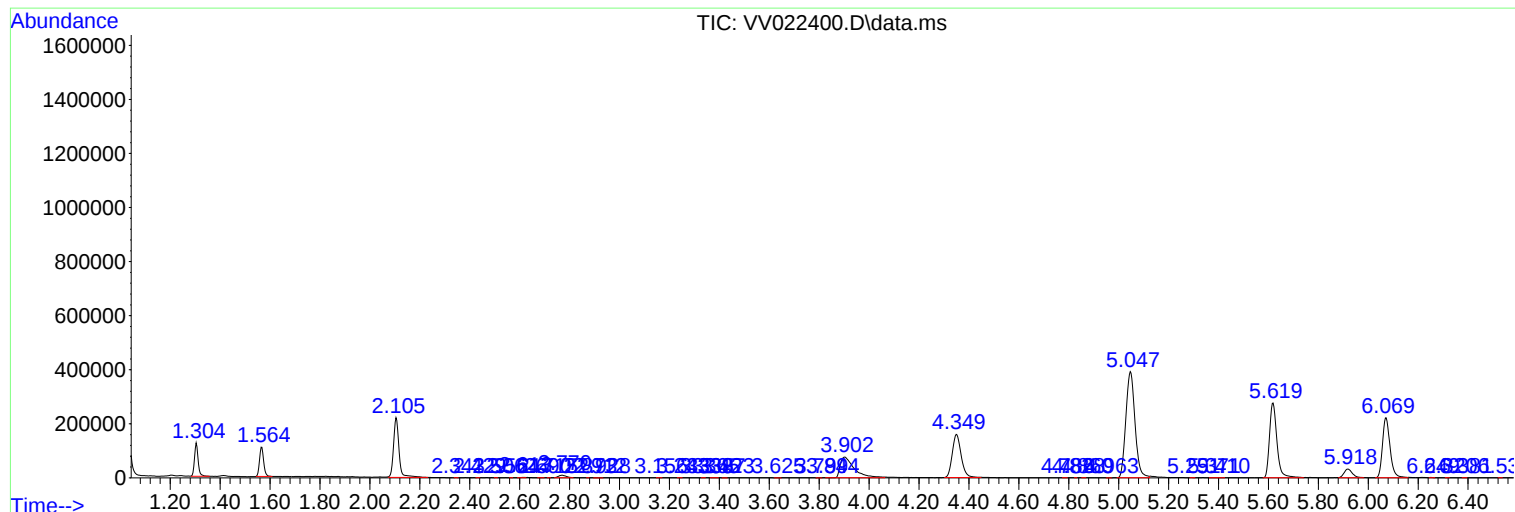

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022400.D
Acq On : 30 Sep 2021 00:32
Operator : SY/MD
Sample : M3979-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022400.D
Acq On : 30 Sep 2021 00:32
Operator : SY/MD
Sample : M3979-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
