

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022401.D
 Acq On : 30 Sep 2021 00:56
 Operator : SY/MD
 Sample : M3979-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	46	50	61	rVB2	25161	24092	2.43%	0.305%
2	1.304	76	82	94	rVB	117695	120713	12.15%	1.529%
3	1.565	157	163	173	rBV	109339	122205	12.30%	1.548%
4	2.105	322	331	343	rBV	207959	298920	30.09%	3.787%
5	2.362	408	411	414	rBV	440	354	0.04%	0.004%
6	2.757	531	534	536	rBV2	756	424	0.04%	0.005%
7	2.892	574	576	578	rBV2	378	206	0.02%	0.003%
8	2.905	578	580	585	rVV3	378	204	0.02%	0.003%
9	3.047	620	624	626	rBV2	312	190	0.02%	0.002%
10	3.063	626	629	633	rVV2	528	354	0.04%	0.004%
11	3.240	681	684	686	rBV2	331	212	0.02%	0.003%
12	3.642	805	809	810	rBV	334	178	0.02%	0.002%
13	3.699	824	827	832	rVB3	220	247	0.02%	0.003%
14	3.786	852	854	859	rVB	226	183	0.02%	0.002%
15	3.822	863	865	873	rVB3	260	229	0.02%	0.003%
16	3.902	878	890	935	rBV2	70141	258103	25.98%	3.270%
17	4.349	1015	1029	1052	rBV	154808	383124	38.56%	4.854%
18	4.863	1181	1189	1191	rBV3	383	410	0.04%	0.005%
19	4.880	1191	1194	1198	rBV3	304	234	0.02%	0.003%
20	4.941	1210	1213	1216	rVB	320	187	0.02%	0.002%
21	5.047	1230	1246	1271	rBV2	390959	993465	100.00%	12.587%
22	5.330	1331	1334	1336	rBV2	411	269	0.03%	0.003%
23	5.404	1354	1357	1361	rBV	330	261	0.03%	0.003%
24	5.423	1361	1363	1368	rVB2	495	246	0.02%	0.003%
25	5.481	1377	1381	1382	rBV	268	171	0.02%	0.002%
26	5.539	1396	1399	1401	rVB	302	175	0.02%	0.002%
27	5.619	1411	1424	1456	rBV	275167	573885	57.77%	7.271%
28	5.918	1504	1517	1538	rBV6	18045	43401	4.37%	0.550%
29	6.011	1543	1546	1547	rBV	483	200	0.02%	0.003%
30	6.072	1549	1565	1595	rBV	222673	465105	46.82%	5.893%
31	6.265	1623	1625	1628	rBV	493	260	0.03%	0.003%
32	6.404	1664	1668	1670	rBV	359	226	0.02%	0.003%
33	6.439	1677	1679	1683	rVB2	424	216	0.02%	0.003%
34	6.461	1684	1686	1690	rVV2	314	170	0.02%	0.002%
35	6.490	1690	1695	1698	rVV3	429	316	0.03%	0.004%
36	6.606	1729	1731	1734	rVB2	404	187	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022401.D
 Acq On : 30 Sep 2021 00:56
 Operator : SY/MD
 Sample : M3979-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.760	1775	1779	1781	rBV3	192	188	0.02%	0.002%
38	6.870	1810	1813	1819	rVB3	349	274	0.03%	0.003%
39	6.899	1819	1822	1825	rBV2	406	267	0.03%	0.003%
40	6.934	1827	1833	1837	rVB3	549	353	0.04%	0.004%

41	6.989	1837	1850	1873	rBV	108732	204011	20.54%	2.585%
42	7.188	1909	1912	1914	rVV2	476	276	0.03%	0.003%
43	7.317	1939	1952	1972	rBV	439460	785260	79.04%	9.949%
44	7.571	2029	2031	2033	rBV	581	186	0.02%	0.002%
45	7.622	2038	2047	2069	rBV	73243	133339	13.42%	1.689%

46	7.818	2106	2108	2111	rBV2	376	188	0.02%	0.002%
47	7.834	2111	2113	2115	rBV2	340	201	0.02%	0.003%
48	7.928	2140	2142	2143	rBV	445	175	0.02%	0.002%
49	7.976	2145	2157	2180	rVV	266203	455536	45.85%	5.771%
50	8.092	2183	2193	2229	rBV	267709	503456	50.68%	6.379%

51	8.394	2285	2287	2289	rBV2	318	171	0.02%	0.002%
52	8.722	2386	2389	2392	rBV	246	183	0.02%	0.002%
53	8.854	2418	2430	2455	rBV	414588	692653	69.72%	8.776%
54	9.043	2486	2489	2491	rBV2	473	287	0.03%	0.004%
55	9.069	2494	2497	2499	rBV3	341	228	0.02%	0.003%

56	9.104	2505	2508	2511	rBV3	491	392	0.04%	0.005%
57	9.465	2617	2620	2624	rBV3	293	249	0.03%	0.003%
58	9.500	2627	2631	2635	rBV3	461	416	0.04%	0.005%
59	9.561	2647	2650	2652	rVB2	482	242	0.02%	0.003%
60	9.616	2664	2667	2669	rBV2	414	219	0.02%	0.003%

61	9.629	2669	2671	2677	rVB2	536	323	0.03%	0.004%
62	9.664	2677	2682	2683	rBV2	391	240	0.02%	0.003%
63	9.715	2696	2698	2701	rVB2	326	213	0.02%	0.003%
64	9.805	2723	2726	2729	rBV2	385	238	0.02%	0.003%
65	9.838	2732	2736	2739	rBV2	356	282	0.03%	0.004%

66	10.021	2792	2793	2798	rVB	342	176	0.02%	0.002%
67	10.050	2798	2802	2804	rBV3	296	205	0.02%	0.003%
68	10.127	2822	2826	2831	rVB2	1093	943	0.09%	0.012%
69	10.217	2842	2854	2879	rBV	325739	517534	52.09%	6.557%
70	10.352	2893	2896	2900	rVB3	529	324	0.03%	0.004%

71	10.577	2957	2966	2970	rBV5	614	839	0.08%	0.011%
72	10.767	3023	3025	3030	rBV3	361	288	0.03%	0.004%
73	10.786	3030	3031	3035	rVB2	444	196	0.02%	0.002%
74	10.918	3064	3072	3079	rBV5	1060	1623	0.16%	0.021%
75	11.024	3101	3105	3107	rBV2	364	252	0.03%	0.003%

76	11.082	3118	3123	3127	rVB3	345	208	0.02%	0.003%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022401.D
 Acq On : 30 Sep 2021 00:56
 Operator : SY/MD
 Sample : M3979-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.140	3139	3141	3144	rBV2	292	186	0.02%	0.002%
78	11.252	3164	3176	3202	rBV	375621	594532	59.84%	7.532%
79	11.387	3216	3218	3219	rBV2	581	327	0.03%	0.004%
80	11.487	3246	3249	3252	rVB2	589	338	0.03%	0.004%
81	11.535	3262	3264	3267	rVV3	317	200	0.02%	0.003%
82	11.625	3279	3292	3318	rBV	441706	701036	70.56%	8.882%
83	11.854	3361	3363	3366	rBV2	298	199	0.02%	0.003%
84	12.005	3406	3410	3411	rBV2	358	213	0.02%	0.003%
85	12.169	3457	3461	3465	rBV3	493	425	0.04%	0.005%
86	12.355	3517	3519	3523	rVB	256	162	0.02%	0.002%
87	12.423	3536	3540	3544	rBV3	277	284	0.03%	0.004%
88	12.628	3601	3604	3608	rVB	223	172	0.02%	0.002%
89	12.648	3608	3610	3612	rBV	317	198	0.02%	0.003%
90	12.754	3641	3643	3647	rBV2	323	194	0.02%	0.002%
91	12.889	3682	3685	3688	rVB	392	253	0.03%	0.003%
92	12.963	3704	3708	3712	rBV2	295	272	0.03%	0.003%
93	13.532	3882	3885	3892	rBV2	374	452	0.05%	0.006%
94	13.744	3950	3951	3954	rBV3	383	206	0.02%	0.003%
95	13.802	3965	3969	3971	rBV3	347	232	0.02%	0.003%
96	14.114	4063	4066	4068	rBV3	385	236	0.02%	0.003%
97	14.127	4068	4070	4075	rVV2	365	284	0.03%	0.004%
98	14.201	4090	4093	4097	rBV2	450	266	0.03%	0.003%
99	14.220	4097	4099	4101	rBV2	343	174	0.02%	0.002%
100	14.805	4279	4281	4284	rBV	361	180	0.02%	0.002%




Sum of corrected areas: 7892977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022401.D
Acq On : 30 Sep 2021 00:56
Operator : SY/MD
Sample : M3979-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

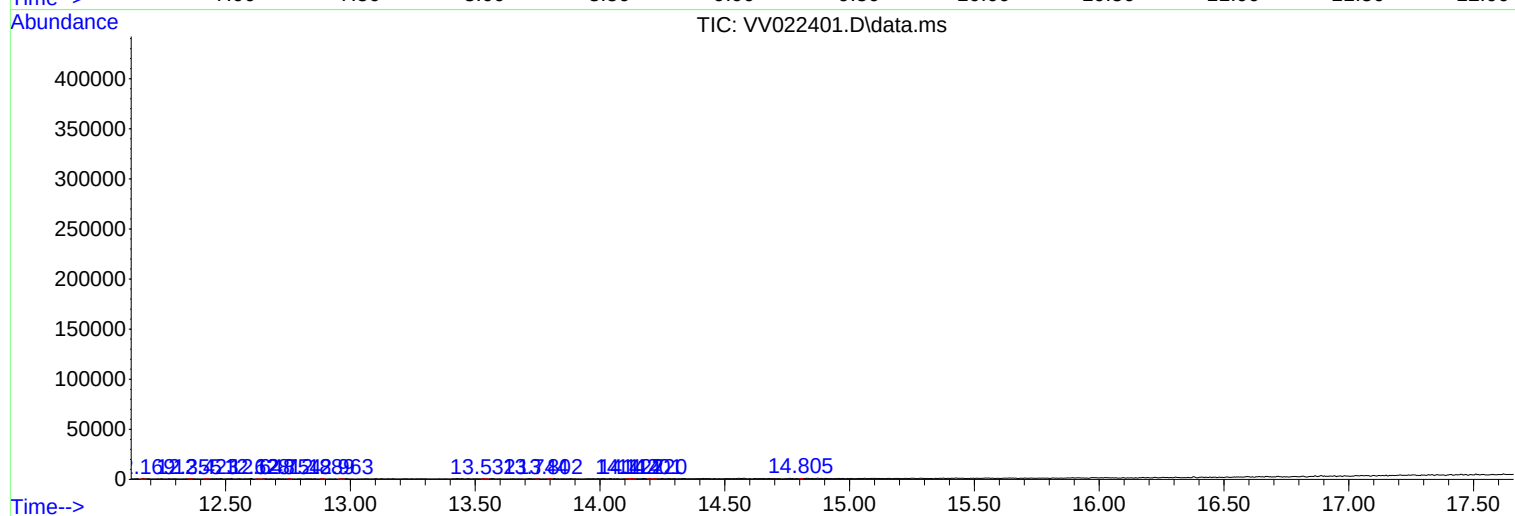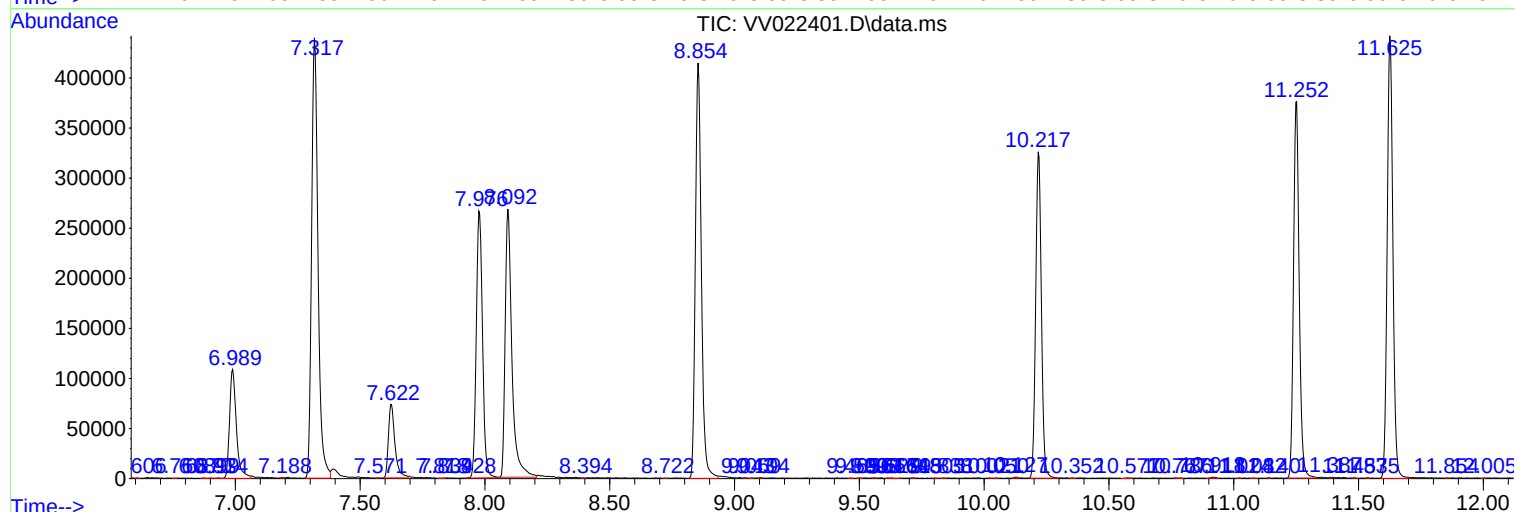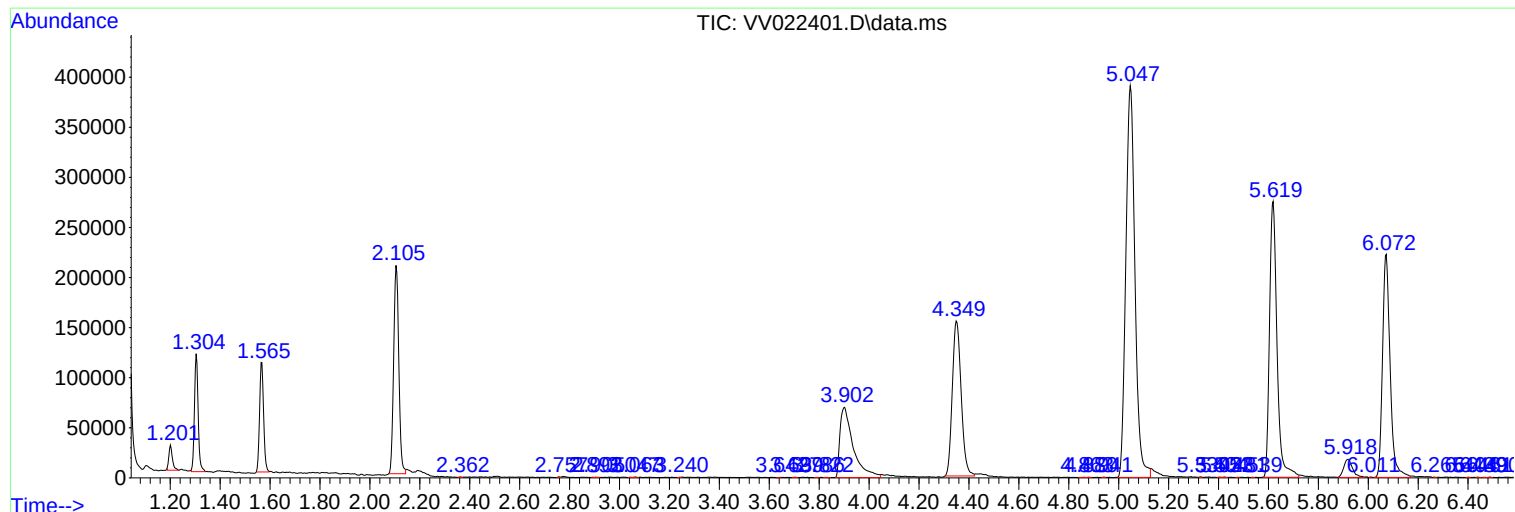

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022401.D
Acq On : 30 Sep 2021 00:56
Operator : SY/MD
Sample : M3979-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022401.D
Acq On : 30 Sep 2021 00:56
Operator : SY/MD
Sample : M3979-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
