

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022404.D
 Acq On : 30 Sep 2021 02:08
 Operator : SY/MD
 Sample : M3979-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	117197	117496	9.28%	1.374%
2	1.564	157	163	173	rVB	108597	119642	9.45%	1.399%
3	2.105	321	331	349	rBV	202982	297493	23.49%	3.478%
4	2.346	404	406	411	rVB3	612	263	0.02%	0.003%
5	2.555	466	471	473	rBV2	475	389	0.03%	0.005%
6	2.590	479	482	486	rBV5	483	368	0.03%	0.004%
7	2.609	486	488	490	rBV5	465	274	0.02%	0.003%
8	2.773	526	539	556	rBV4	5906	13649	1.08%	0.160%
9	2.918	582	584	588	rVB3	416	182	0.01%	0.002%
10	3.079	632	634	636	rBV2	363	213	0.02%	0.002%
11	3.098	638	640	644	rVB2	251	153	0.01%	0.002%
12	3.195	668	670	675	rVB2	353	151	0.01%	0.002%
13	3.355	717	720	723	rBV2	227	161	0.01%	0.002%
14	3.400	731	734	739	rVB3	231	172	0.01%	0.002%
15	3.767	844	848	852	rBV2	316	246	0.02%	0.003%
16	3.822	864	865	870	rVB2	302	212	0.02%	0.002%
17	3.850	870	874	875	rBV2	345	148	0.01%	0.002%
18	3.902	878	890	935	rBV	71010	267335	21.11%	3.125%
19	4.349	1013	1029	1050	rBV2	154653	385189	30.42%	4.503%
20	4.703	1136	1139	1142	rBV2	353	236	0.02%	0.003%
21	4.751	1152	1154	1156	rBV2	275	140	0.01%	0.002%
22	4.786	1163	1165	1171	rVB2	447	240	0.02%	0.003%
23	4.821	1171	1176	1177	rBV	311	269	0.02%	0.003%
24	4.876	1191	1193	1195	rBV	359	176	0.01%	0.002%
25	5.047	1229	1246	1286	rBV2	381593	993045	78.41%	11.609%
26	5.336	1334	1336	1339	rBV3	242	173	0.01%	0.002%
27	5.410	1356	1359	1362	rVB3	573	354	0.03%	0.004%
28	5.429	1364	1365	1369	rVB2	449	183	0.01%	0.002%
29	5.448	1369	1371	1377	rBV2	568	435	0.03%	0.005%
30	5.474	1377	1379	1382	rBV	337	225	0.02%	0.003%
31	5.558	1401	1405	1407	rBV	321	230	0.02%	0.003%
32	5.619	1412	1424	1465	rVV	261607	551690	43.56%	6.449%
33	6.072	1552	1565	1594	rBV	214511	451757	35.67%	5.281%
34	6.249	1618	1620	1622	rBV	490	318	0.03%	0.004%
35	6.400	1665	1667	1670	rVB2	296	143	0.01%	0.002%
36	6.426	1670	1675	1679	rBV2	294	293	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022404.D
 Acq On : 30 Sep 2021 02:08
 Operator : SY/MD
 Sample : M3979-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.522	1695	1705	1711	rBV5	1049	1929	0.15%	0.023%
38	6.651	1741	1745	1748	rBV3	685	488	0.04%	0.006%
39	6.690	1755	1757	1759	rVB2	417	174	0.01%	0.002%
40	6.783	1784	1786	1789	rVB2	306	152	0.01%	0.002%
41	6.911	1824	1826	1830	rBV	608	318	0.03%	0.004%
42	6.989	1839	1850	1876	rBV	104393	199042	15.72%	2.327%
43	7.182	1908	1910	1912	rBV2	249	134	0.01%	0.002%
44	7.252	1930	1932	1936	rVB2	380	197	0.02%	0.002%
45	7.317	1940	1952	1971	rBV	430665	767696	60.62%	8.975%
46	7.622	2037	2047	2066	rBV	72136	131698	10.40%	1.540%
47	7.789	2095	2099	2100	rBV2	490	336	0.03%	0.004%
48	7.825	2108	2110	2114	rVB3	457	296	0.02%	0.003%
49	7.844	2114	2116	2120	rBV	376	241	0.02%	0.003%
50	7.889	2126	2130	2134	rVB4	372	258	0.02%	0.003%
51	7.976	2144	2157	2183	rBV	741557	1266415	100.00%	14.805%
52	8.091	2184	2193	2227	rVV	274767	511146	40.36%	5.975%
53	8.390	2284	2286	2289	rBV3	509	281	0.02%	0.003%
54	8.477	2310	2313	2319	rBV5	479	606	0.05%	0.007%
55	8.551	2334	2336	2339	rBV2	424	197	0.02%	0.002%
56	8.619	2354	2357	2361	rBV3	349	257	0.02%	0.003%
57	8.667	2370	2372	2375	rVB	405	216	0.02%	0.003%
58	8.686	2375	2378	2384	rBV3	374	365	0.03%	0.004%
59	8.728	2389	2391	2392	rBV2	312	145	0.01%	0.002%
60	8.773	2401	2405	2408	rVB2	405	264	0.02%	0.003%
61	8.789	2408	2410	2413	rBV2	371	227	0.02%	0.003%
62	8.853	2416	2430	2454	rBV	409106	668685	52.80%	7.817%
63	9.098	2503	2506	2507	rBV2	348	213	0.02%	0.002%
64	9.246	2551	2552	2555	rVB2	454	163	0.01%	0.002%
65	9.268	2555	2559	2561	rBV	505	287	0.02%	0.003%
66	9.452	2613	2616	2619	rBV	329	241	0.02%	0.003%
67	9.677	2683	2686	2687	rBV2	279	168	0.01%	0.002%
68	9.712	2694	2697	2700	rBV2	257	240	0.02%	0.003%
69	9.879	2748	2749	2752	rBV	238	155	0.01%	0.002%
70	10.030	2793	2796	2798	rBV2	224	136	0.01%	0.002%
71	10.107	2816	2820	2821	rBV	311	200	0.02%	0.002%
72	10.124	2821	2825	2833	rVB3	844	1024	0.08%	0.012%
73	10.217	2843	2854	2873	rBV	324875	515003	40.67%	6.021%
74	10.361	2895	2899	2902	rBV2	515	242	0.02%	0.003%
75	10.378	2902	2904	2906	rVV2	334	171	0.01%	0.002%
76	10.390	2906	2908	2909	rVV2	439	163	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022404.D
 Acq On : 30 Sep 2021 02:08
 Operator : SY/MD
 Sample : M3979-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.413	2912	2915	2920	rVB2	397	259	0.02%	0.003%
78	10.455	2925	2928	2932	rVB3	470	283	0.02%	0.003%
79	10.480	2932	2936	2941	rVB	547	385	0.03%	0.005%
80	10.599	2970	2973	2975	rBV	168	141	0.01%	0.002%
81	10.914	3065	3071	3073	rBV4	900	828	0.07%	0.010%
82	11.008	3098	3100	3105	rVB2	309	232	0.02%	0.003%
83	11.072	3117	3120	3127	rVB2	265	168	0.01%	0.002%
84	11.207	3159	3162	3164	rVB2	317	204	0.02%	0.002%
85	11.252	3164	3176	3200	rBV	356835	577549	45.61%	6.752%
86	11.625	3279	3292	3311	rBV	440653	696711	55.01%	8.145%
87	11.908	3377	3380	3382	rBV3	260	177	0.01%	0.002%
88	11.950	3389	3393	3397	rBV3	551	506	0.04%	0.006%
89	12.278	3493	3495	3498	rBV2	334	143	0.01%	0.002%
90	12.358	3516	3520	3526	rVB3	688	761	0.06%	0.009%
91	12.474	3553	3556	3558	rBV	255	169	0.01%	0.002%
92	12.631	3603	3605	3609	rVB	271	159	0.01%	0.002%
93	12.776	3647	3650	3652	rBV2	265	164	0.01%	0.002%
94	12.818	3661	3663	3668	rBV	257	210	0.02%	0.002%
95	13.303	3812	3814	3817	rBV	224	141	0.01%	0.002%
96	13.355	3828	3830	3832	rBV	481	200	0.02%	0.002%
97	14.220	4097	4099	4101	rBV2	433	212	0.02%	0.002%
98	14.381	4147	4149	4156	rVB3	520	336	0.03%	0.004%
99	14.413	4156	4159	4160	rBV2	301	179	0.01%	0.002%
100	14.651	4231	4233	4236	rBV2	342	172	0.01%	0.002%




Sum of corrected areas: 8554101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022404.D
Acq On : 30 Sep 2021 02:08
Operator : SY/MD
Sample : M3979-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

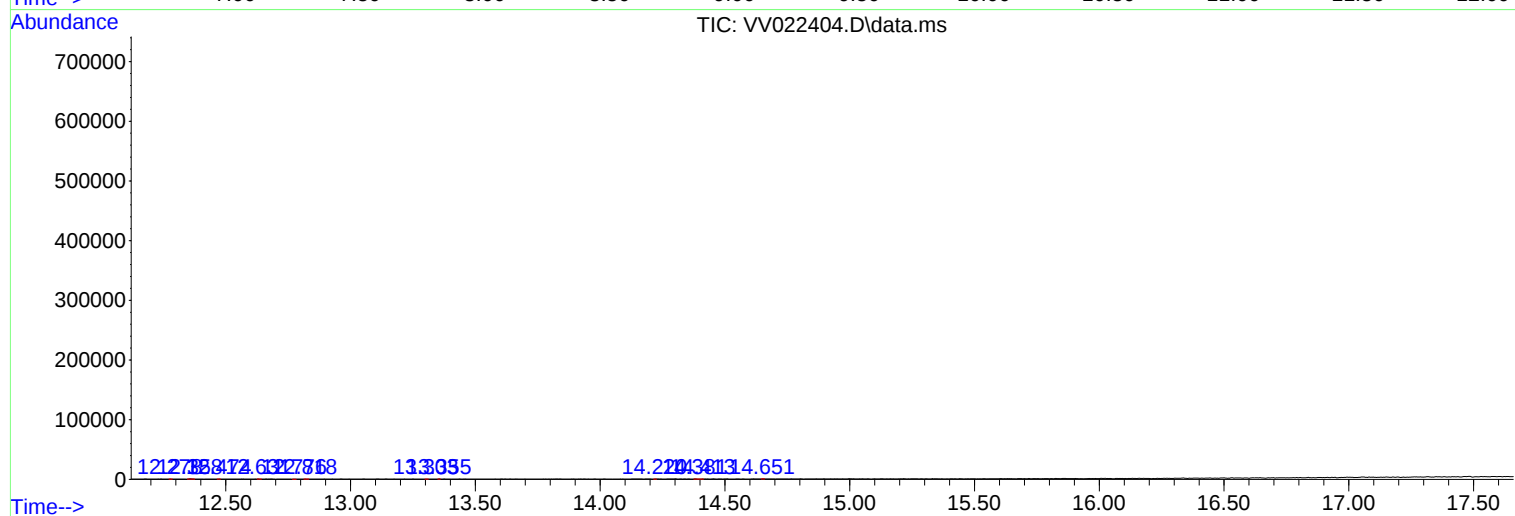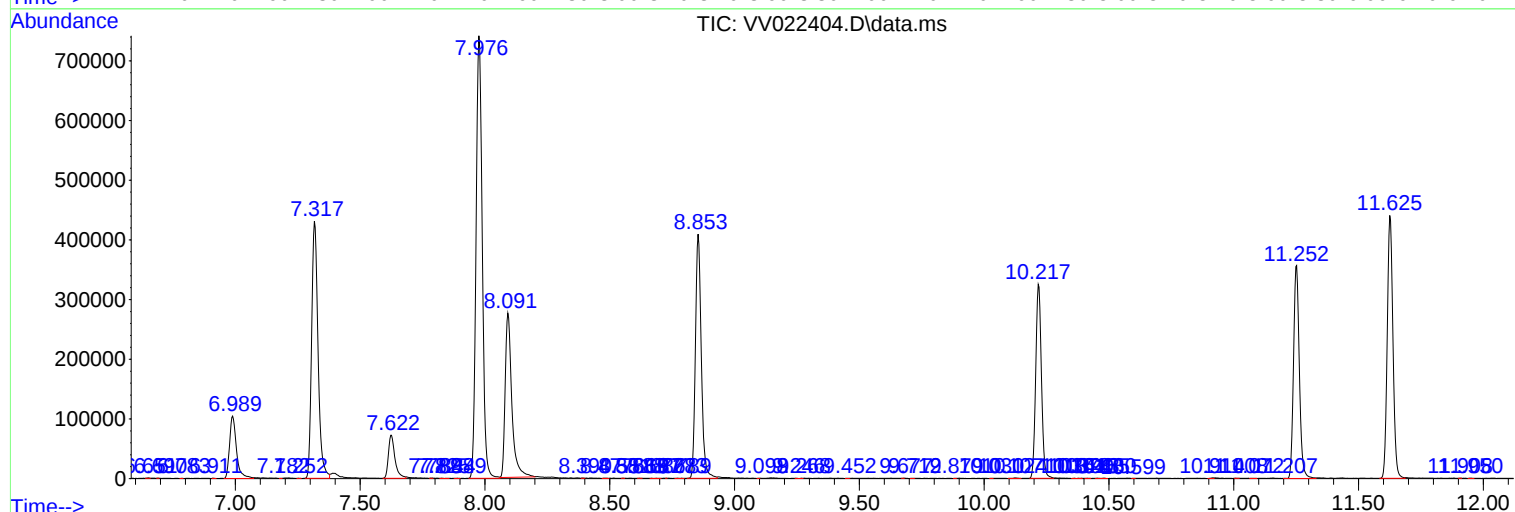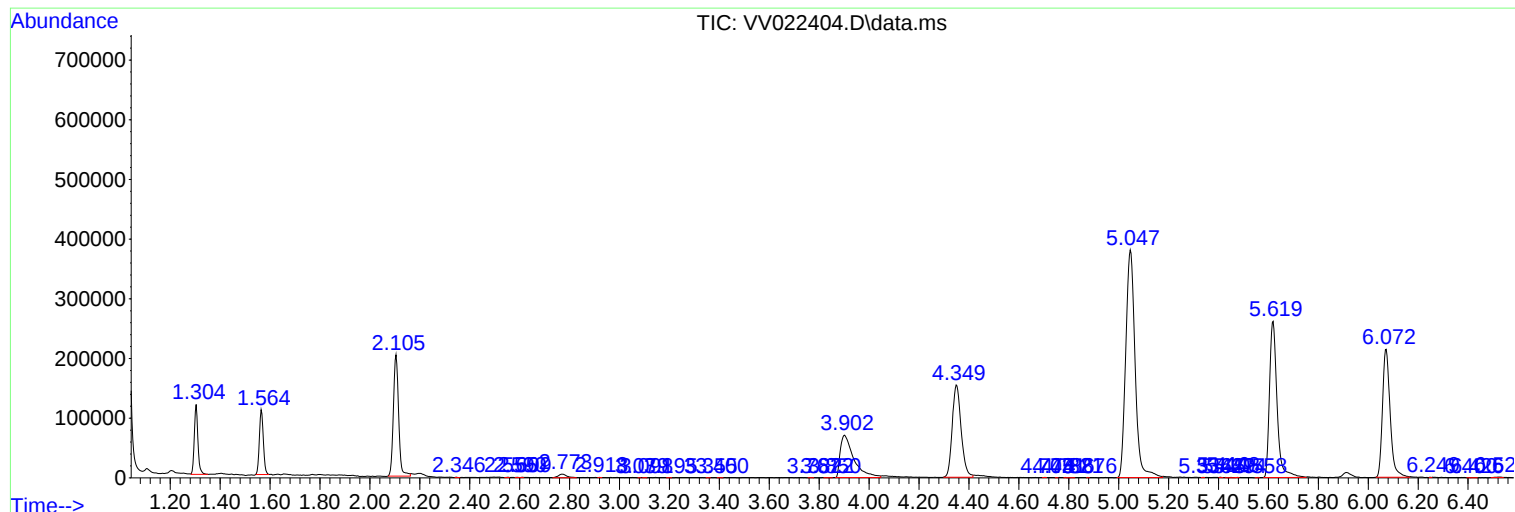

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022404.D
Acq On : 30 Sep 2021 02:08
Operator : SY/MD
Sample : M3979-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022404.D
Acq On : 30 Sep 2021 02:08
Operator : SY/MD
Sample : M3979-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
