

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022405.D
 Acq On : 30 Sep 2021 02:32
 Operator : SY/MD
 Sample : M3979-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	119582	117974	11.63%	1.537%
2	1.564	157	163	177	rVB	113039	125147	12.34%	1.631%
3	2.105	321	331	345	rBV	208565	303248	29.90%	3.951%
4	2.584	478	480	483	rBV2	476	273	0.03%	0.004%
5	2.770	525	538	548	rBV4	4150	8355	0.82%	0.109%
6	2.863	565	567	570	rBV2	347	201	0.02%	0.003%
7	2.879	570	572	575	rVB2	311	169	0.02%	0.002%
8	3.056	624	627	628	rBV	406	186	0.02%	0.002%
9	3.191	667	669	673	rBV	194	144	0.01%	0.002%
10	3.252	686	688	690	rBV	254	157	0.02%	0.002%
11	3.452	746	750	751	rBV	329	245	0.02%	0.003%
12	3.670	813	818	819	rBV3	338	227	0.02%	0.003%
13	3.722	832	834	838	rVB2	236	105	0.01%	0.001%
14	3.809	858	861	864	rBV2	231	142	0.01%	0.002%
15	3.902	877	890	927	rBV2	67682	262201	25.86%	3.417%
16	4.349	1014	1029	1053	rBV	157785	390000	38.46%	5.082%
17	4.744	1150	1152	1154	rBV2	267	148	0.01%	0.002%
18	4.809	1170	1172	1176	rVB2	348	171	0.02%	0.002%
19	4.828	1176	1178	1179	rBV	262	105	0.01%	0.001%
20	5.047	1229	1246	1285	rBV2	394540	1014046	100.00%	13.213%
21	5.407	1355	1358	1363	rBV2	279	303	0.03%	0.004%
22	5.497	1384	1386	1389	rVB	522	233	0.02%	0.003%
23	5.526	1393	1395	1397	rBV2	192	100	0.01%	0.001%
24	5.619	1412	1424	1456	rBV	263563	552328	54.47%	7.197%
25	5.911	1504	1515	1533	rBV7	9537	21887	2.16%	0.285%
26	6.005	1542	1544	1547	rVB	373	157	0.02%	0.002%
27	6.072	1549	1565	1596	rBV	219361	467049	46.06%	6.086%
28	6.326	1641	1644	1647	rBV3	526	311	0.03%	0.004%
29	6.387	1660	1663	1669	rVB3	340	188	0.02%	0.002%
30	6.436	1675	1678	1682	rBV4	444	287	0.03%	0.004%
31	6.481	1689	1692	1693	rBV	229	108	0.01%	0.001%
32	6.577	1720	1722	1724	rBV3	341	163	0.02%	0.002%
33	6.619	1732	1735	1736	rBV	269	167	0.02%	0.002%
34	6.728	1765	1769	1773	rBV3	440	348	0.03%	0.005%
35	6.767	1779	1781	1784	rVB	240	115	0.01%	0.001%
36	6.809	1792	1794	1797	rBV2	290	162	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022405.D
 Acq On : 30 Sep 2021 02:32
 Operator : SY/MD
 Sample : M3979-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.863	1809	1811	1812	rBV	351	115	0.01%	0.001%
38	6.902	1820	1823	1826	rVB	248	157	0.02%	0.002%
39	6.927	1826	1831	1833	rBV2	478	418	0.04%	0.005%
40	6.989	1838	1850	1881	rBV	108577	205585	20.27%	2.679%
41	7.243	1927	1929	1931	rVB	390	143	0.01%	0.002%
42	7.262	1932	1935	1937	rBV2	304	207	0.02%	0.003%
43	7.317	1941	1952	1972	rBV	439395	783302	77.25%	10.207%
44	7.625	2038	2048	2074	rBV	75293	137139	13.52%	1.787%
45	7.857	2117	2120	2125	rBV4	589	428	0.04%	0.006%
46	7.924	2138	2141	2142	rBV	314	166	0.02%	0.002%
47	7.979	2146	2158	2180	rVV	165397	282211	27.83%	3.677%
48	8.091	2184	2193	2227	rBV	273672	522420	51.52%	6.807%
49	8.439	2299	2301	2303	rBV	412	278	0.03%	0.004%
50	8.487	2313	2316	2318	rBV2	487	290	0.03%	0.004%
51	8.583	2344	2346	2349	rVB3	456	207	0.02%	0.003%
52	8.661	2367	2370	2371	rBV	621	257	0.03%	0.003%
53	8.689	2376	2379	2381	rBV	298	174	0.02%	0.002%
54	8.734	2391	2393	2396	rVB2	286	121	0.01%	0.002%
55	8.751	2396	2398	2403	rBV3	419	352	0.03%	0.005%
56	8.789	2407	2410	2413	rBV2	239	146	0.01%	0.002%
57	8.853	2419	2430	2462	rBV	399024	666173	65.69%	8.680%
58	9.072	2495	2498	2499	rBV	250	110	0.01%	0.001%
59	9.130	2514	2516	2517	rBV	297	113	0.01%	0.001%
60	9.287	2563	2565	2566	rBV2	325	107	0.01%	0.001%
61	9.445	2611	2614	2616	rBV2	326	154	0.02%	0.002%
62	9.471	2620	2622	2626	rVV3	505	454	0.04%	0.006%
63	9.503	2630	2632	2636	rBV2	200	98	0.01%	0.001%
64	9.548	2643	2646	2647	rBV2	310	144	0.01%	0.002%
65	9.773	2714	2716	2721	rBV	267	213	0.02%	0.003%
66	9.828	2729	2733	2737	rBV2	371	374	0.04%	0.005%
67	10.053	2801	2803	2805	rBV	246	123	0.01%	0.002%
68	10.130	2824	2827	2836	rVB4	943	826	0.08%	0.011%
69	10.165	2836	2838	2840	rBV	246	173	0.02%	0.002%
70	10.217	2842	2854	2872	rBV	329815	524112	51.69%	6.829%
71	10.464	2926	2931	2933	rBB4	497	308	0.03%	0.004%
72	10.480	2933	2936	2938	rVB	289	166	0.02%	0.002%
73	10.767	3023	3025	3027	rVB	253	98	0.01%	0.001%
74	10.824	3040	3043	3047	rVB2	231	151	0.01%	0.002%
75	10.863	3053	3055	3057	rBV2	310	112	0.01%	0.001%
76	10.921	3067	3073	3075	rBV4	1100	1137	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022405.D
 Acq On : 30 Sep 2021 02:32
 Operator : SY/MD
 Sample : M3979-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.252	3164	3176	3198	rBV	359641	568077	56.02%	7.402%
78	11.451	3236	3238	3245	rVB3	358	314	0.03%	0.004%
79	11.484	3245	3248	3249	rBV	281	155	0.02%	0.002%
80	11.532	3261	3263	3267	rBV3	425	265	0.03%	0.003%
81	11.625	3281	3292	3311	rBV	446456	704660	69.49%	9.182%
82	11.847	3359	3361	3364	rBV2	280	156	0.02%	0.002%
83	12.111	3437	3443	3445	rBV3	455	398	0.04%	0.005%
84	12.326	3508	3510	3513	rBV	393	203	0.02%	0.003%
85	12.500	3561	3564	3566	rBV2	338	191	0.02%	0.002%
86	12.599	3592	3595	3597	rBV	575	336	0.03%	0.004%
87	12.622	3599	3602	3606	rVB	371	259	0.03%	0.003%
88	12.882	3679	3683	3688	rVB2	793	668	0.07%	0.009%
89	12.911	3689	3692	3695	rBV2	270	204	0.02%	0.003%
90	12.937	3698	3700	3703	rVV	281	138	0.01%	0.002%
91	12.953	3703	3705	3708	rVB	256	102	0.01%	0.001%
92	13.065	3739	3740	3742	rBV	394	166	0.02%	0.002%
93	13.085	3744	3746	3749	rVB2	277	129	0.01%	0.002%
94	13.265	3799	3802	3805	rBV	421	218	0.02%	0.003%
95	13.606	3905	3908	3910	rBV	264	156	0.02%	0.002%
96	13.725	3943	3945	3946	rBV	323	120	0.01%	0.002%
97	13.856	3984	3986	3988	rVB	533	211	0.02%	0.003%
98	13.911	4002	4003	4009	rVB3	433	318	0.03%	0.004%
99	14.207	4093	4095	4099	rBV	449	261	0.03%	0.003%
100	14.358	4140	4142	4147	rBV2	411	302	0.03%	0.004%




Sum of corrected areas: 7674419

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022405.D
Acq On : 30 Sep 2021 02:32
Operator : SY/MD
Sample : M3979-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

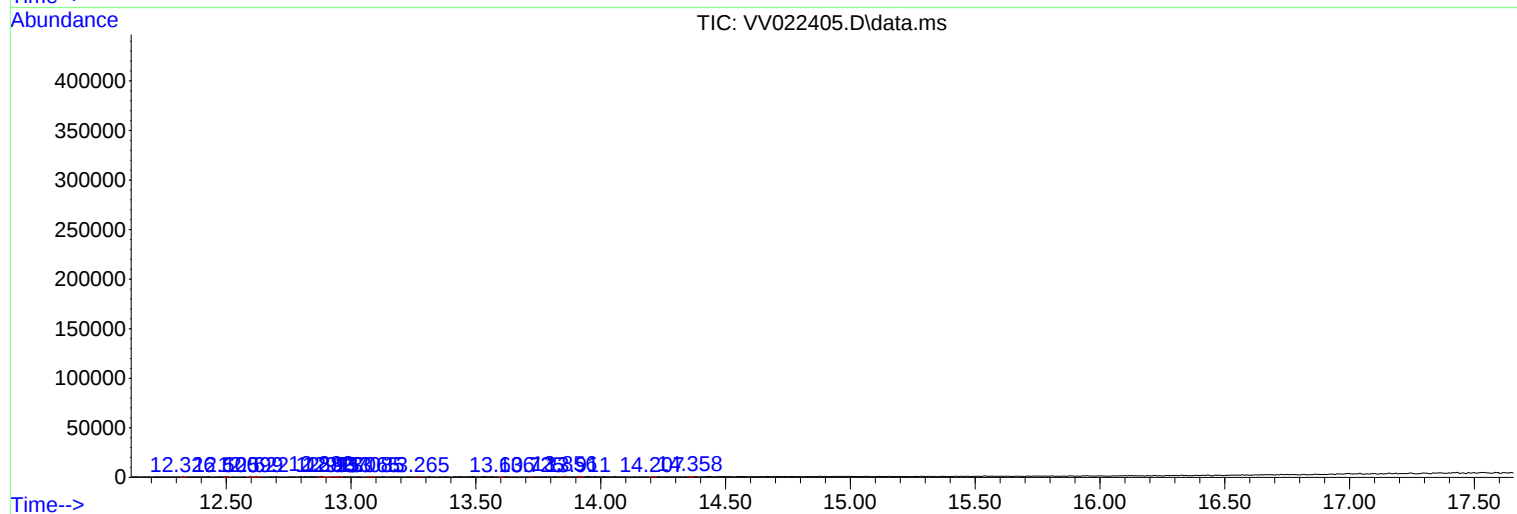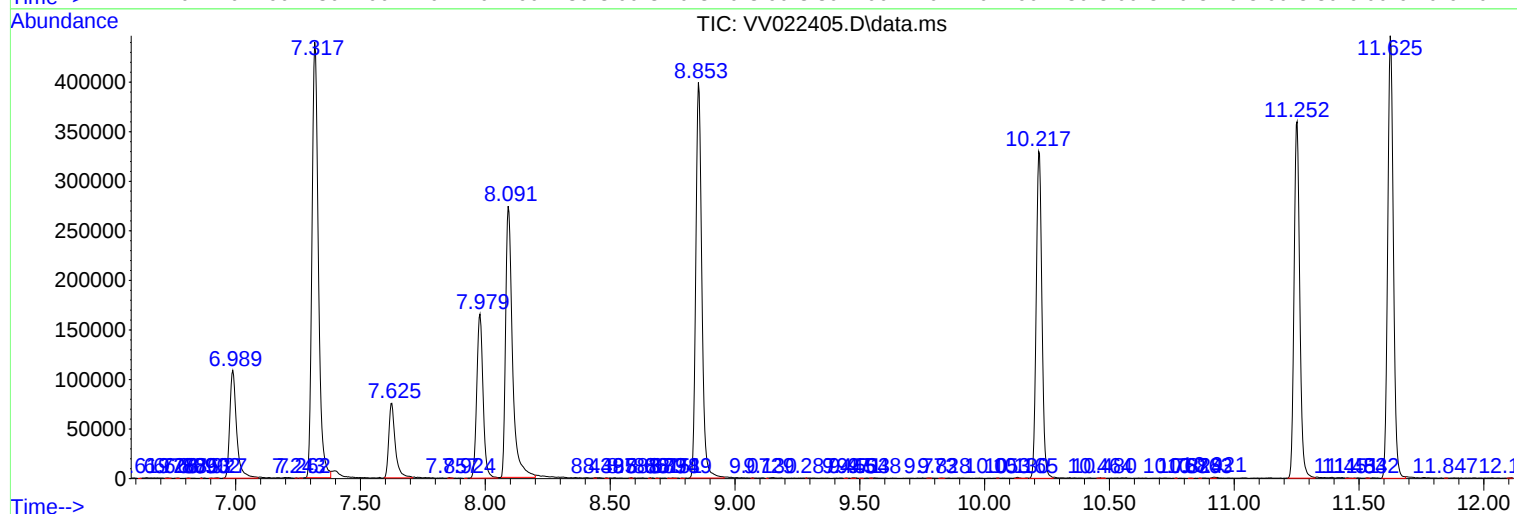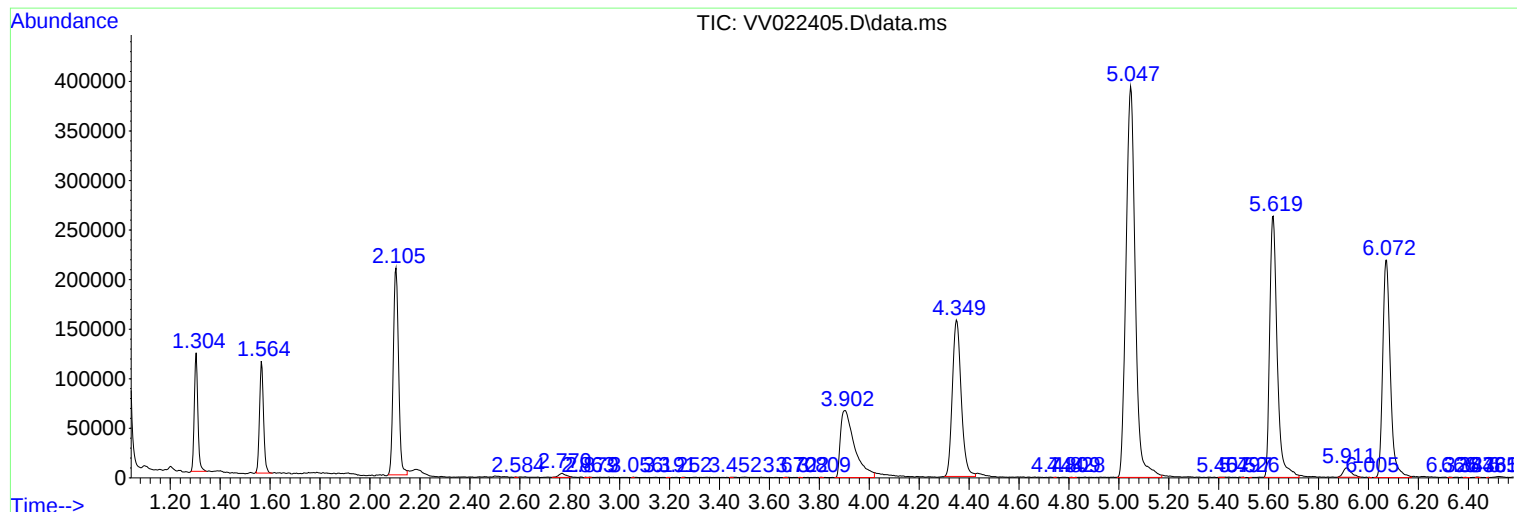

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022405.D
Acq On : 30 Sep 2021 02:32
Operator : SY/MD
Sample : M3979-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022405.D
Acq On : 30 Sep 2021 02:32
Operator : SY/MD
Sample : M3979-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------